
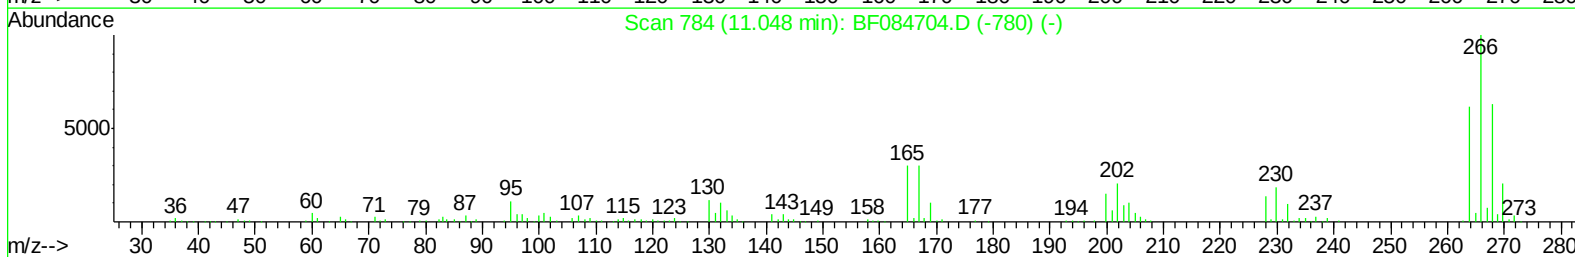
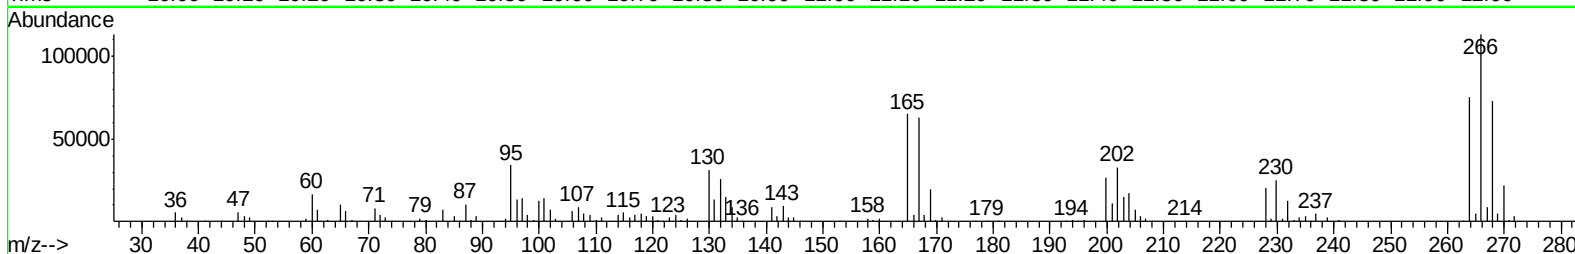


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021216\
Data File : BF085030.D
Acq On : 12 Feb 2016 00:00
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 08:23:18 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 10 13:28:51 2016
Response via : Initial Calibration

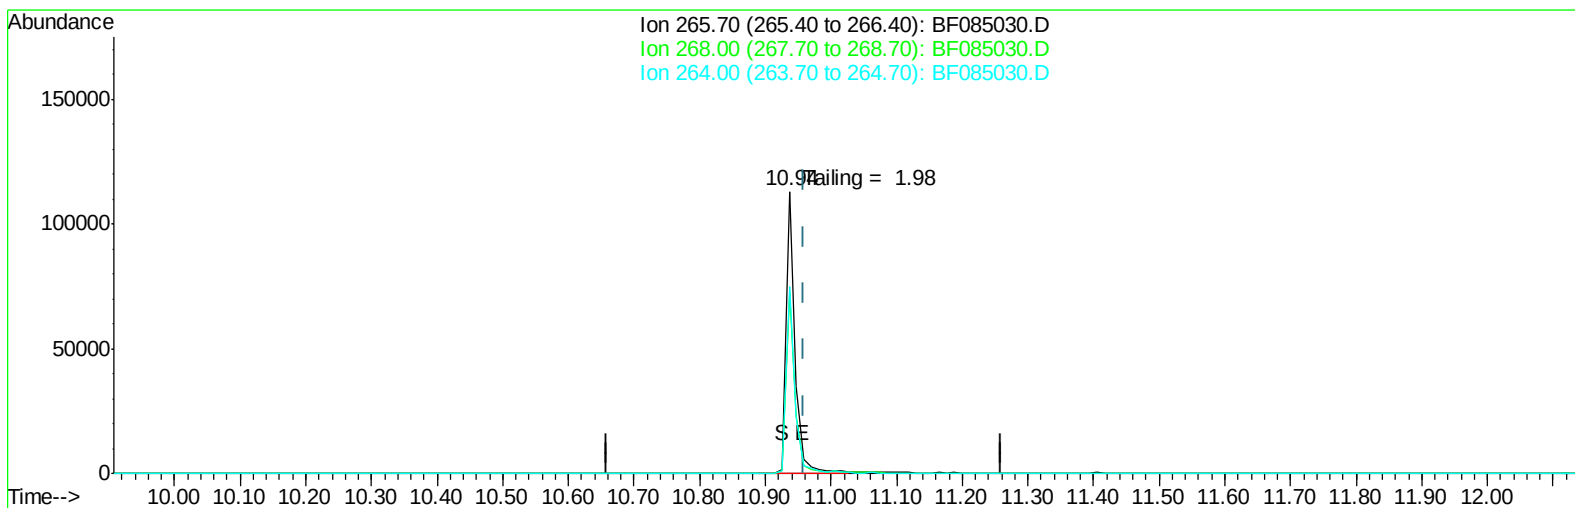

TIC: BF085030.D

(69) Pentachlorophenol (C)




10.936min (-0.023) 30329.97ng

response 113906

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	64.22
264.00	62.70	66.24
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021216\
Data File : BF085030.D
Acq On : 12 Feb 2016 00:00
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 08:23:18 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 10 13:28:51 2016
Response via : Initial Calibration

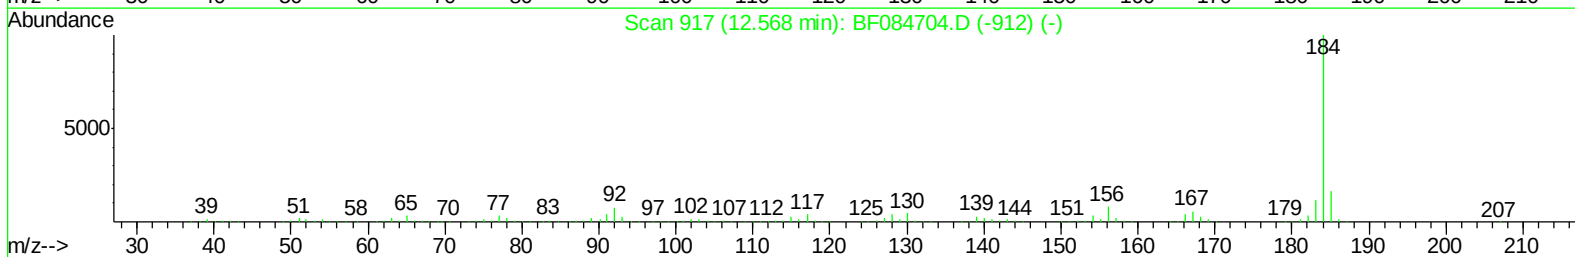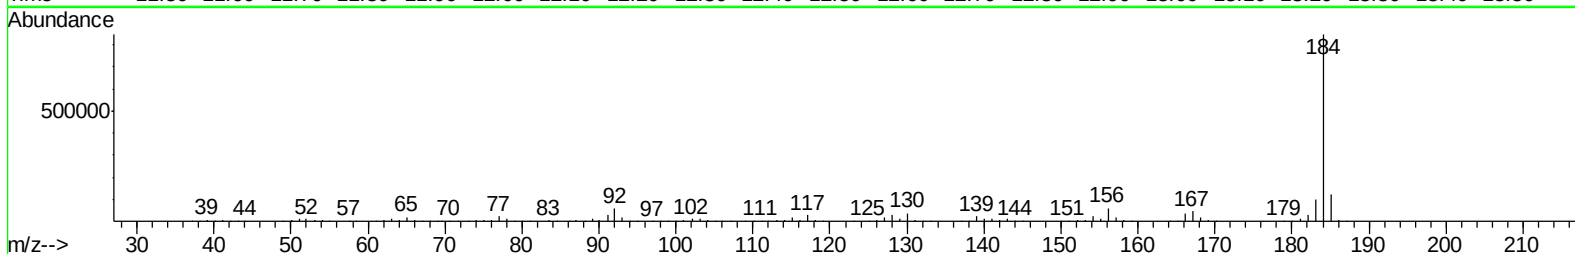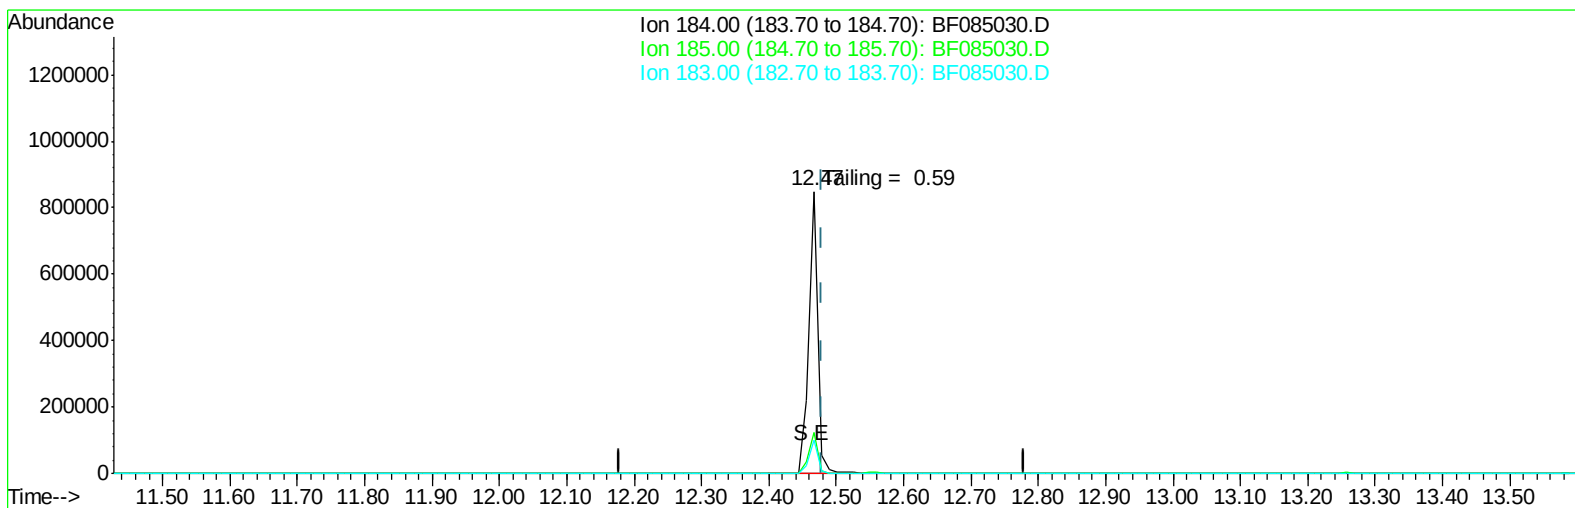

TIC: BF085030.D

(76) Benzidine

12.468min (-0.012) -20.00ng

response 790304

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.48
183.00	12.30	11.80
0.00	0.00	0.00