


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021216\
 Data File : BF085030.D
 Acq On : 12 Feb 2016 00:00
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 10 13:28:51 2016

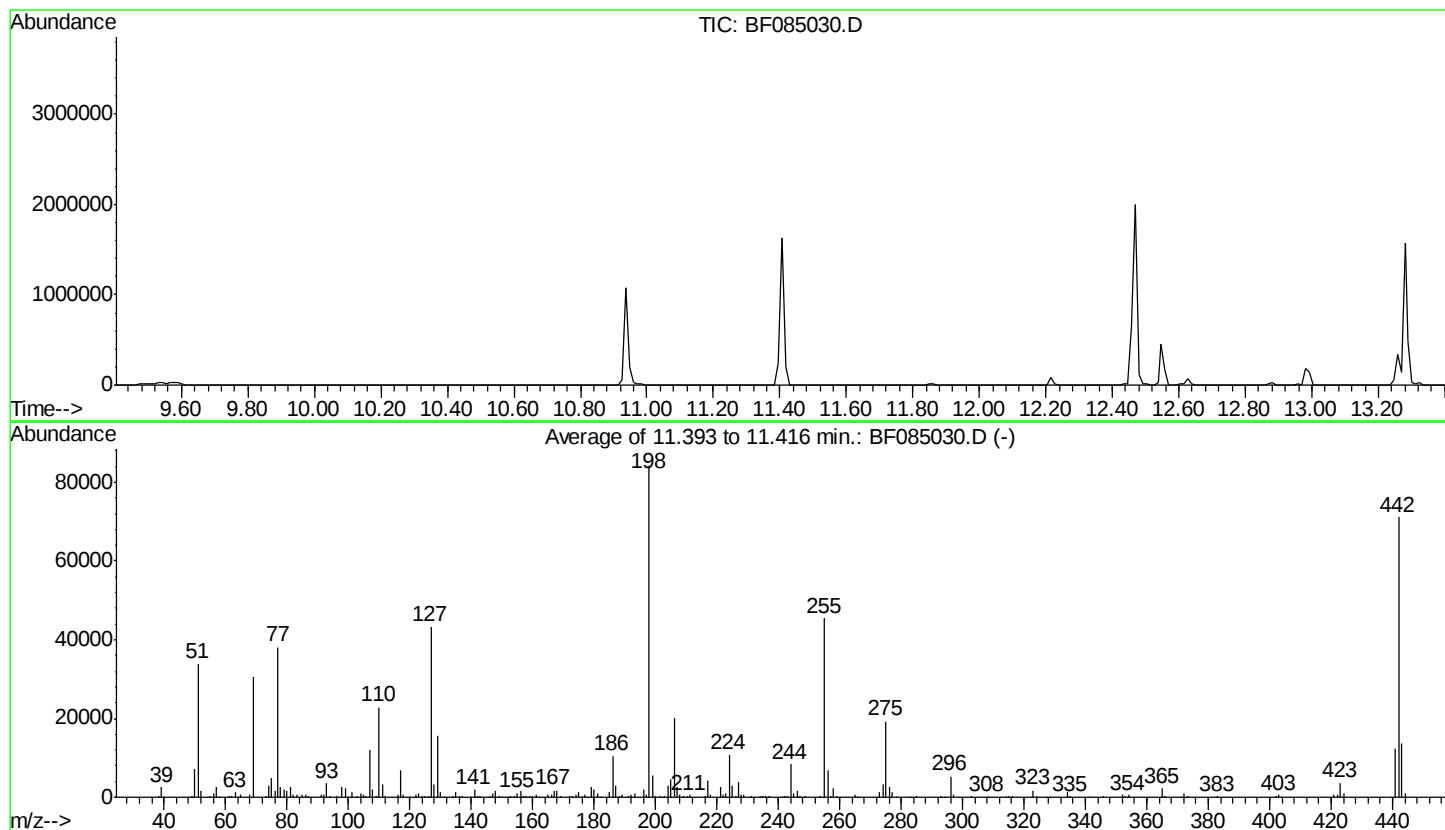

AutoFind: Scans 858, 859, 860; Background Corrected with Scan 855

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	33895	PASS
68	69	0.00	2	1.7	527	PASS
69	198	0.00	100	36.4	30632	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.4	43320	PASS
197	198	0.00	2	0.7	621	PASS
198	198	100	100	100.0	84207	PASS
199	198	5	9	6.5	5507	PASS
275	198	10	60	23.0	19349	PASS
365	198	1	100	2.6	2214	PASS
441	442	0.01	24	17.2	12238	PASS
442	198	50	100	84.5	71130	PASS
443	442	15	24	19.1	13570	PASS