
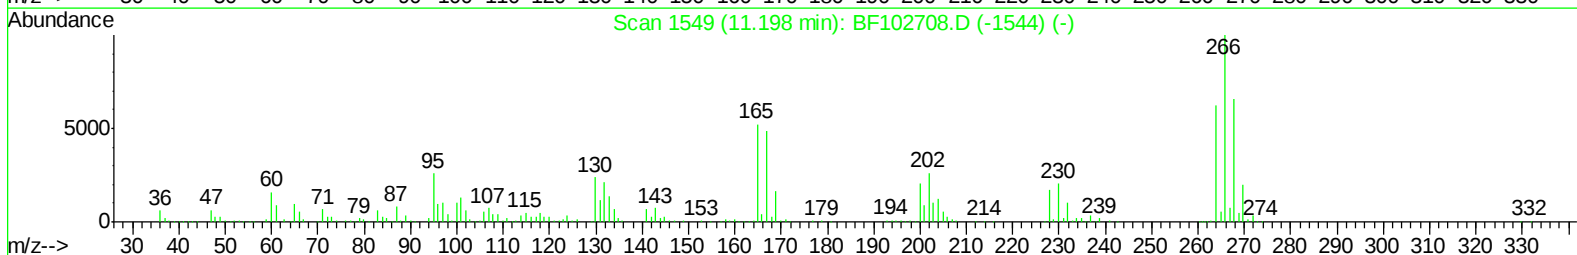
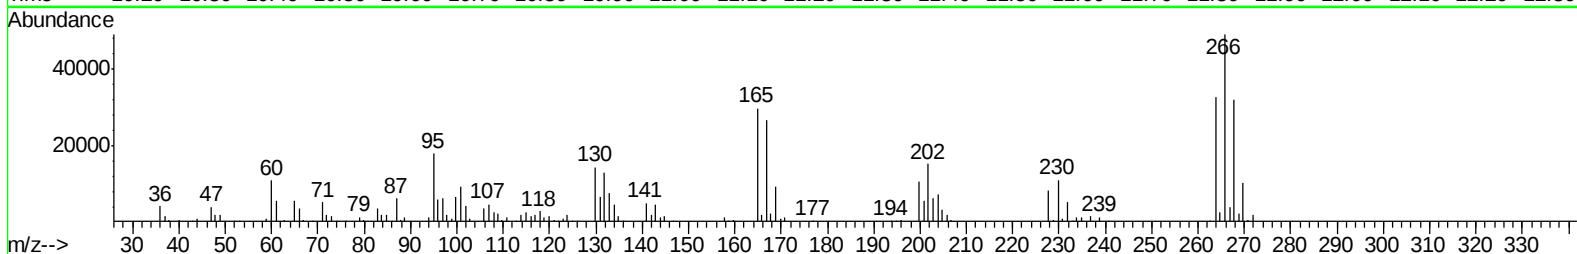


Data Path : Z:\HPCHEM1\BNA F\DATA\BF021218\
Data File : BF102906.D
Acq On : 12 Feb 2018 8:15
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 06:26:23 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 12:44:16 2018
Response via : Initial Calibration

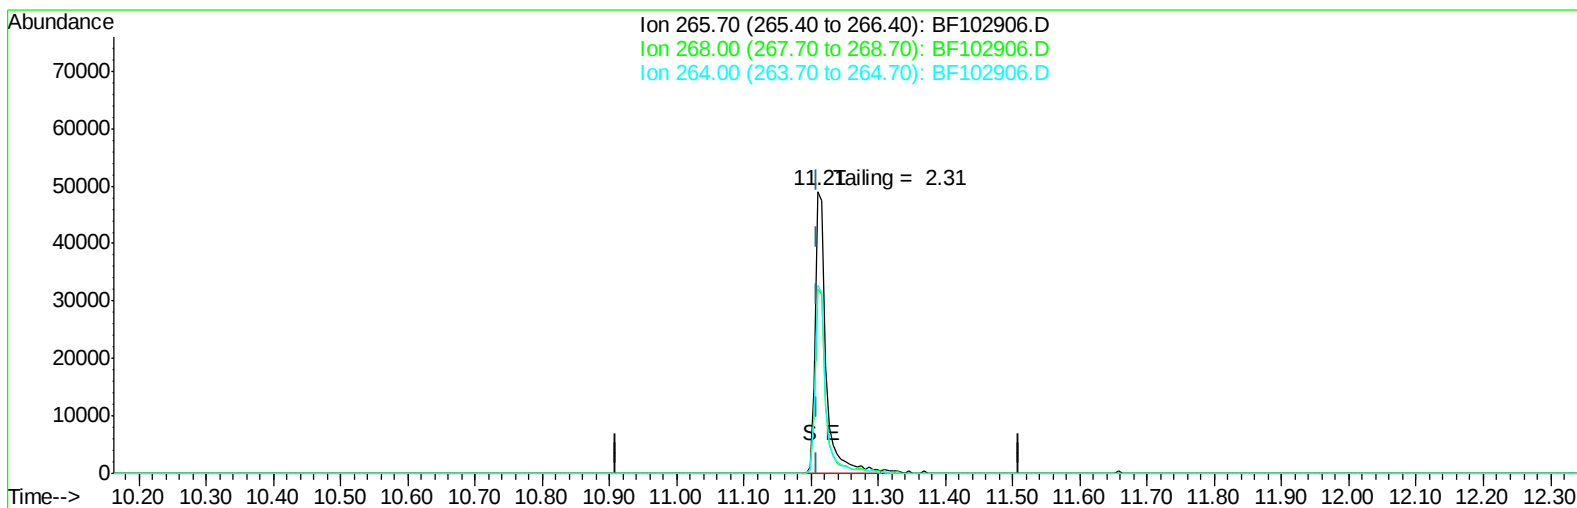

TIC: BF102906.D

(69) Pentachlorophenol (C)




11.210min (-0.000) 20482.83ng

response 57669

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.32
264.00	61.90	66.90
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF021218\
Data File : BF102906.D
Acq On : 12 Feb 2018 8:15
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 06:26:23 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 12:44:16 2018
Response via : Initial Calibration

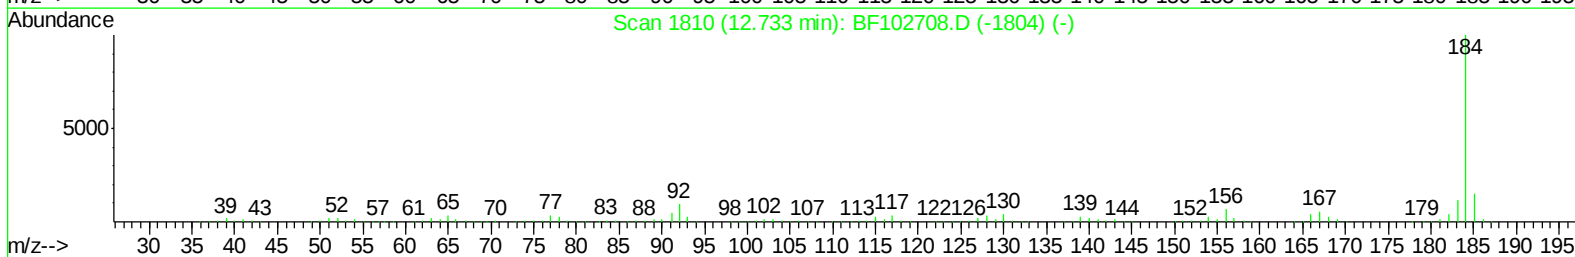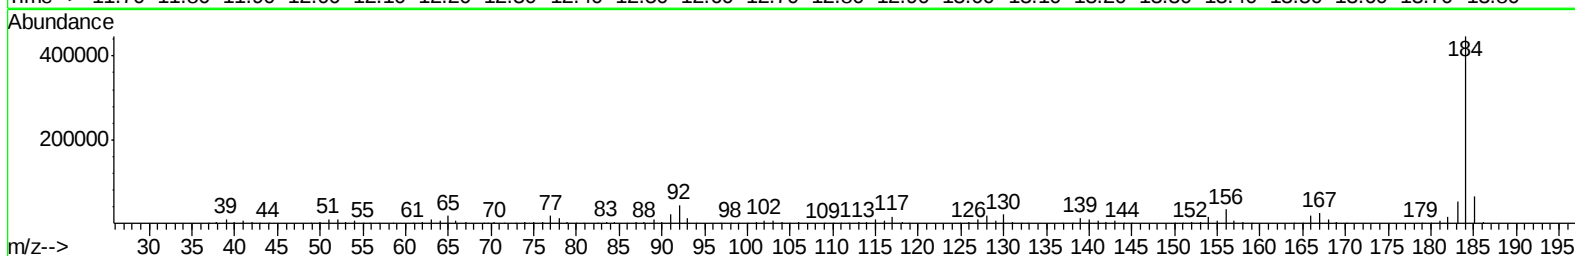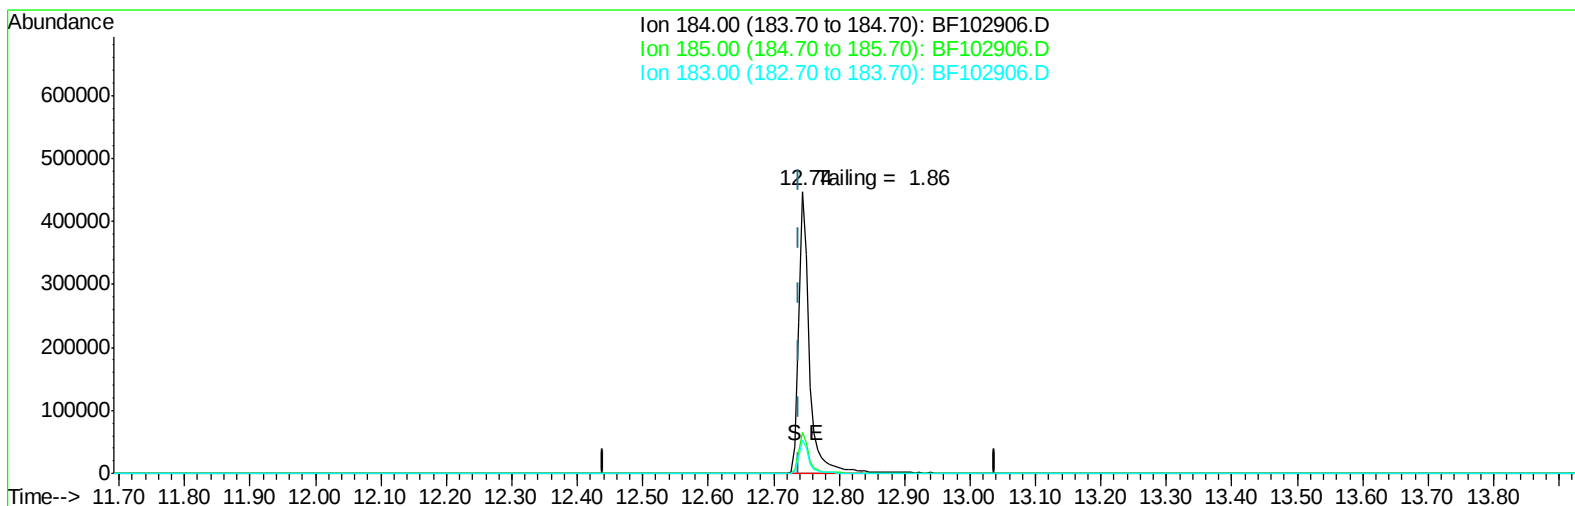

TIC: BF102906.D

(76) Benzidine

12.745min (+0.006) 0.00ng

response 513933

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.61
183.00	11.60	11.62
0.00	0.00	0.00