
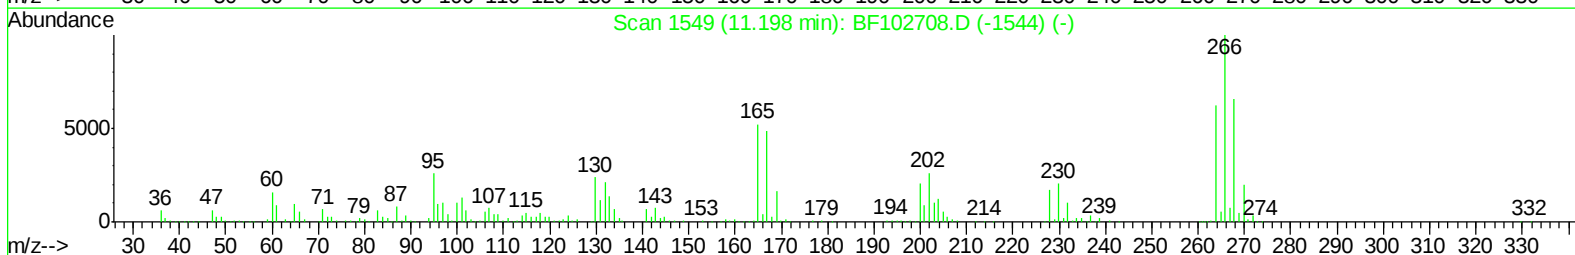
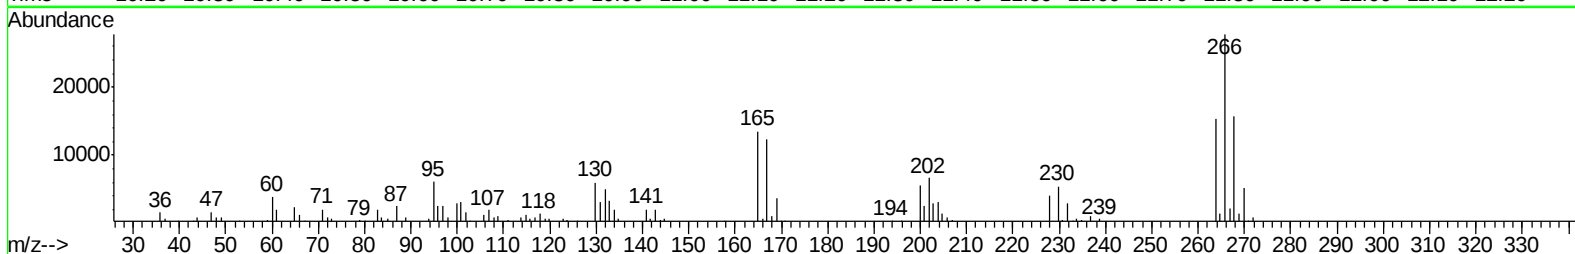


Data Path : Z:\HPCHEM1\BNA F\DATA\BF021218\
Data File : BF102932.D
Acq On : 12 Feb 2018 21:25
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 06:27:53 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 12:44:16 2018
Response via : Initial Calibration

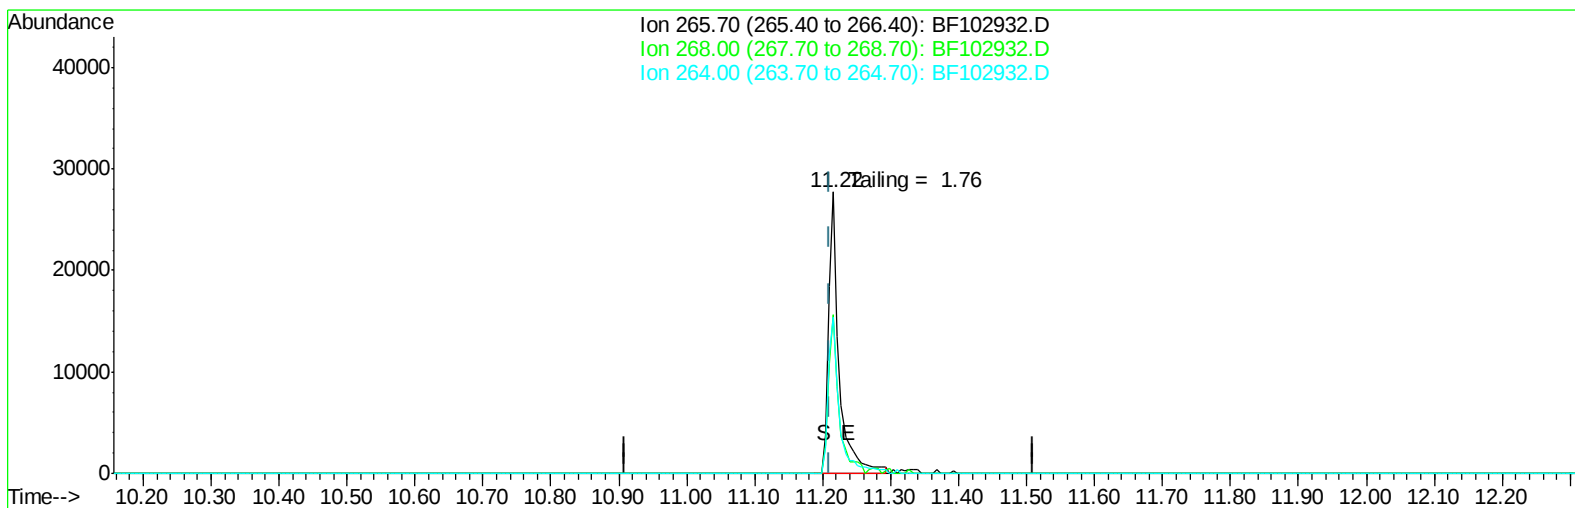

TIC: BF102932.D

(69) Pentachlorophenol (C)




11.216min (+0.006) 0.00ng

response 30286

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	56.48
264.00	61.90	55.50
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF021218\
 Data File : BF102932.D
 Acq On : 12 Feb 2018 21:25
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 06:27:53 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 12:44:16 2018
 Response via : Initial Calibration

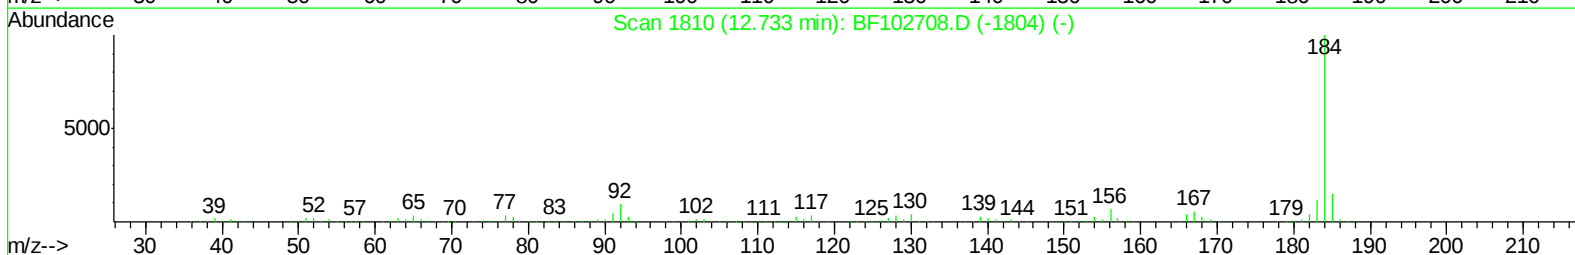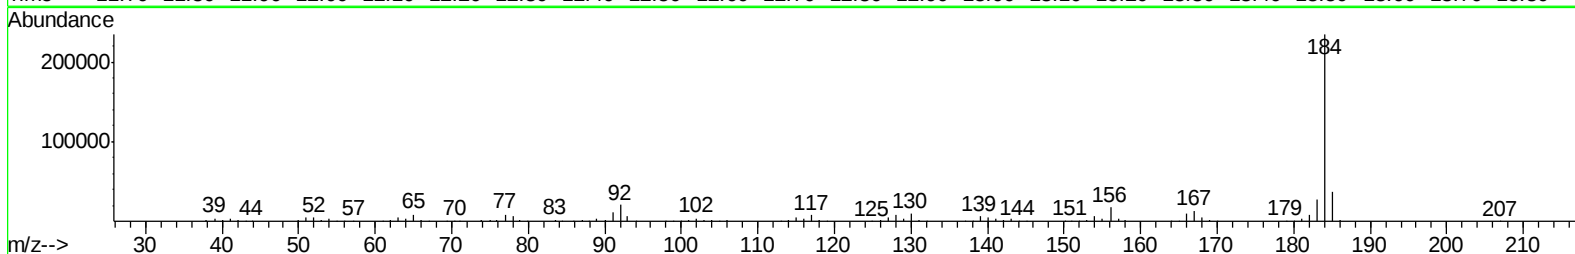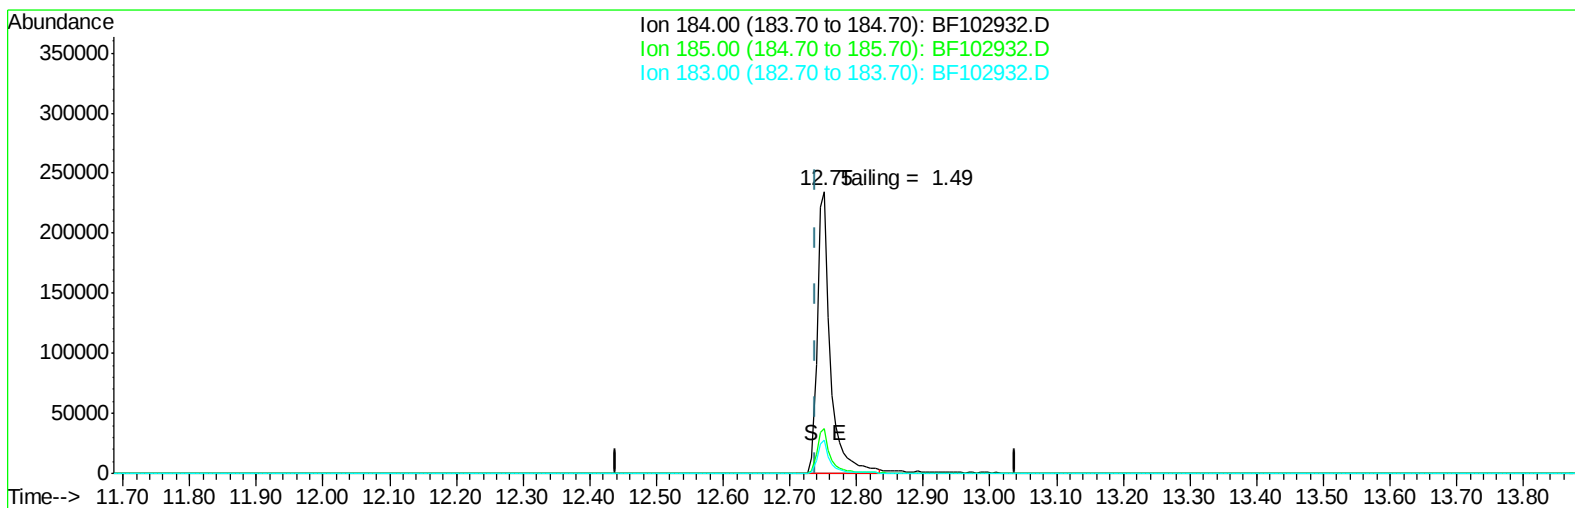

TIC: BF102932.D

(76) Benzidine

12.751min (+0.012) 0.00ng

response 324203

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.72
183.00	11.60	11.74
0.00	0.00	0.00