


Data Path : Z:\HPCHEM1\BNA F\Data\BF021218\
 Data File : BF102906.D
 Acq On : 12 Feb 2018 8:15
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 05 00:38:27 2018

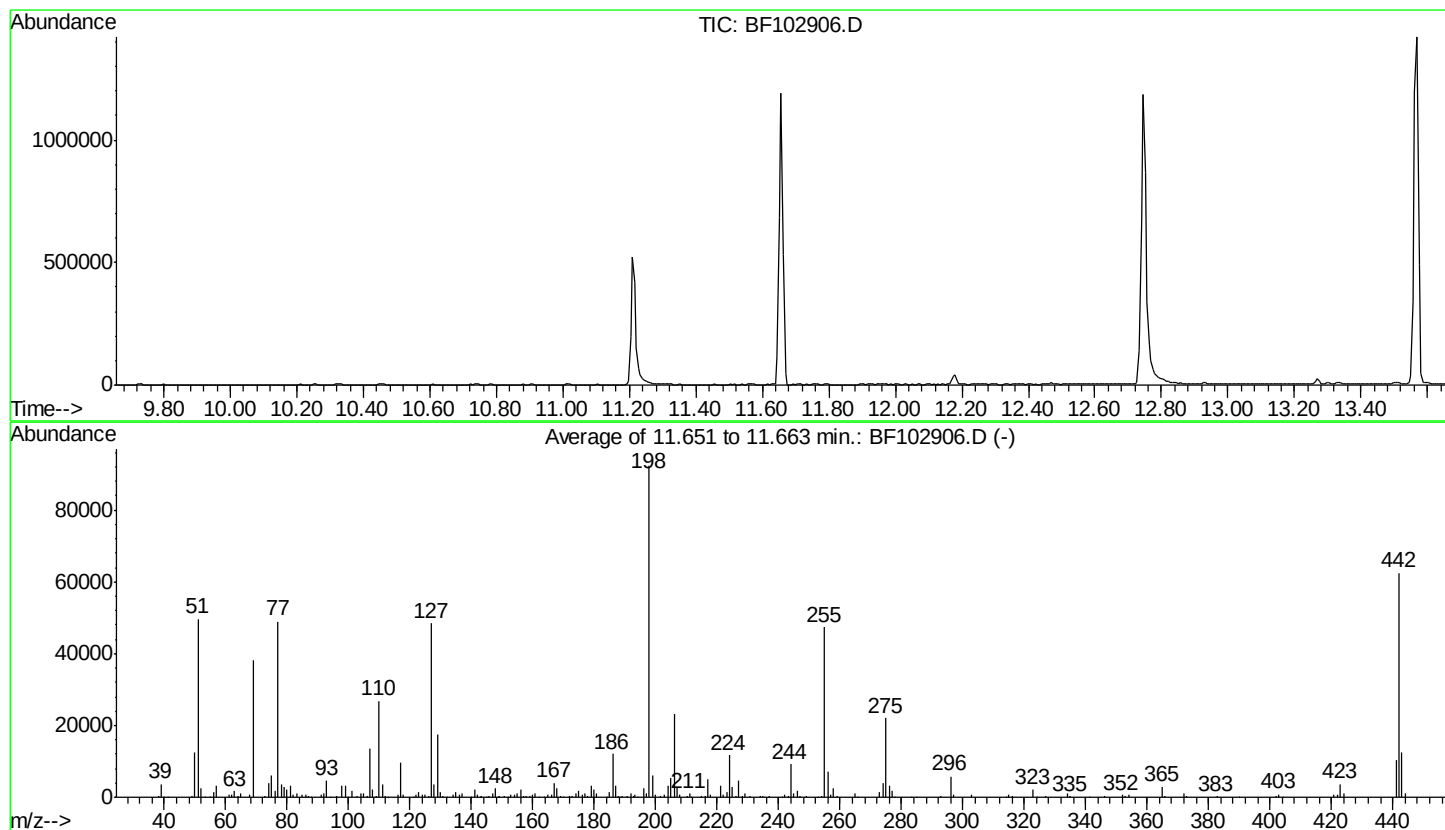

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.7	49621	PASS
68	69	0.00	2	1.9	725	PASS
69	198	0.00	100	41.4	38264	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.4	48405	PASS
197	198	0.00	2	1.0	908	PASS
198	198	100	100	100.0	92386	PASS
199	198	5	9	6.6	6085	PASS
275	198	10	60	23.9	22039	PASS
365	198	1	100	3.2	2939	PASS
441	443	0.01	100	83.7	10530	PASS
442	198	50	100	67.6	62429	PASS
443	442	15	24	20.1	12576	PASS