


Data Path : Z:\HPCHEM1\BNA F\Data\BF021218\
 Data File : BF102932.D
 Acq On : 12 Feb 2018 21:25
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 05 00:38:27 2018

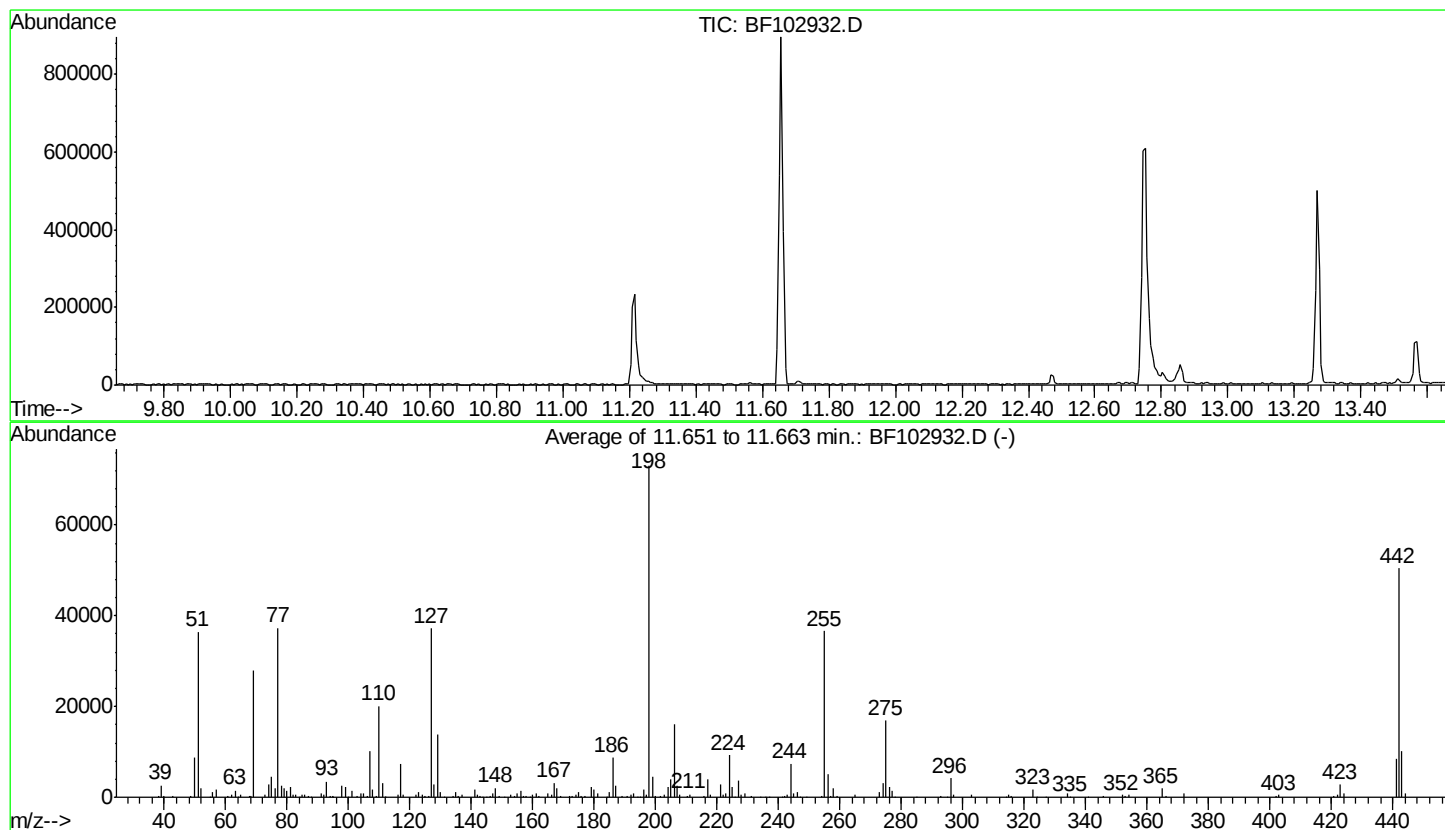

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.0	36522	PASS
68	69	0.00	2	0.9	256	PASS
69	198	0.00	100	38.3	27999	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.9	37242	PASS
197	198	0.00	2	0.7	539	PASS
198	198	100	100	100.0	73104	PASS
199	198	5	9	6.2	4543	PASS
275	198	10	60	23.0	16826	PASS
365	198	1	100	2.7	1975	PASS
441	443	0.01	100	84.8	8542	PASS
442	198	50	100	69.1	50514	PASS
443	442	15	24	20.0	10079	PASS