

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF021219\
 Data File : BF112510.D
 Acq On : 12 Feb 2019 14:41
 Operator : JU/SJ
 Sample : K1459-07RE
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 M-10-D

Quant Time: Feb 13 03:38:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 10:38:18 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	88564	20.00	ng	-0.01
21) Naphthalene-d8	8.12	136	354041	20.00	ng	-0.01
39) Acenaphthene-d10	9.87	164	174088	20.00	ng	-0.02
64) Phenanthrene-d10	11.36	188	369055	20.00	ng	0.00
76) Chrysene-d12	14.01	240	297393	20.00	ng	0.00
87) Perylene-d12	15.49	264	217197	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	488971	117.27	ng	-0.01
7) Phenol-d6	6.49	99	632484	109.17	ng	0.00
23) Nitrobenzene-d5	7.40	82	392185	63.83	ng	-0.01
42) 2,4,6-Tribromophenol	10.67	330	216107	106.65	ng	-0.01
45) 2-Fluorobiphenyl	9.19	172	804274	65.34	ng	-0.02
79) Terphenyl-d14	12.95	244	976496	61.84	ng	0.00
Target Compounds						
10) Phenol	6.50	94	26730	4.205	ng	96
19) n-Nitroso-di-n-propylamine	7.40	70	54260	13.582	ng	# 76
25) Isophorone	7.40	82	392182	40.686	ng	# 63
50) Dimethylphthalate	9.58	163	59766	4.419	ng	100
51) 2,6-Dinitrotoluene	9.87	165	21876	7.222	ng	# 33
57) 2,4-Dinitrotoluene	9.87	165	21876	5.673	ng	# 31
67) 4-Bromophenyl-phenylether	10.67	248	12614	2.906	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF021219\
Data File : BF112510.D
Acq On : 12 Feb 2019 14:41
Operator : JU/SJ
Sample : K1459-07RE
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
M-10-D

Quant Time: Feb 13 03:38:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

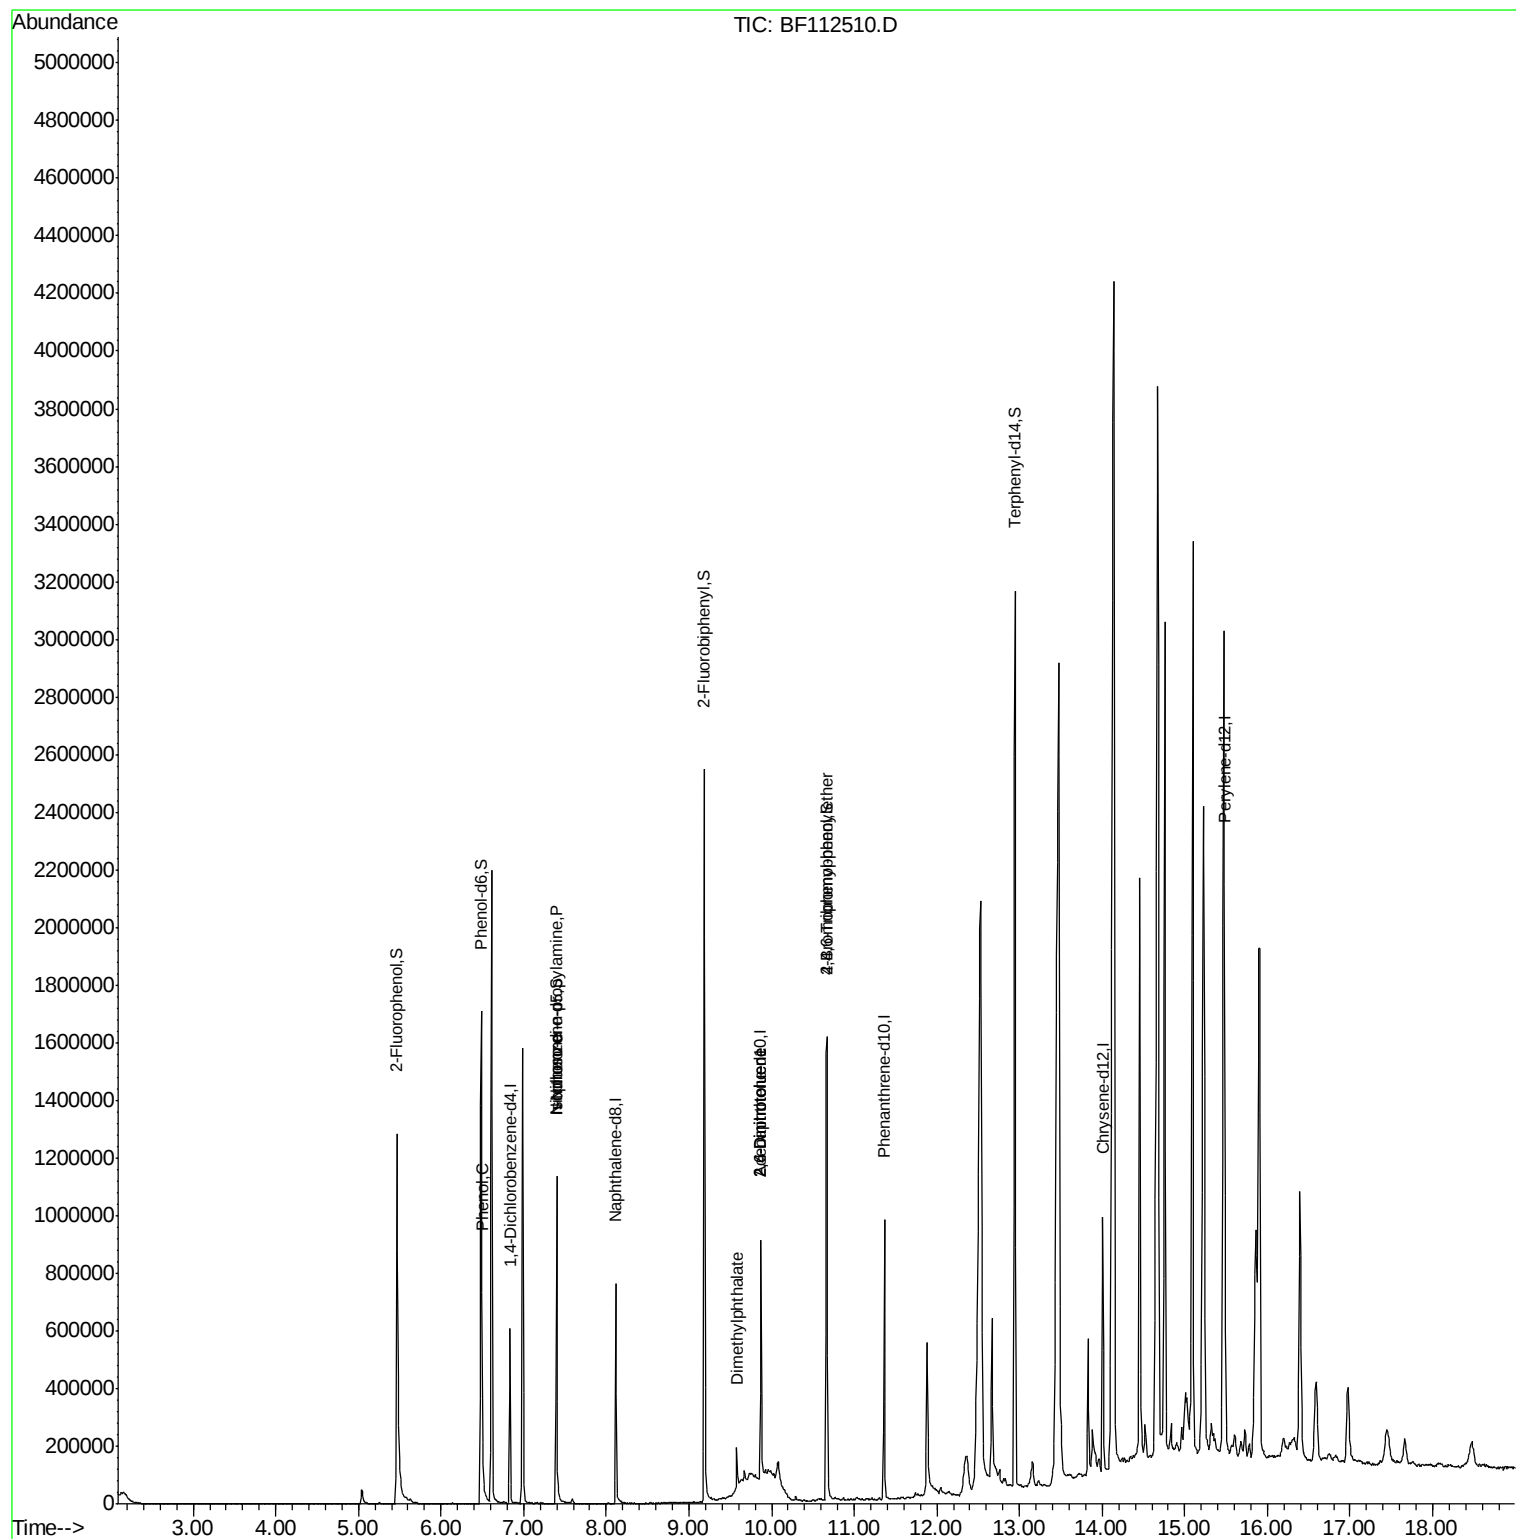

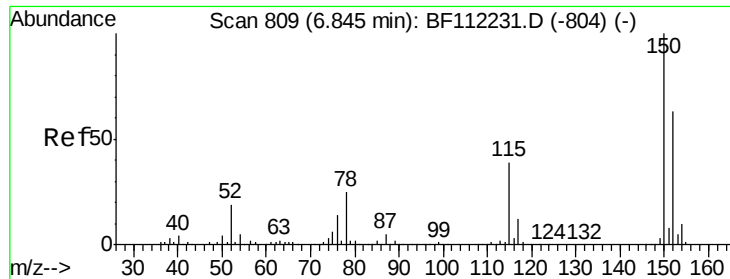


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.83 min Scan# 807
 Delta R.T. -0.01 min
 Lab File: BF112510.D
 Acq: 12 Feb 2019 14:41

Instrument :
 BNA_F
 ClientSampleId :
 M-10-D

Tgt Ion:152 Resp: 88564
 Ion Ratio Lower Upper
 152 100
 150 154.6 127.4 191.0
 115 60.7 45.5 68.3

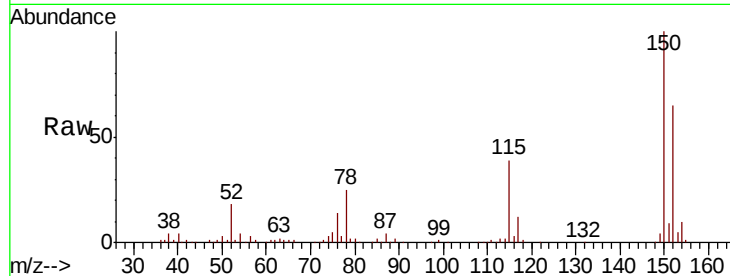


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

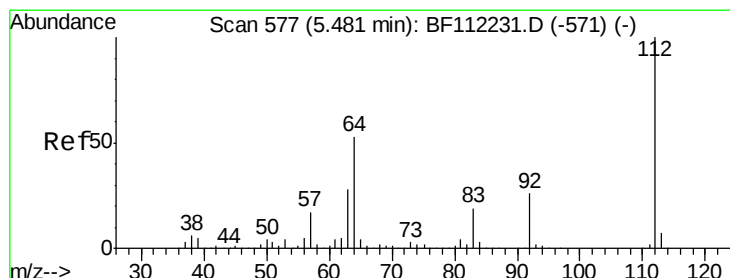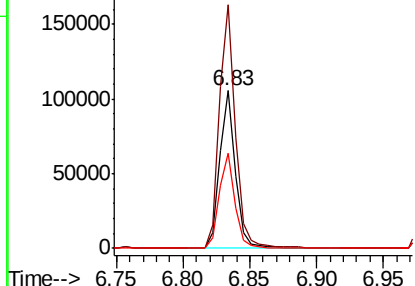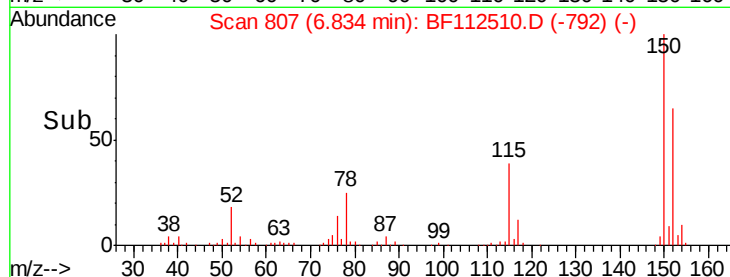



#5


2-Fluorophenol
 Concen: 117.272 ng
 RT: 5.47 min Scan# 575
 Delta R.T. -0.01 min
 Lab File: BF112510.D
 Acq: 12 Feb 2019 14:41

Tgt Ion:112 Resp: 488971
 Ion Ratio Lower Upper
 112 100
 64 55.2 45.7 68.5
 63 30.3 23.6 35.4

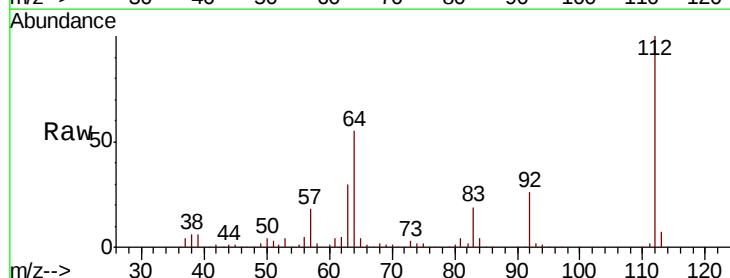

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

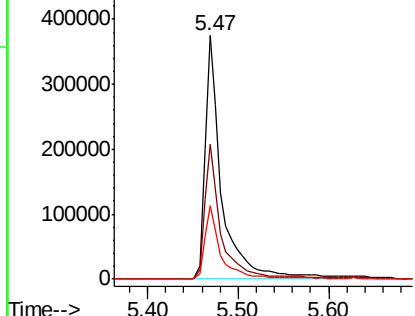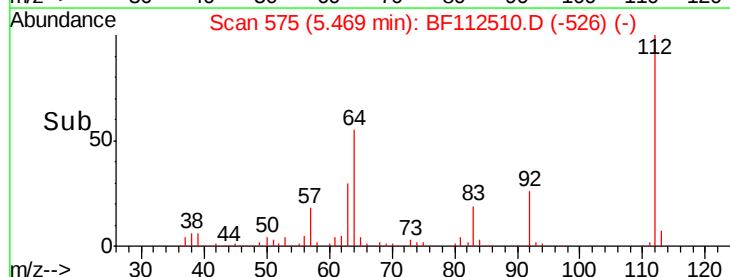

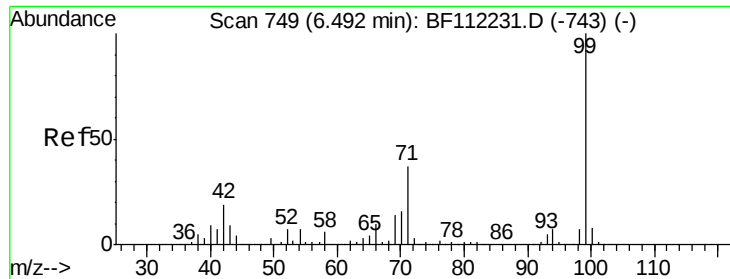

#7

Phenol-d6

Concen: 109.166 ng

RT: 6.49 min Scan# 748

Delta R.T. -0.01 min

Lab File: BF112510.D

Acq: 12 Feb 2019 14:41

Instrument :

BNA_F

ClientSampleId :

M-10-D


Tgt Ion: 99 Resp: 632484

Ion Ratio Lower Upper




99 100

42 17.9 15.1 22.7

71 35.9 26.9 40.3

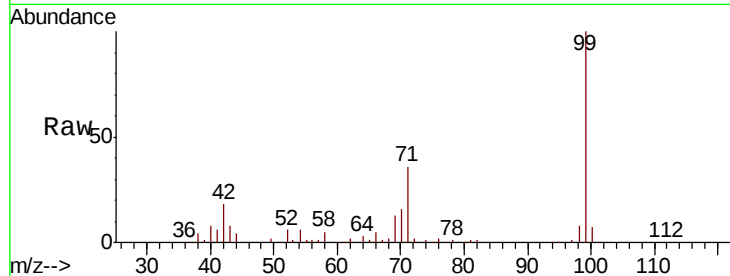

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

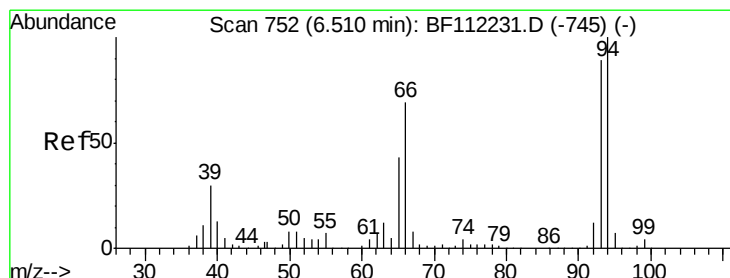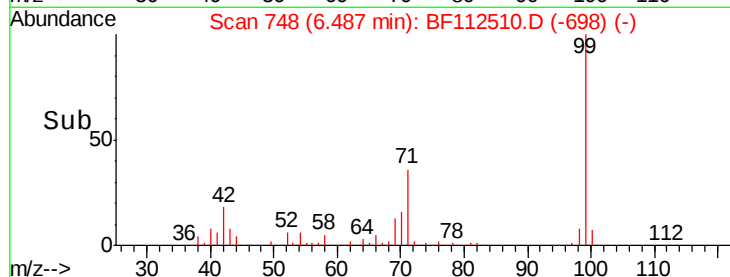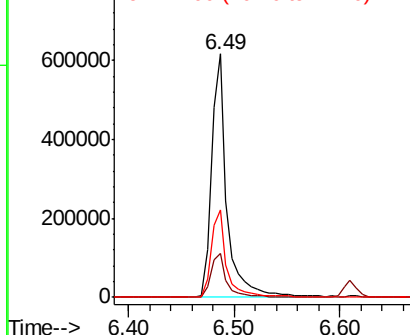

#10

Phenol

Concen: 4.205 ng

RT: 6.50 min Scan# 750

Delta R.T. -0.01 min

Lab File: BF112510.D

Acq: 12 Feb 2019 14:41


Tgt Ion: 94 Resp: 26730

Ion Ratio Lower Upper



94 100


65 33.5 20.3 60.3

66 62.4 42.4 82.4

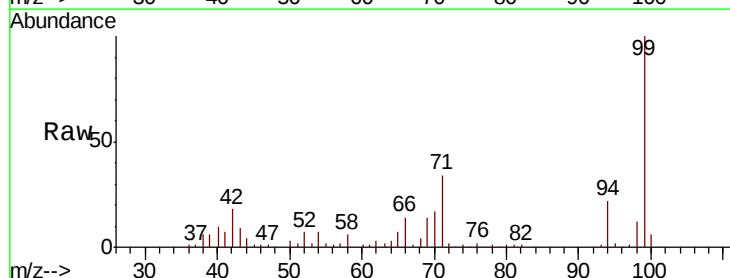

Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1



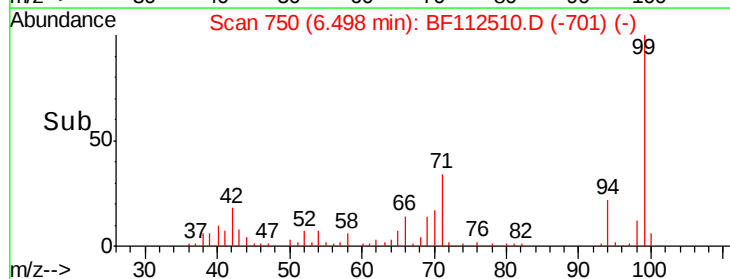
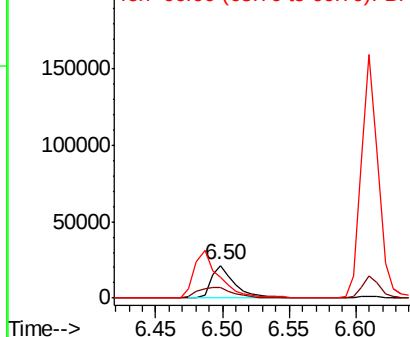


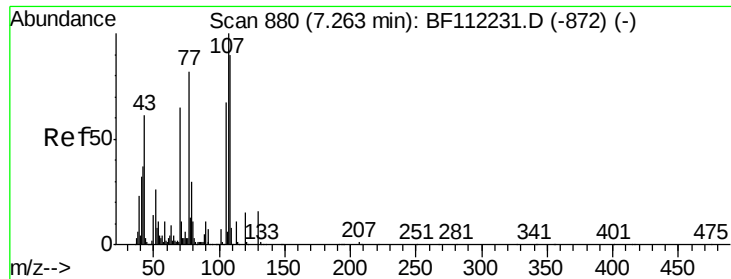

#19
n-Nitroso-di-n-propylamine
Concen: 13.582 ng
RT: 7.40 min Scan# 903
Delta R.T. 0.14 min
Lab File: BF112510.D
Acq: 12 Feb 2019 14:41




Instrument :
BNA_F
ClientSampleId :
M-10-D


Tgt Ion: 70 Resp: 54260
Ion Ratio Lower Upper
70 100
42 47.1 47.6 71.4#
101 0.0 7.9 11.9#
130 1.9 18.4 27.6#

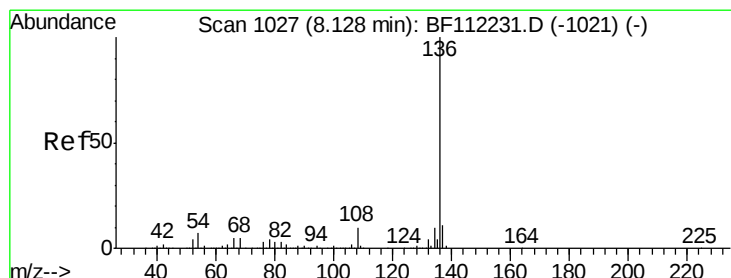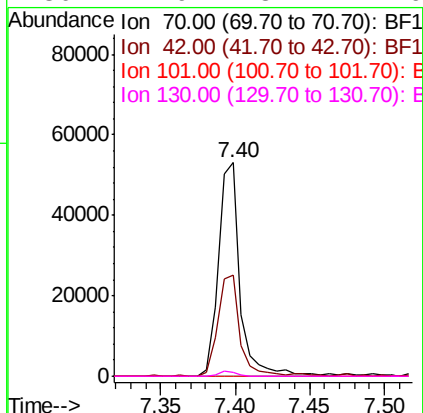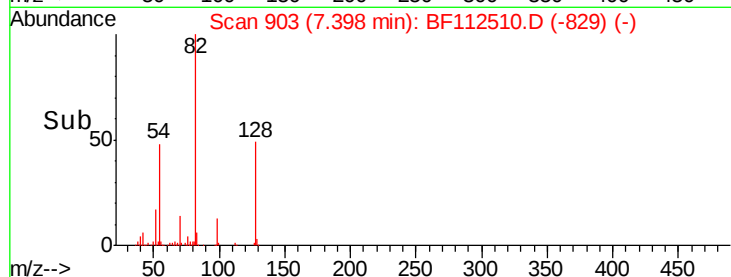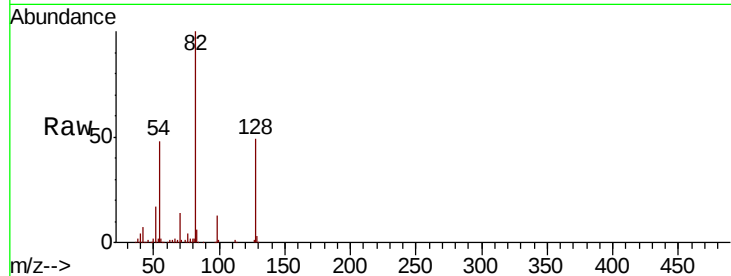

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.12 min Scan# 1025
Delta R.T. -0.01 min
Lab File: BF112510.D
Acq: 12 Feb 2019 14:41

Tgt Ion: 136 Resp: 354041
Ion Ratio Lower Upper
136 100
137 10.3 9.1 13.7
54 5.9 5.9 8.9#
68 4.5 5.1 7.7#

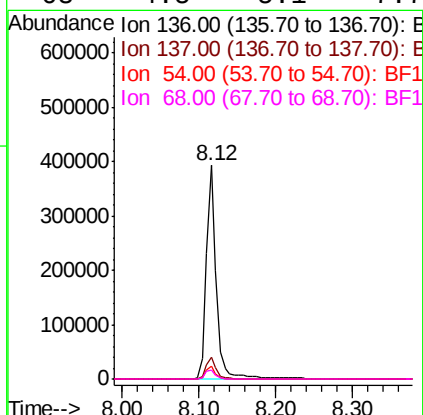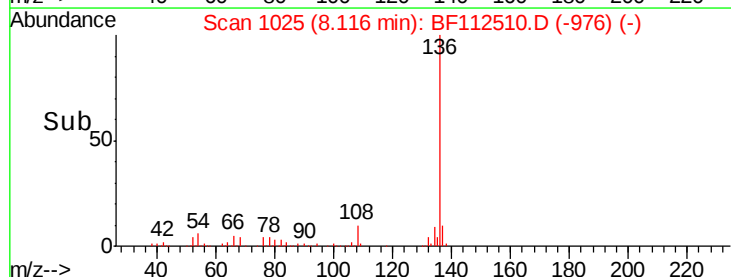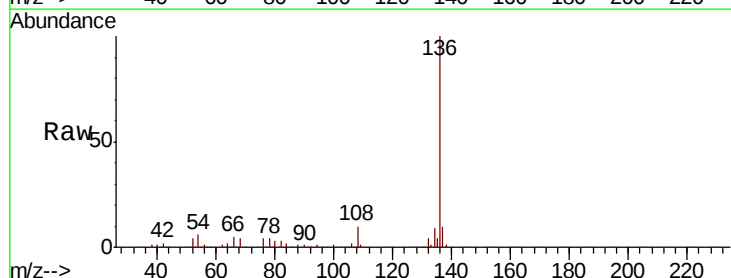


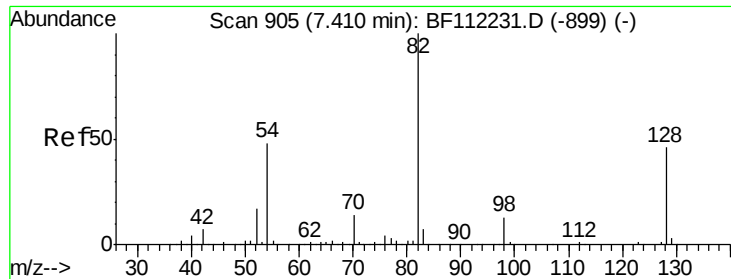




#23
 Nitrobenzene-d5
 Concen: 63.828 ng
 RT: 7.40 min Scan# 903
 Delta R.T. -0.01 min
 Lab File: BF112510.D
 Acq: 12 Feb 2019 14:41

Instrument :
 BNA_F
 ClientSampleID :
 M-10-D

Tgt Ion	Ratio	Lower	Upper
82	100		
128	48.8	37.8	56.8
54	47.9	39.7	59.5

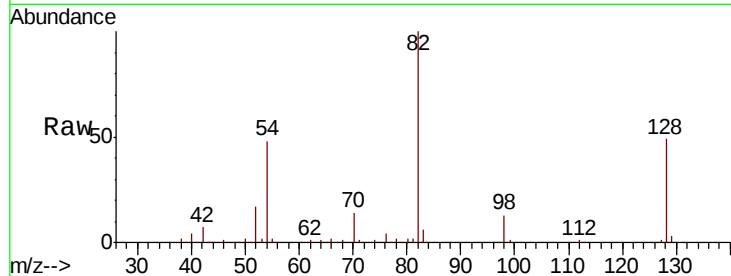


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

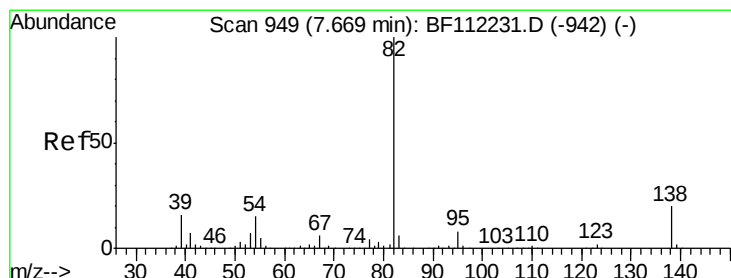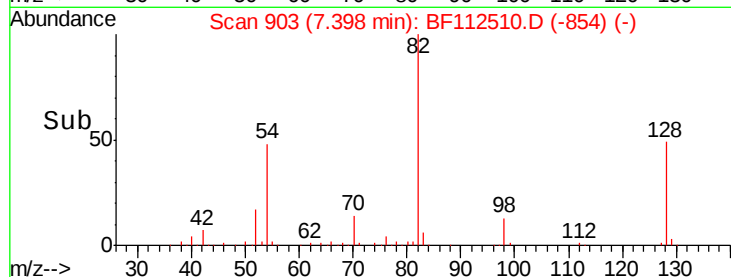
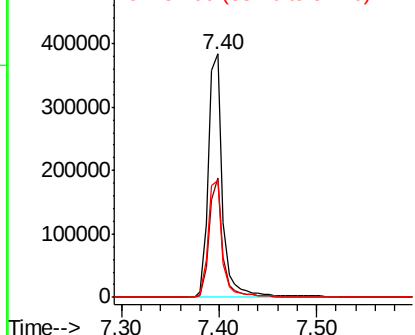



#25
 Isophorone
 Concen: 40.686 ng
 RT: 7.40 min Scan# 903
 Delta R.T. -0.27 min
 Lab File: BF112510.D
 Acq: 12 Feb 2019 14:41

Tgt Ion	Ratio	Lower	Upper
82	100		
95	0.0	5.7	8.5#
138	0.0	15.4	23.0#

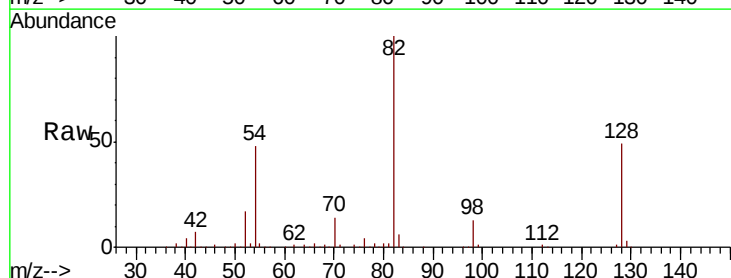

Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 95.00 (94.70 to 95.70): BF1
 Ion 138.00 (137.70 to 138.70): BF1

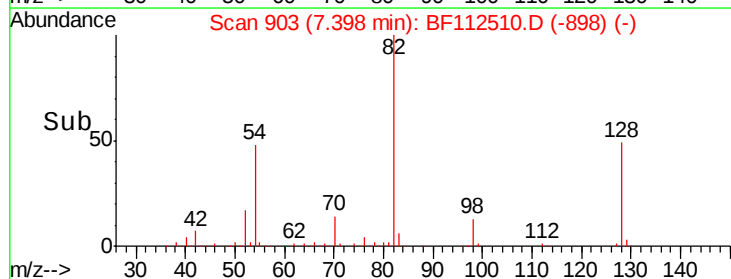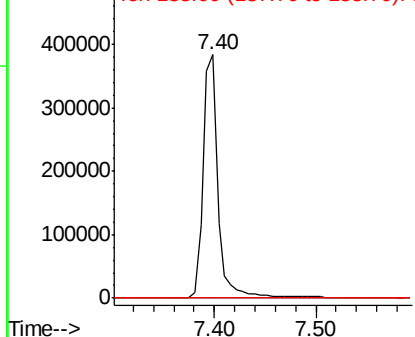

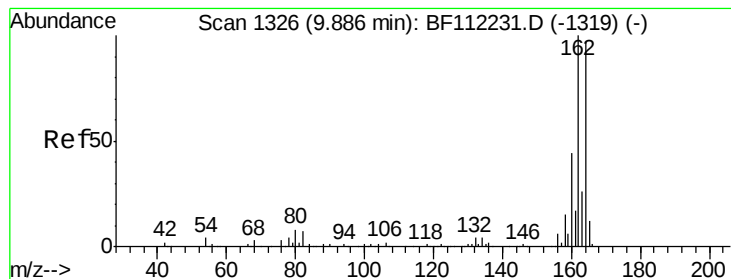

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.87 min Scan# 1323

Delta R.T. -0.02 min

Lab File: BF112510.D

Acq: 12 Feb 2019 14:41

Instrument :

BNA_F

ClientSampleId :

M-10-D


Tgt Ion:164 Resp: 174088

Ion Ratio Lower Upper




164 100

162 106.3 82.2 123.4

160 48.8 36.2 54.4

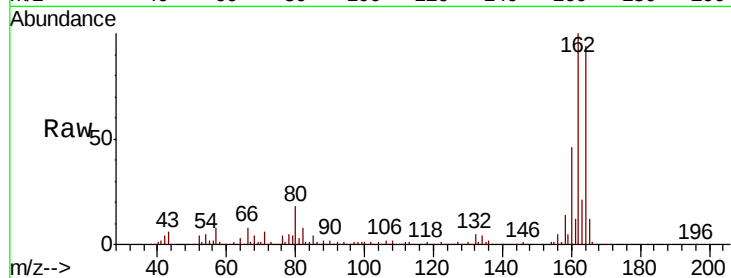

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

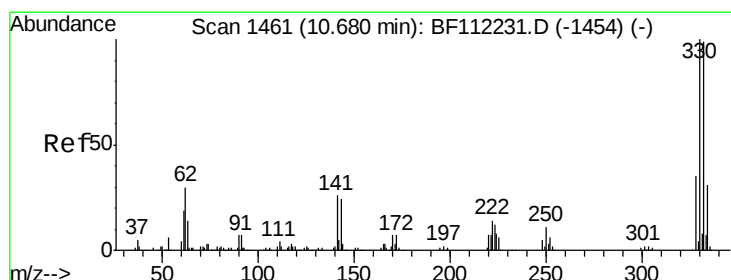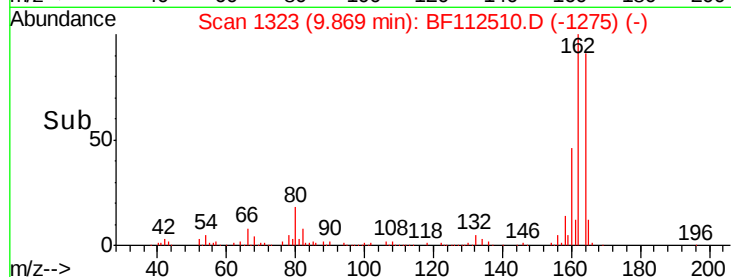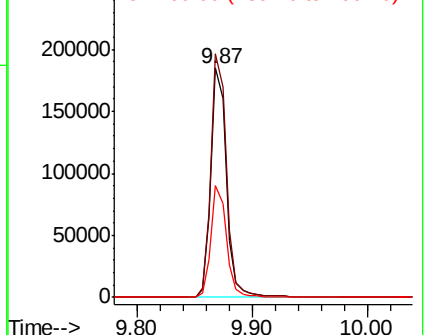

#42

2,4,6-Tribromophenol

Concen: 106.649 ng

RT: 10.67 min Scan# 1459

Delta R.T. -0.01 min

Lab File: BF112510.D

Acq: 12 Feb 2019 14:41


Tgt Ion:330 Resp: 216107

Ion Ratio Lower Upper



330 100


332 97.4 76.6 114.8

141 34.3 24.3 36.5

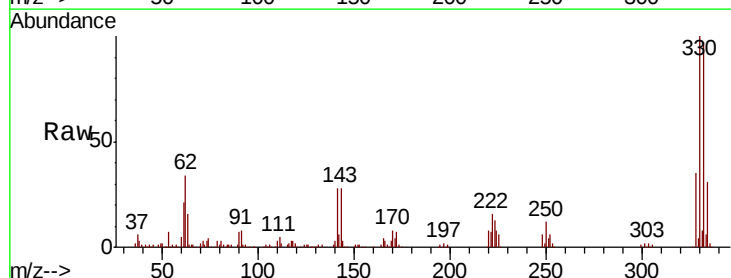

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

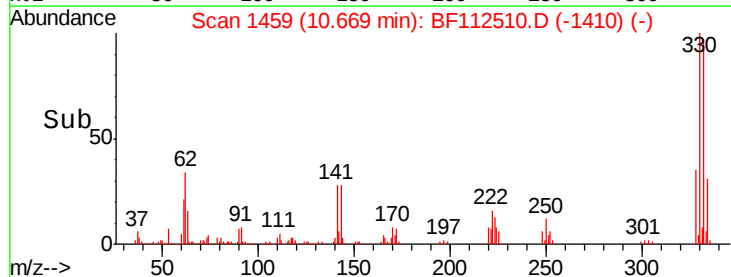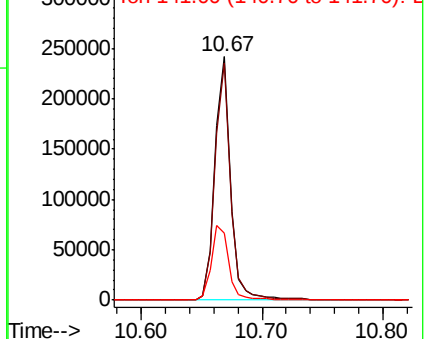

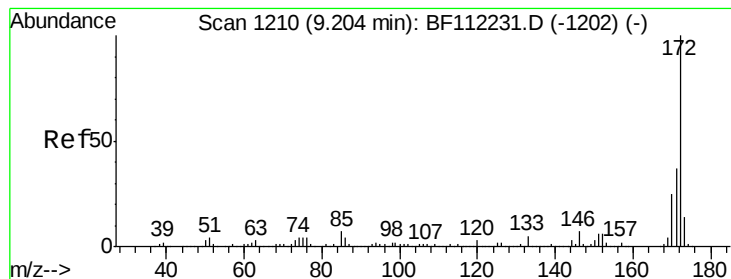

#45

2-Fluorobiphenyl

Concen: 65.341 ng

RT: 9.19 min Scan# 1207

Delta R.T. -0.02 min

Lab File: BF112510.D

Acq: 12 Feb 2019 14:41

Instrument :

BNA_F

ClientSampled :

M-10-D


Tgt Ion:172 Resp: 804274

Ion Ratio Lower Upper

172 100

171 35.7 30.5 45.7




170 23.7 20.2 30.4

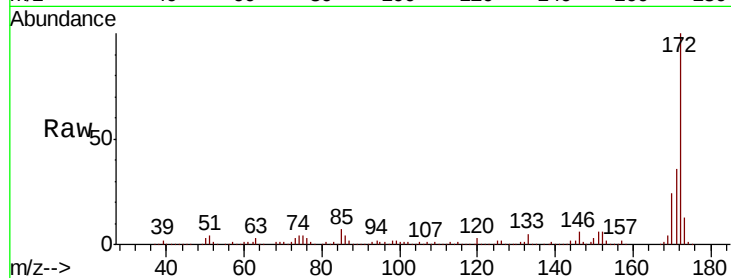

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

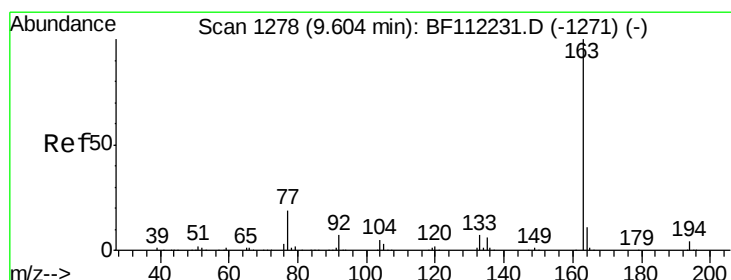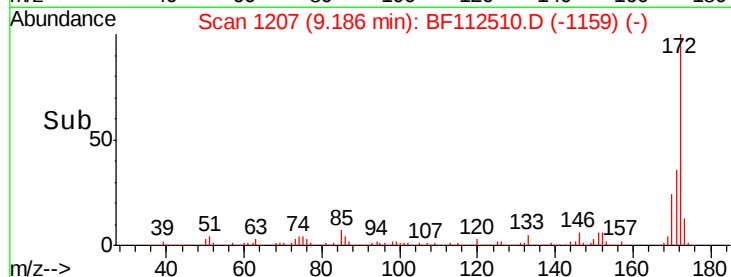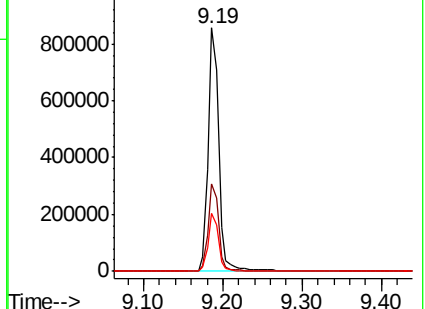

#50

Dimethylphthalate

Concen: 4.419 ng

RT: 9.58 min Scan# 1274

Delta R.T. -0.02 min

Lab File: BF112510.D

Acq: 12 Feb 2019 14:41


Tgt Ion:163 Resp: 59766

Ion Ratio Lower Upper

163 100

194 4.1 3.3 4.9



164 10.4 8.5 12.7

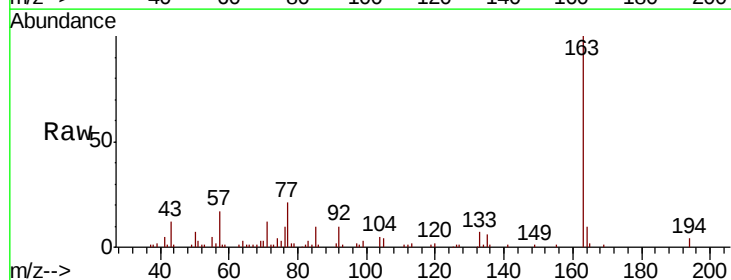


Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E



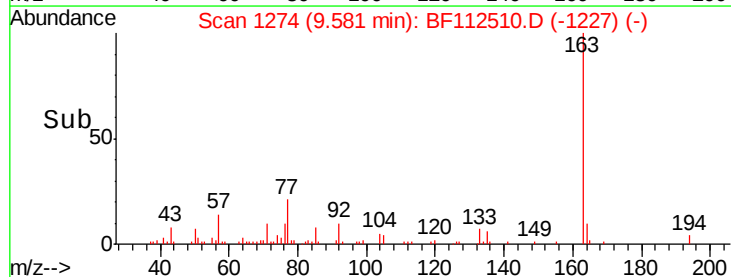
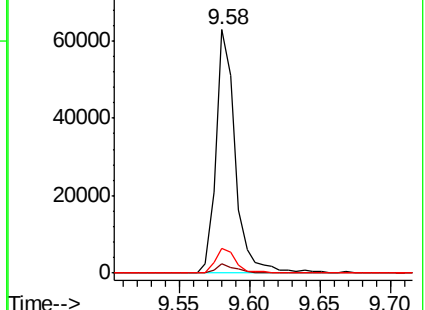


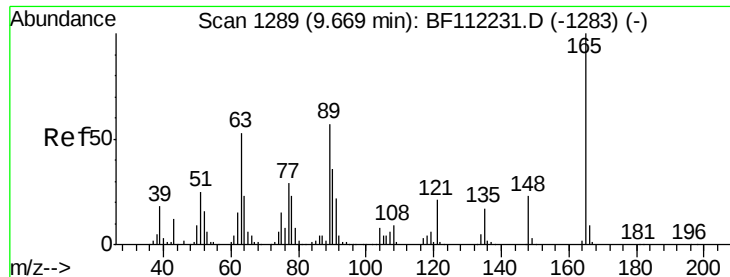

#51
 2,6-Dinitrotoluene
 Concen: 7.222 ng
 RT: 9.87 min Scan# 1323
 Delta R.T. 0.20 min
 Lab File: BF112510.D
 Acq: 12 Feb 2019 14:41




Instrument :
 BNA_F
 ClientSampleId :
 M-10-D


Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	33.8	50.8#
89	1.6	36.9	55.3#

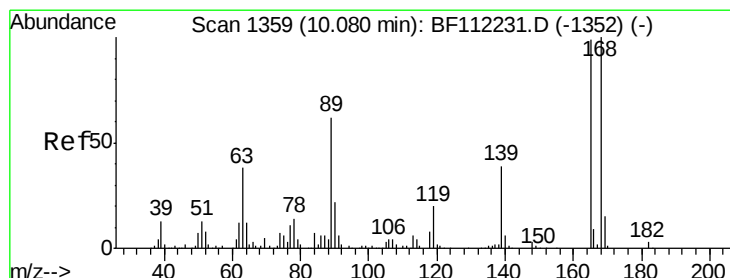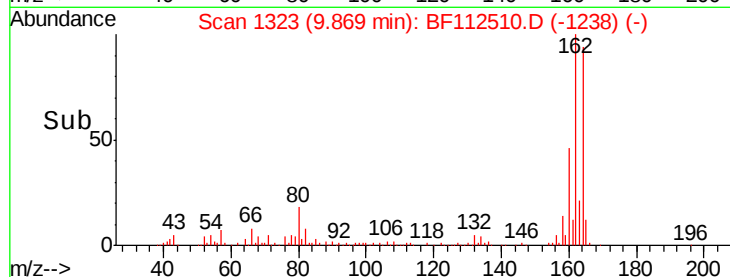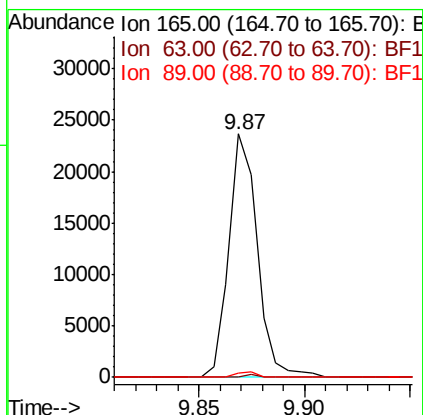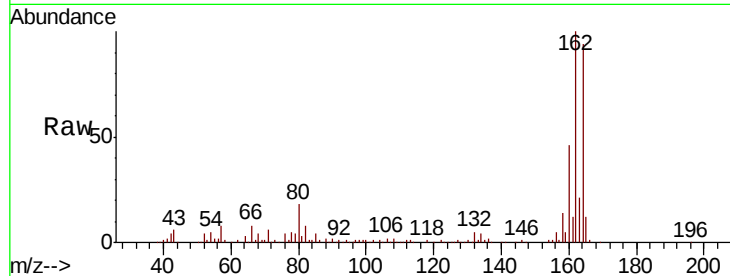

#57
 2,4-Dinitrotoluene
 Concen: 5.673 ng
 RT: 9.87 min Scan# 1323
 Delta R.T. -0.21 min
 Lab File: BF112510.D
 Acq: 12 Feb 2019 14:41

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	27.9	41.9#
89	1.6	47.9	71.9#
182	0.0	2.2	3.4#


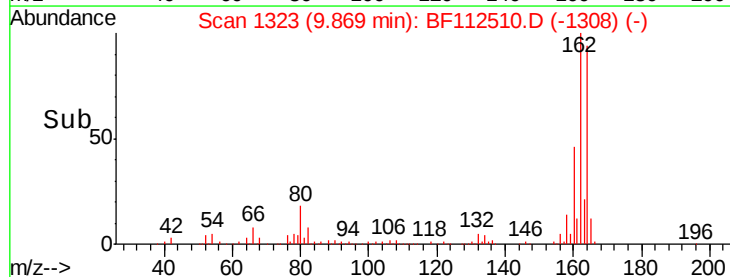
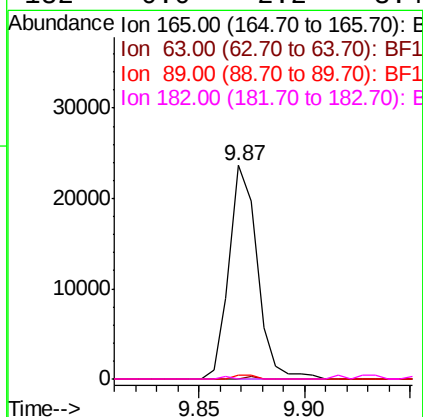
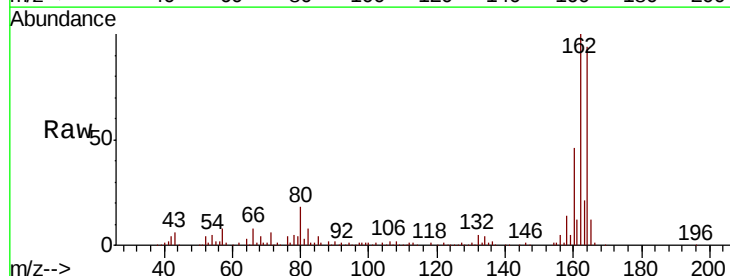


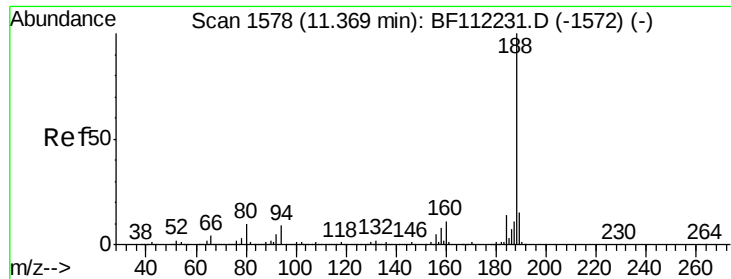

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.36 min Scan# 1577
 Delta R.T. -0.01 min
 Lab File: BF112510.D
 Acq: 12 Feb 2019 14:41




Instrument :
 BNA_F
 ClientSampleId :
 M-10-D


Tgt Ion:188 Resp: 369055
 Ion Ratio Lower Upper
 188 100
 94 7.9 8.2 12.2#
 80 8.6 8.9 13.3#

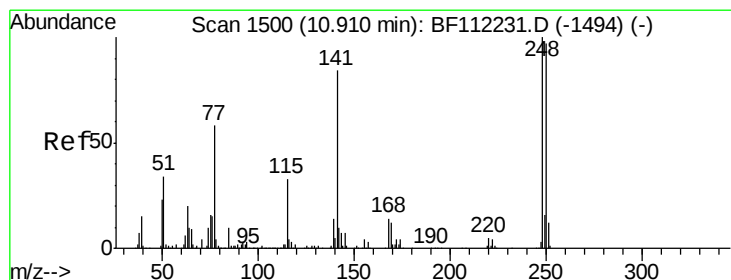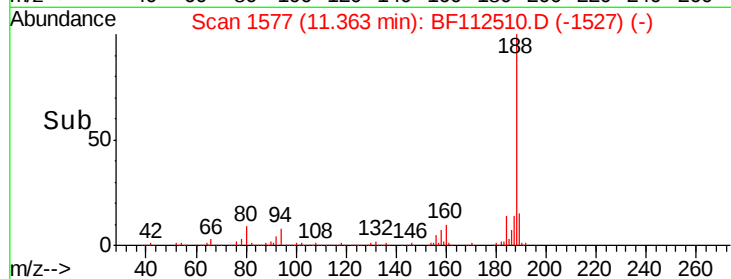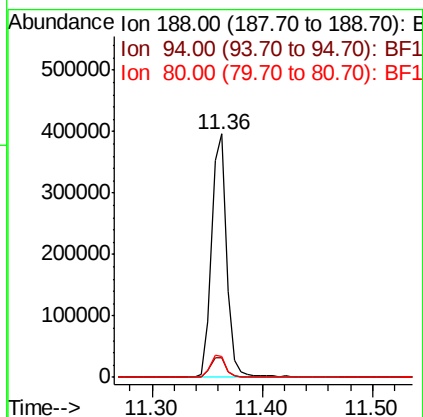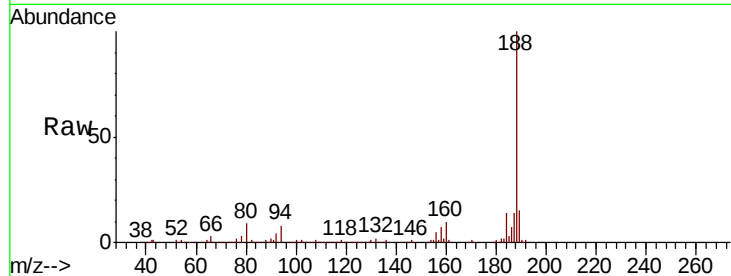

#67
 4-Bromophenyl-phenylether
 Concen: 2.906 ng
 RT: 10.67 min Scan# 1459
 Delta R.T. -0.24 min
 Lab File: BF112510.D
 Acq: 12 Feb 2019 14:41

Tgt Ion:248 Resp: 12614
 Ion Ratio Lower Upper
 248 100
 250 204.0 79.7 119.5#
 141 487.1 60.3 90.5#


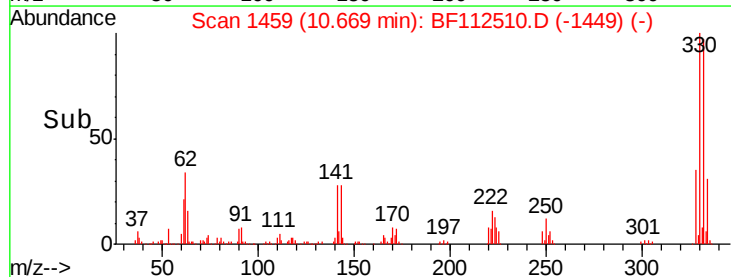
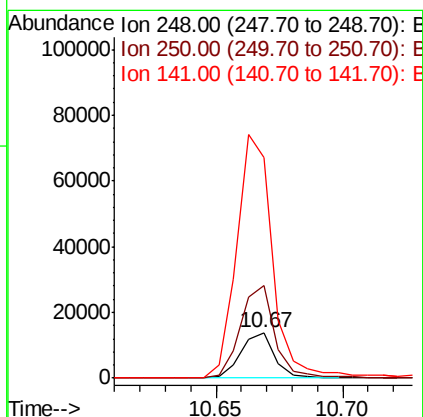
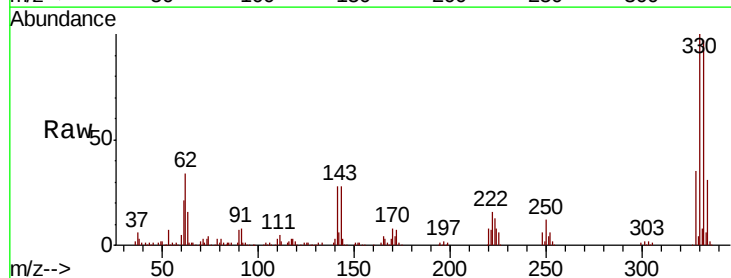


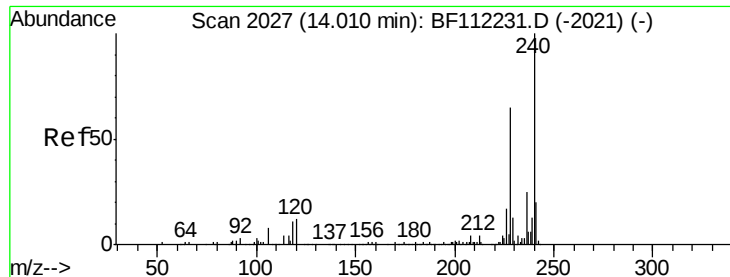

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.01 min Scan# 2027
Delta R.T. 0.00 min
Lab File: BF112510.D
Acq: 12 Feb 2019 14:41




Instrument :
BNA_F
ClientSampleId :
M-10-D


Tgt Ion:240 Resp: 297393
Ion Ratio Lower Upper
240 100
120 10.1 9.0 13.6
236 25.4 20.7 31.1

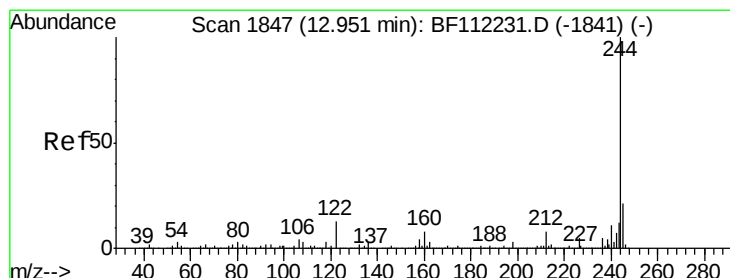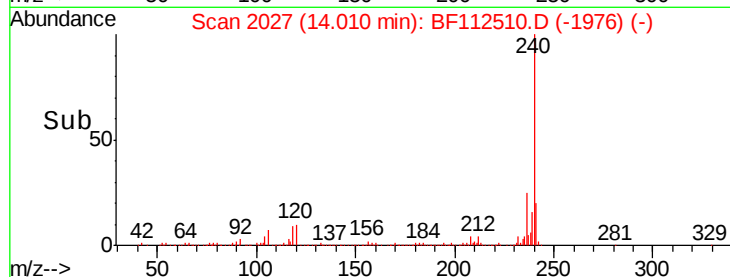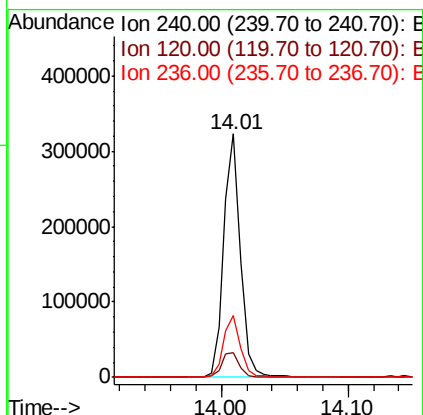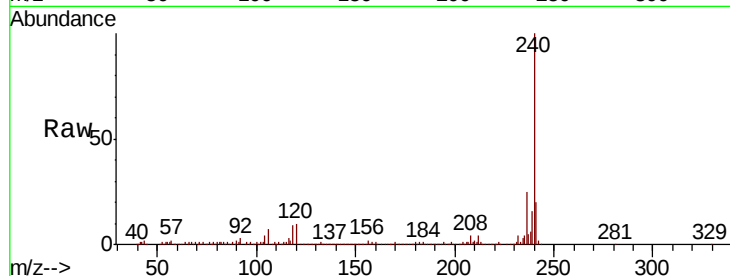

#79
Terphenyl-d14
Concen: 61.843 ng
RT: 12.95 min Scan# 1846
Delta R.T. -0.01 min
Lab File: BF112510.D
Acq: 12 Feb 2019 14:41

Tgt Ion:244 Resp: 976496
Ion Ratio Lower Upper
244 100
212 7.1 5.9 8.9
122 10.5 9.8 14.6

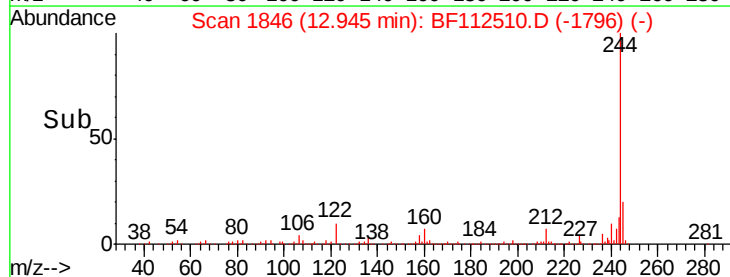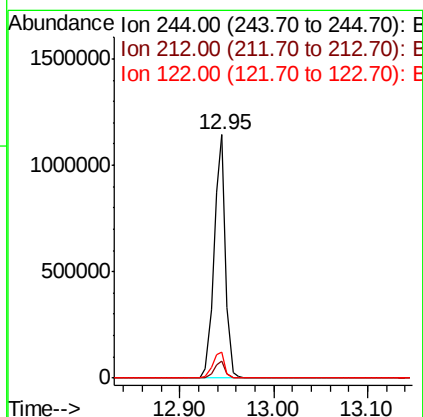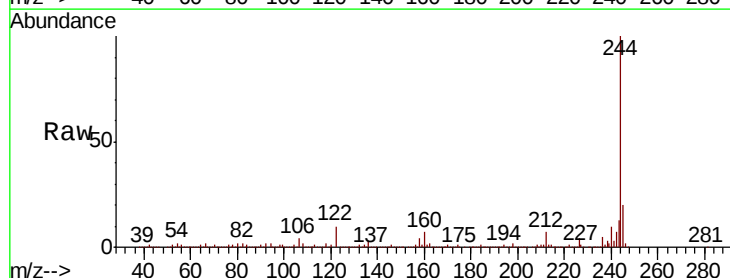

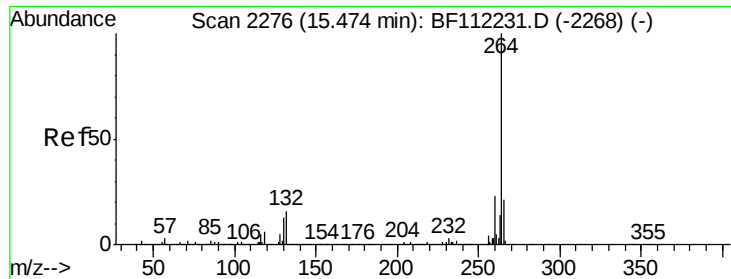

#87
Perylene-d12
Concen: 20.000 ng
RT: 15.49 min Scan# 2278
Delta R.T. 0.01 min
Lab File: BF112510.D
Acq: 12 Feb 2019 14:41

Instrument :
BNA_F
ClientSampleId :
M-10-D

Tgt Ion	Ratio	Lower	Upper
264	100		
260	22.3	18.2	27.2
265	21.4	17.0	25.4

