
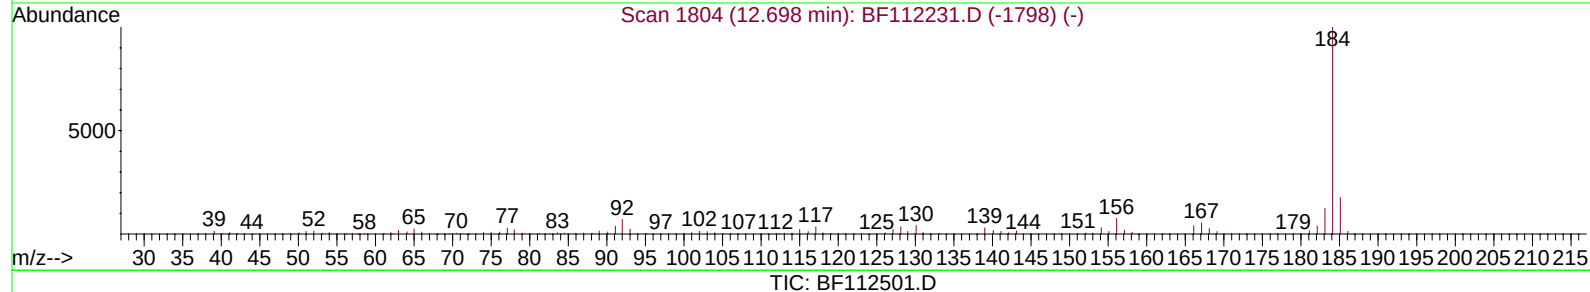
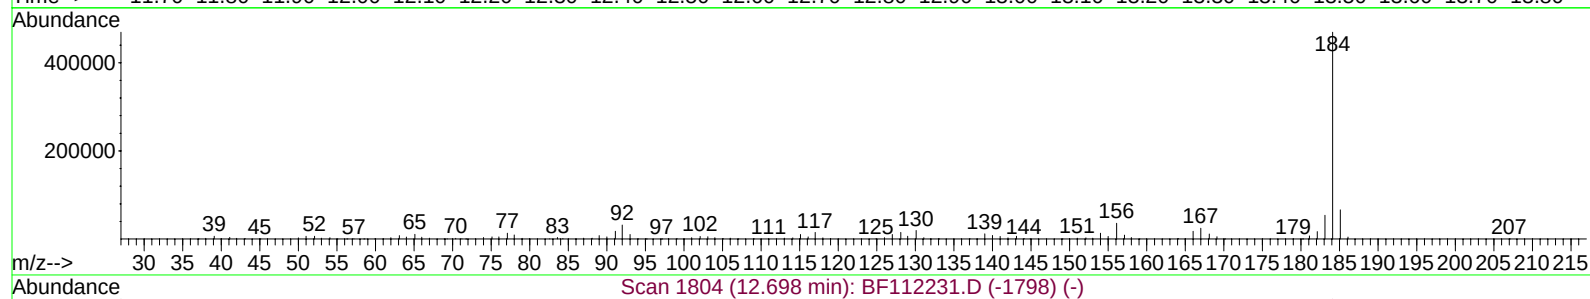


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF021219\
 Data File : BF112501.D
 Acq On : 12 Feb 2019 9:40
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 10:14:28 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 10:38:18 2019
 Response via : Initial Calibration

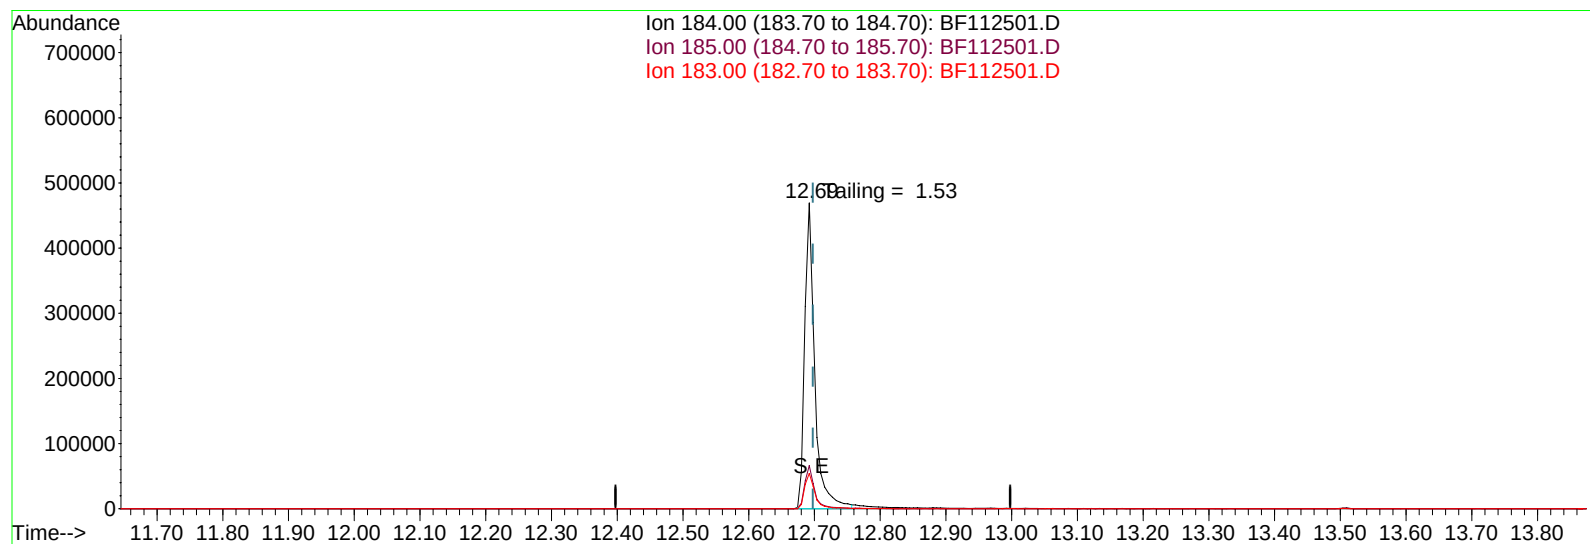

(77) Benzidine




12.692min (-0.006) 45112.54ng

response 514044

Ion	Exp%	Act%
184.00	100	100
185.00	17.40	14.16
183.00	12.50	11.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF021219\
Data File : BF112501.D
Acq On : 12 Feb 2019 9:40
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 10:14:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

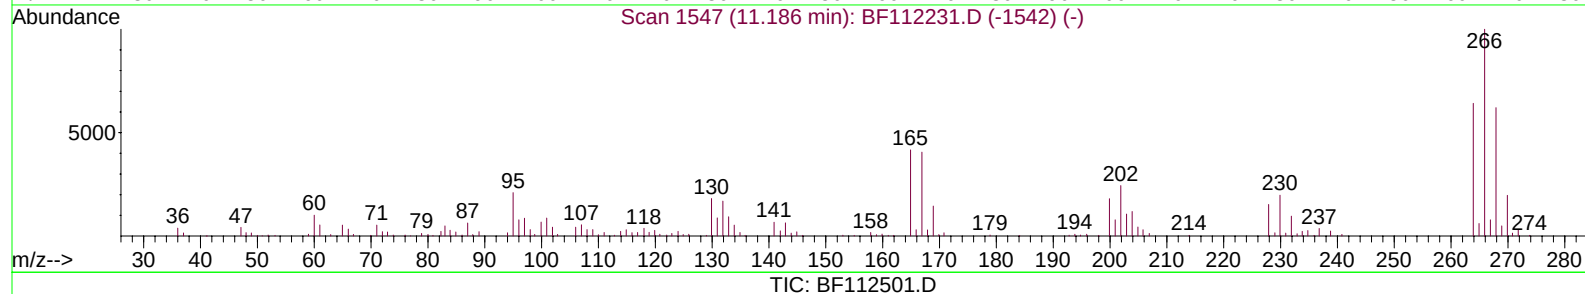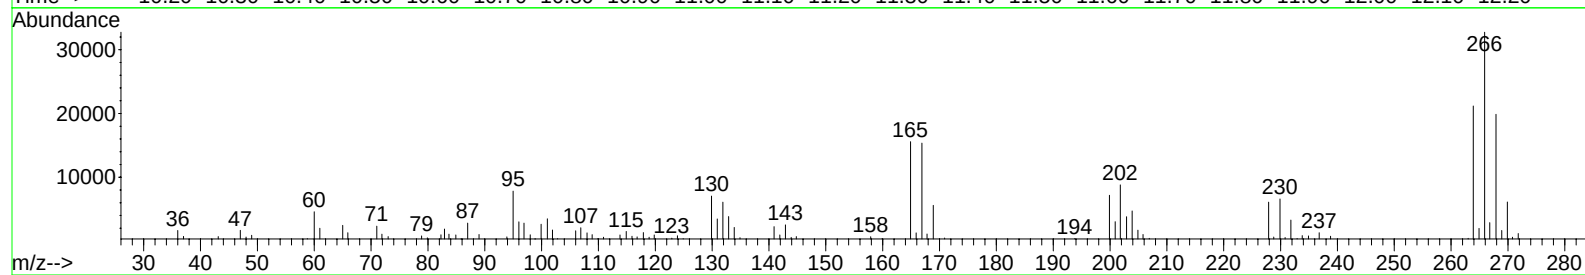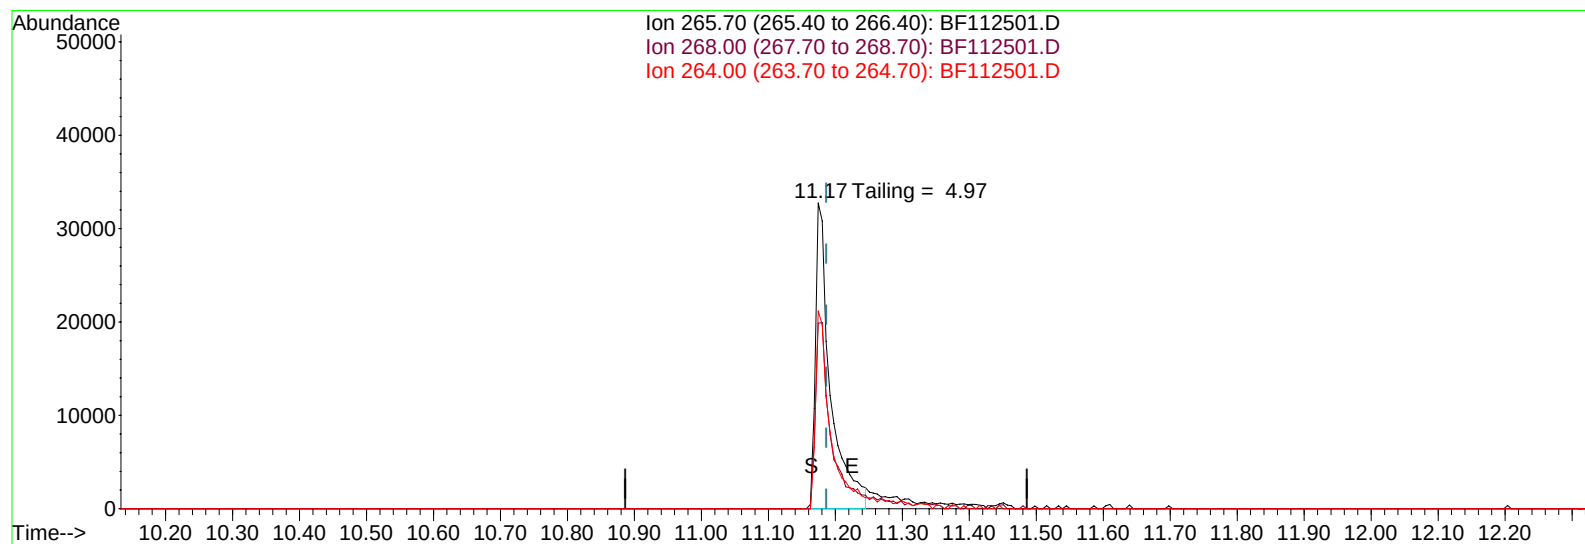

(70) Pentachlorophenol (C)

11.174min (-0.012) 34657.04ng

response 56665

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	60.69
264.00	63.60	64.67
0.00	0.00	0.00