


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF021219\
 Data File : BF112501.D
 Acq On : 12 Feb 2019 9:40
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 28 10:38:18 2019

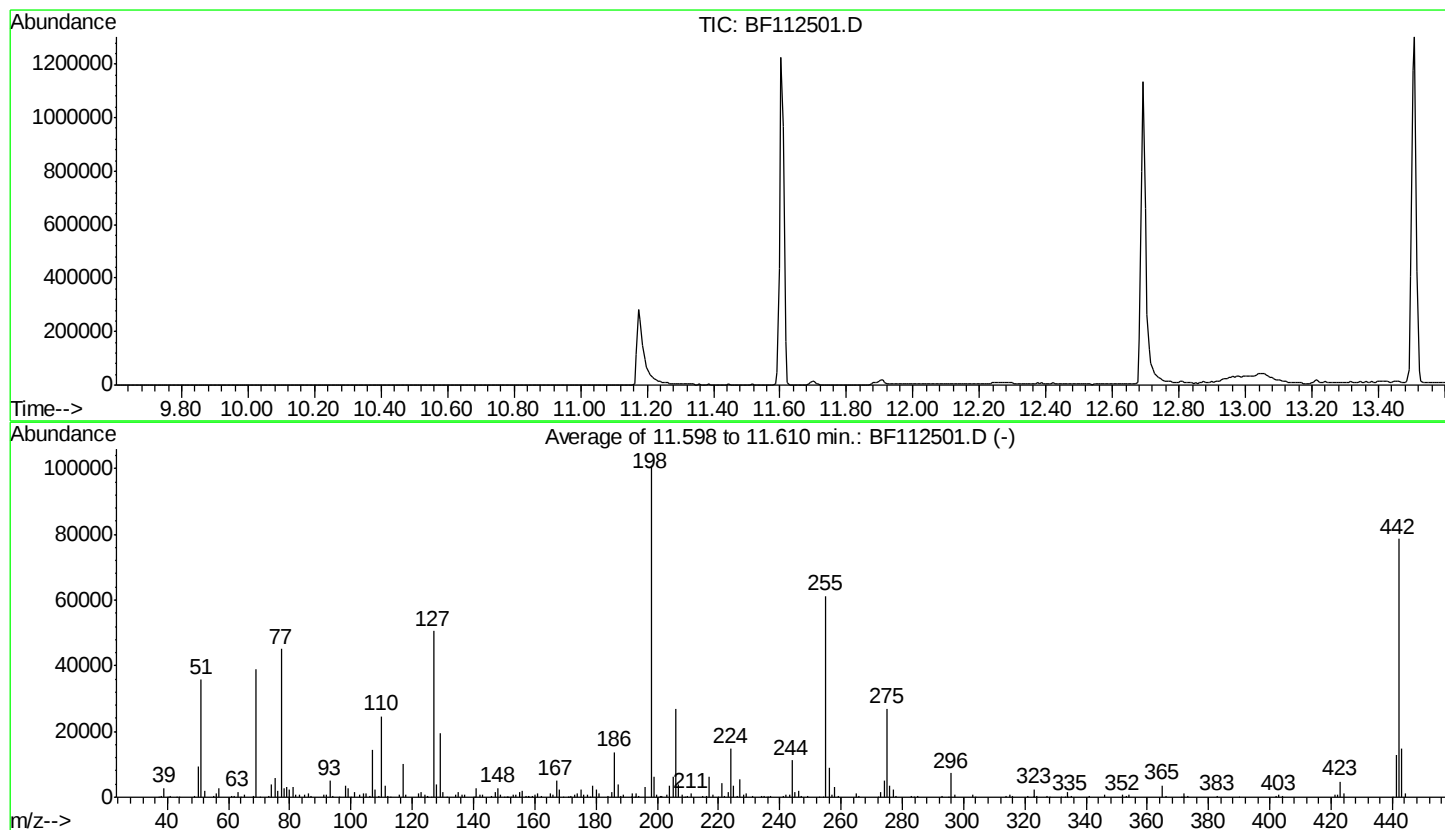

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	35674	PASS
68	69	0.00	2	1.3	517	PASS
69	198	0.00	100	38.5	38877	PASS
70	69	0.00	2	0.4	151	PASS
127	198	10	80	50.1	50517	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	100922	PASS
199	198	5	9	6.3	6383	PASS
275	198	10	60	26.8	27057	PASS
365	198	1	100	3.6	3634	PASS
441	198	0.01	100	12.6	12749	PASS
442	198	50	100	77.8	78562	PASS
443	442	15	24	18.9	14832	PASS