


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021220\  
 Data File : BF118908.D  
 Acq On : 12 Feb 2020 9:52  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF020320.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Feb 03 16:26:03 2020

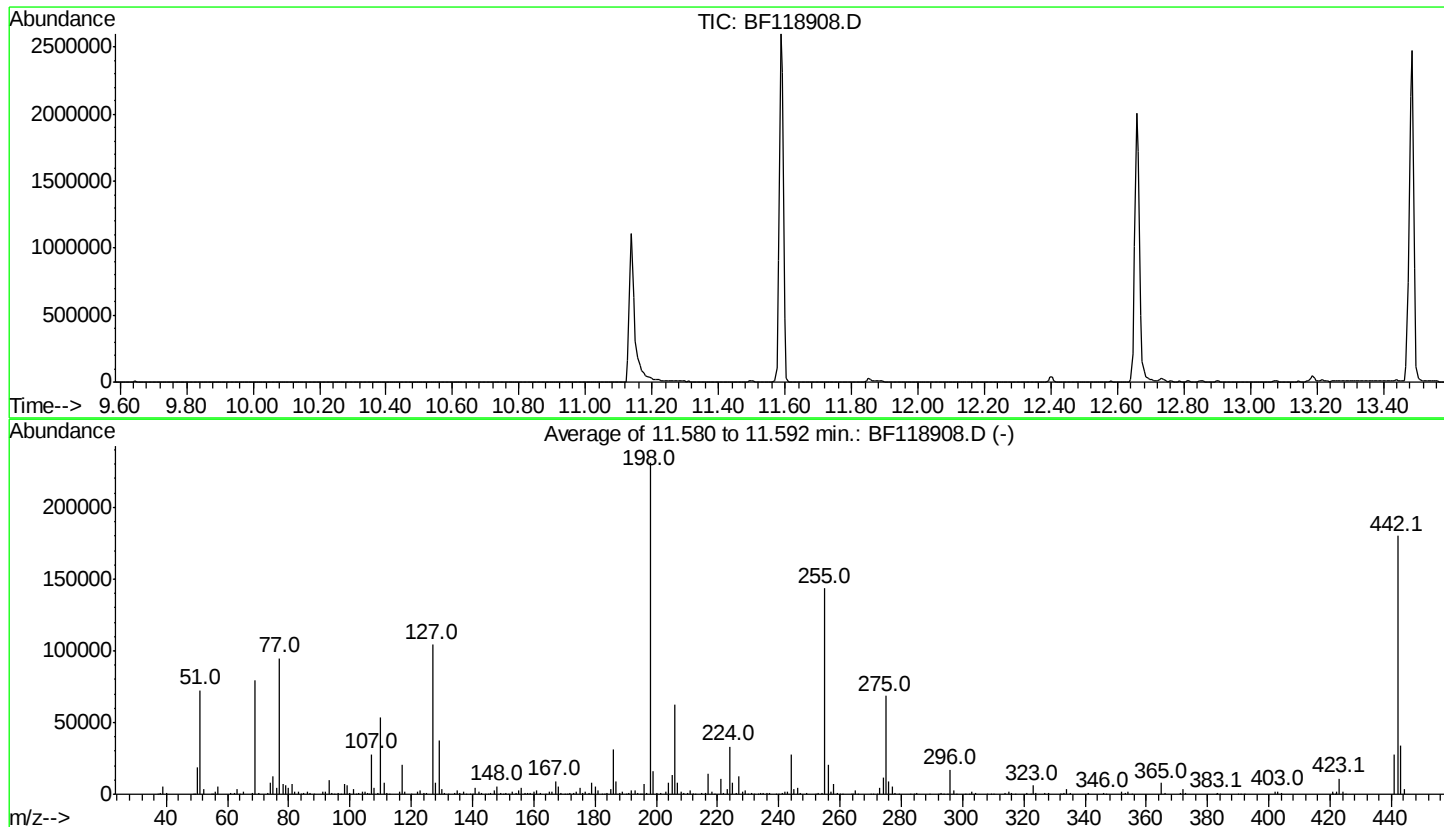

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 31.4      | 72536   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.3       | 1076    | PASS             |
| 69          | 198          | 0.00         | 100          | 34.5      | 79813   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 495     | PASS             |
| 127         | 198          | 10           | 80           | 45.1      | 104224  | PASS             |
| 197         | 198          | 0.00         | 2            | 0.4       | 855     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 231144  | PASS             |
| 199         | 198          | 5            | 9            | 6.9       | 15962   | PASS             |
| 275         | 198          | 10           | 60           | 29.7      | 68706   | PASS             |
| 365         | 198          | 1            | 100          | 3.4       | 7948    | PASS             |
| 441         | 198          | 0.01         | 100          | 12.1      | 27953   | PASS             |
| 442         | 198          | 50           | 100          | 77.8      | 179850  | PASS             |
| 443         | 442          | 15           | 24           | 18.9      | 34057   | PASS             |