
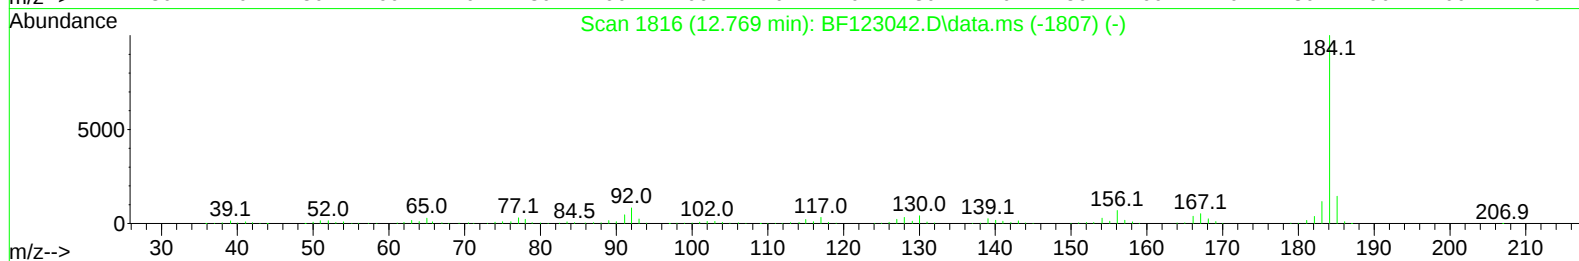
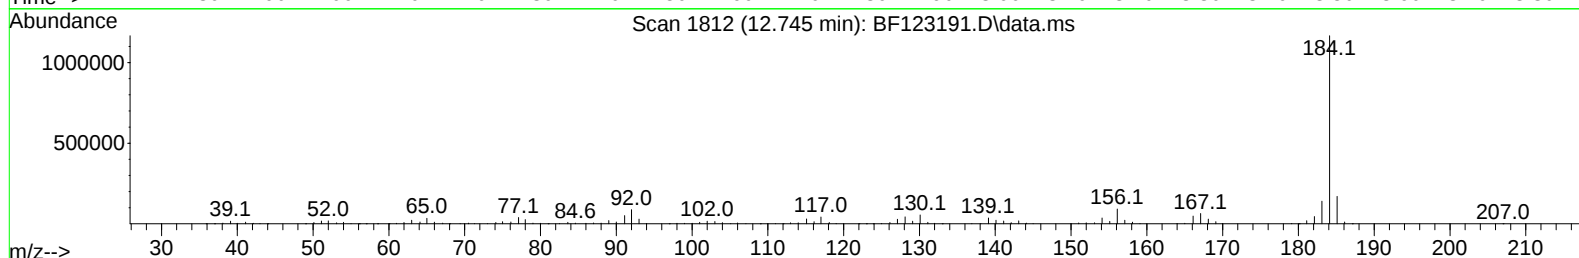


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021221\
Data File : BF123191.D
Acq On : 12 Feb 2021 11:37
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 12:24:43 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 12 12:13:40 2021
Response via : Initial Calibration

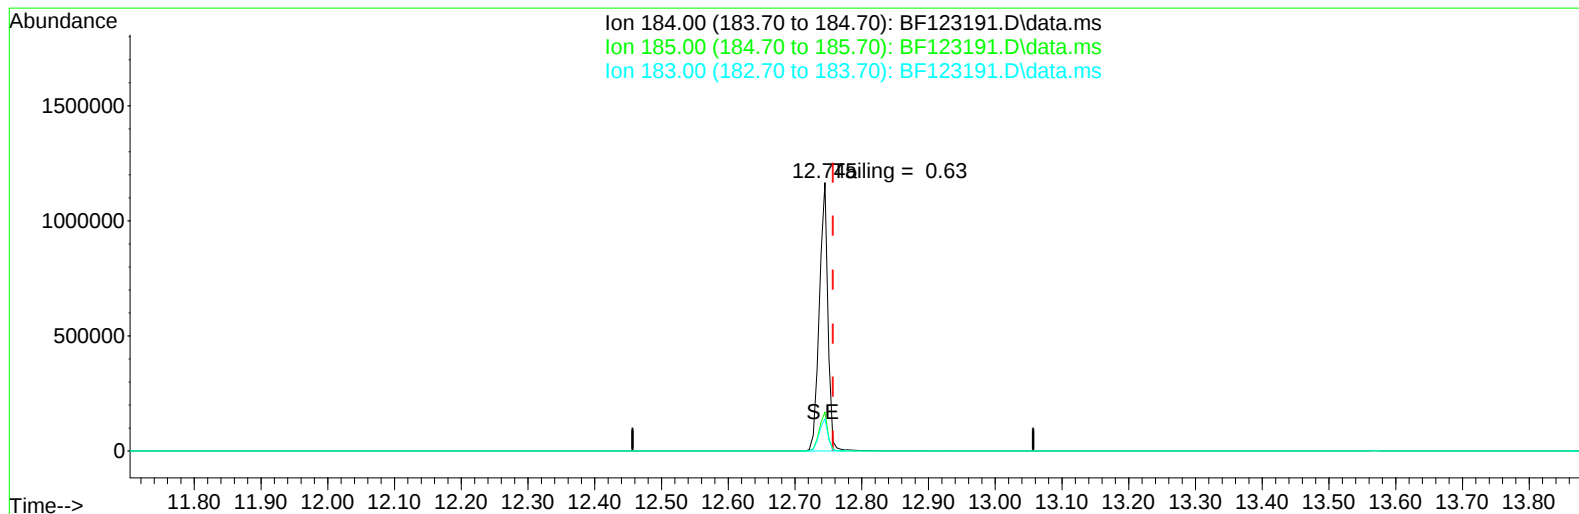

TIC: BF123191.D\data.ms

(77) Benzidine




12.745min (-0.012) 0.00 ng

response 1044070

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.55
183.00	12.10	12.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021221\
Data File : BF123191.D
Acq On : 12 Feb 2021 11:37
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 12:24:43 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 12 12:13:40 2021
Response via : Initial Calibration

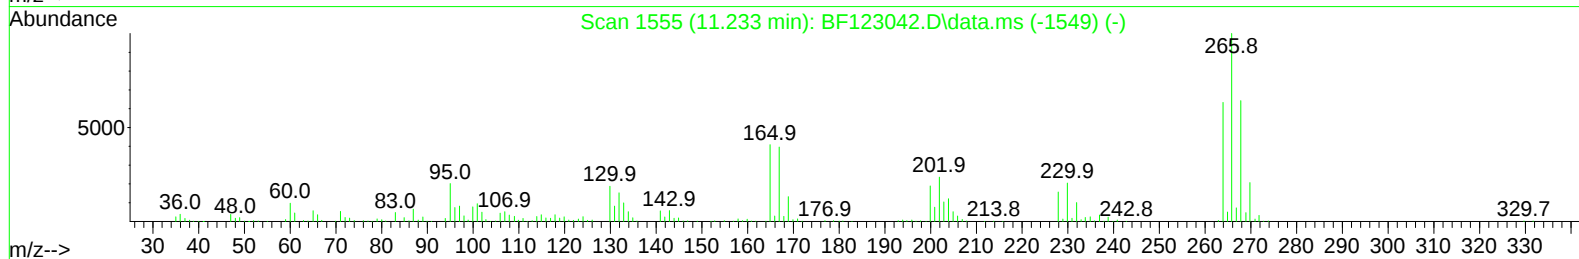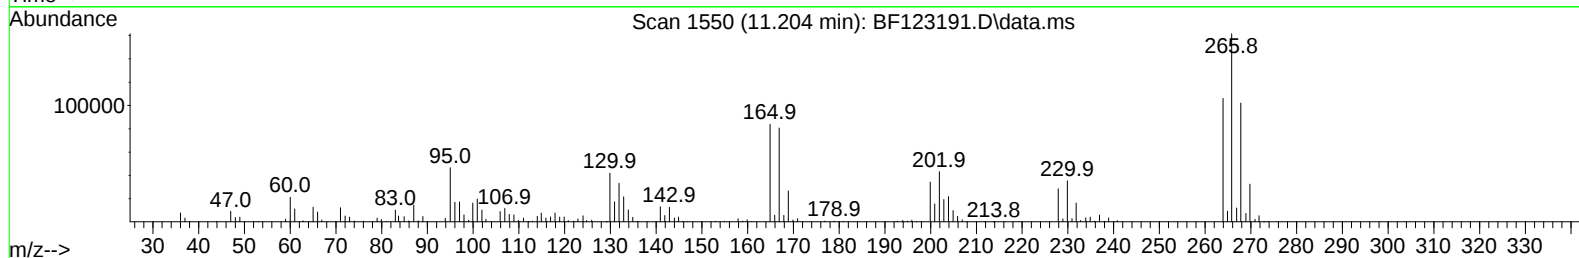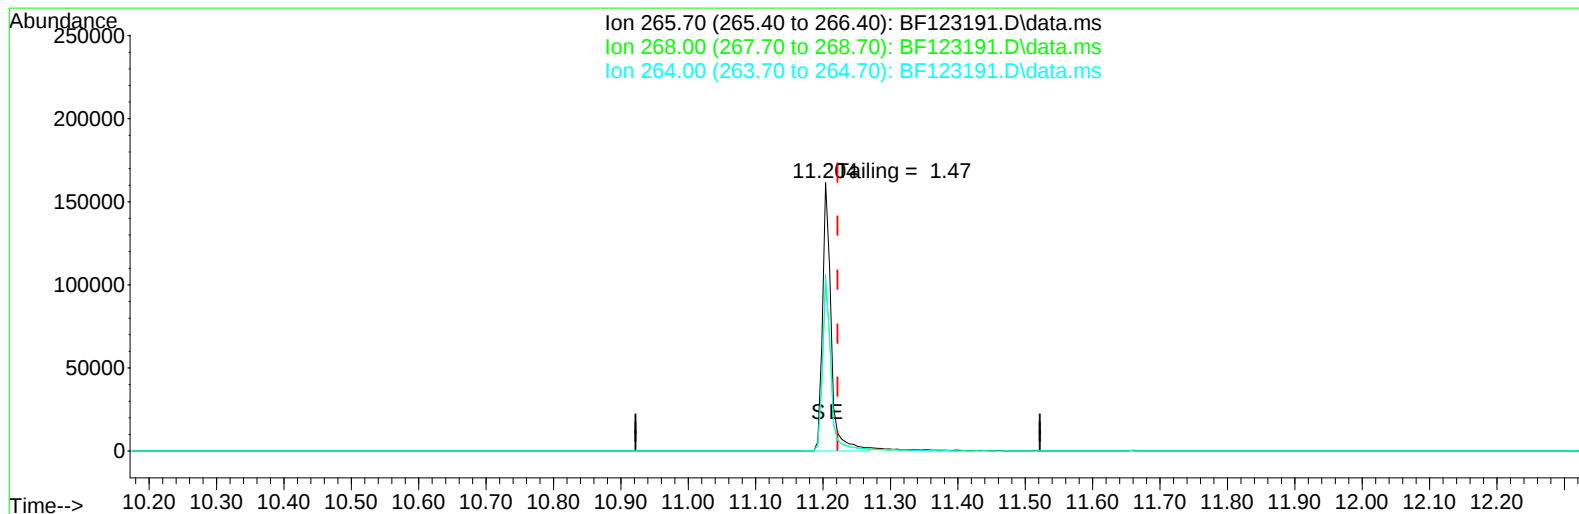

TIC: BF123191.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.018) 34707.44 ng

response 148000

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.21
264.00	62.30	65.72
0.00	0.00	0.00