


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021221\
 Data File : BF123191.D
 Acq On : 12 Feb 2021 11:37
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 12 16:59:49 2021

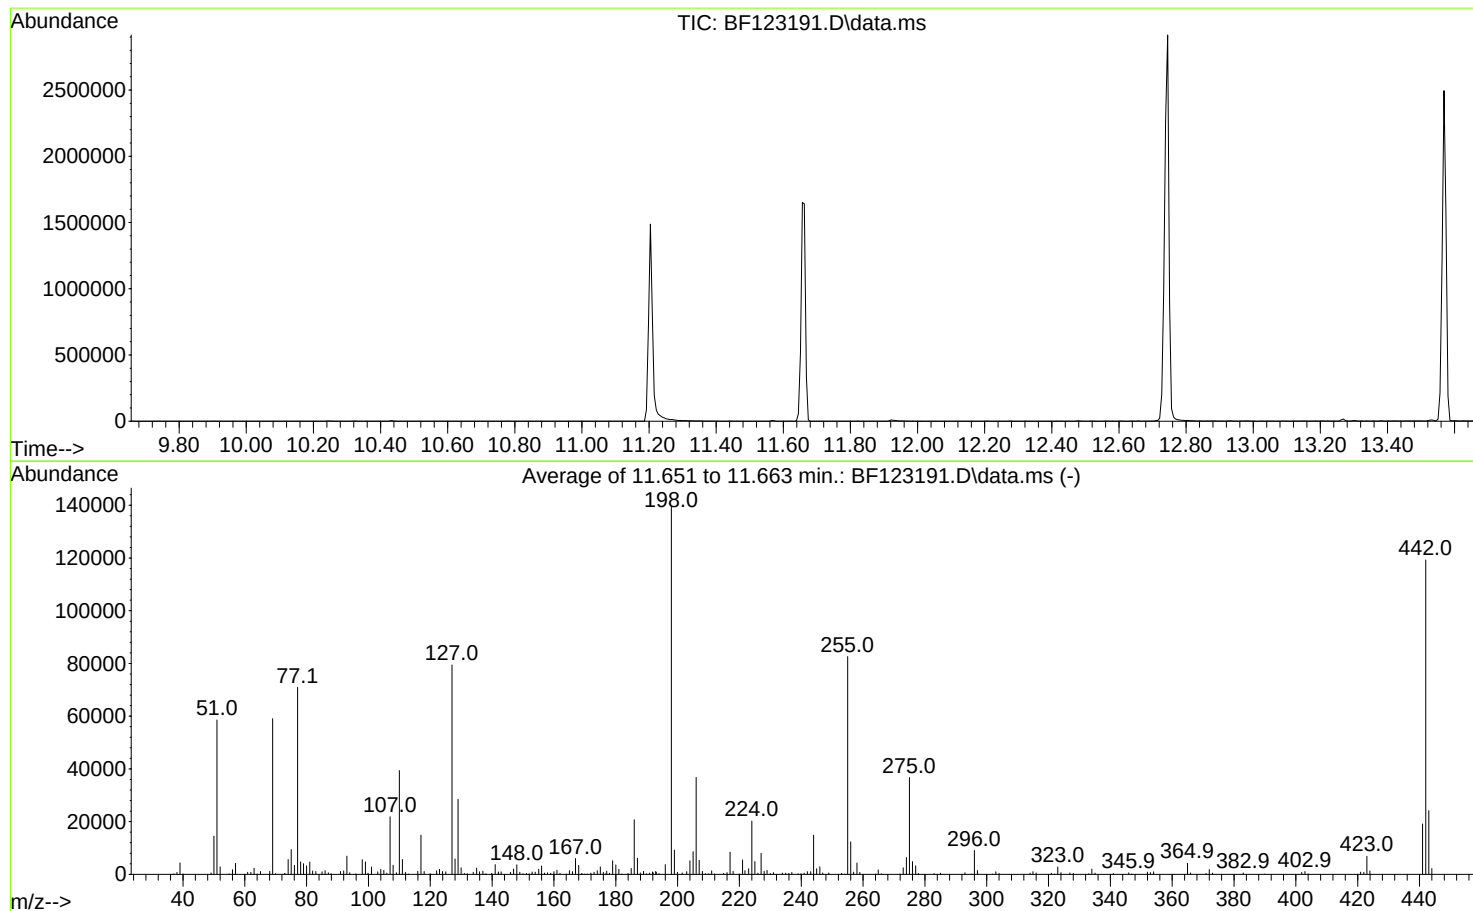

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	58568	PASS
68	69	0.00	2	1.9	1135	PASS
69	198	0.00	100	42.3	59043	PASS
70	69	0.00	2	0.5	304	PASS
127	198	10	80	56.9	79448	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	139528	PASS
199	198	5	9	6.6	9220	PASS
275	198	10	60	26.3	36743	PASS
365	198	1	100	3.0	4203	PASS
441	198	0.01	100	13.7	19108	PASS
442	442	50	100	100.0	119235	PASS
443	442	15	24	20.3	24168	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/12/2021	BNA_F	<u>BF123191.D</u>
Compound Name	Response	Retention Time
DDT	381627	13.56
DDD	3493	13.26
DDE	462	12.93
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3955	385582	1.03

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021221\
 Data File : BF123191.D
 Acq On : 12 Feb 2021 11:37
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 12 12:24:43 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 12 12:13:40 2021
 Response via : Initial Calibration

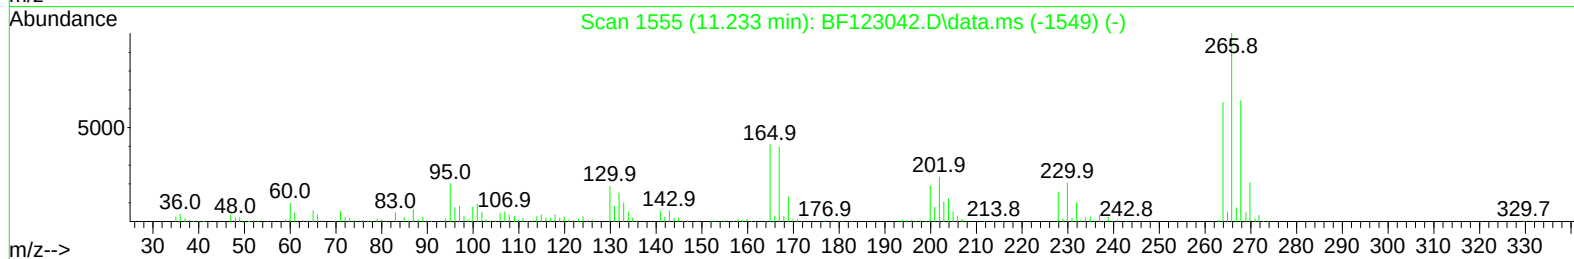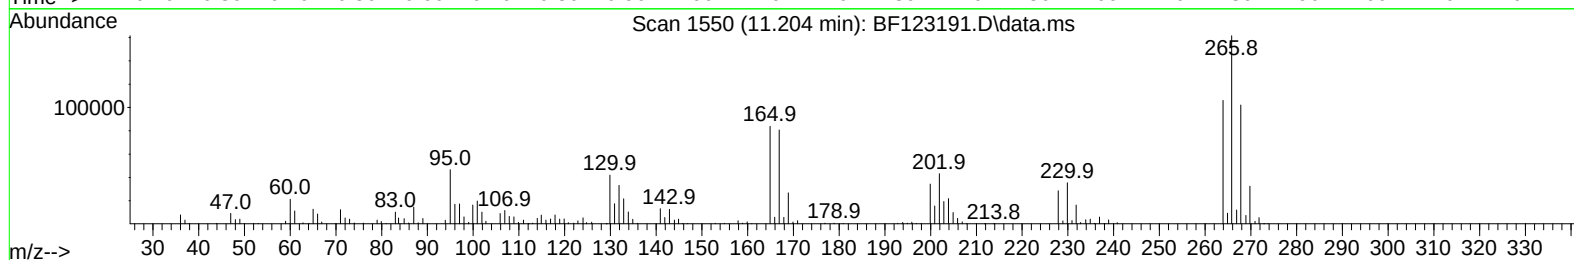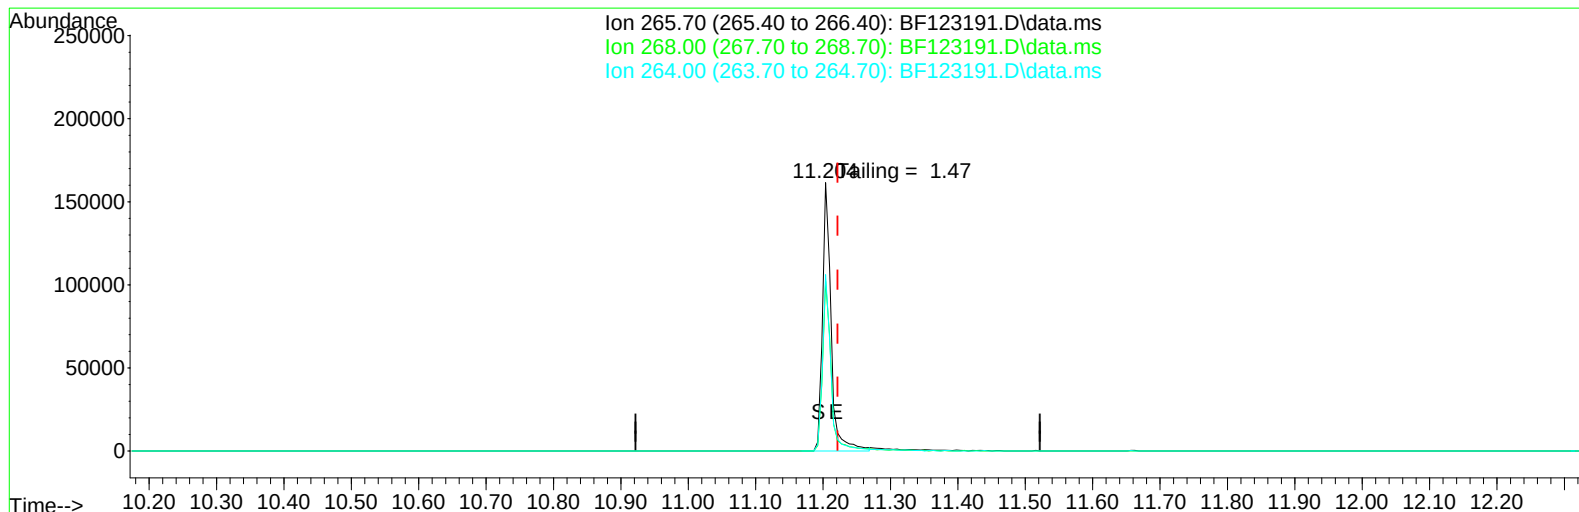

TIC: BF123191.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.018) 34707.44 ng




response 148000

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.21
264.00	62.30	65.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021221\
Data File : BF123191.D
Acq On : 12 Feb 2021 11:37
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 12 12:24:43 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 12 12:13:40 2021
Response via : Initial Calibration

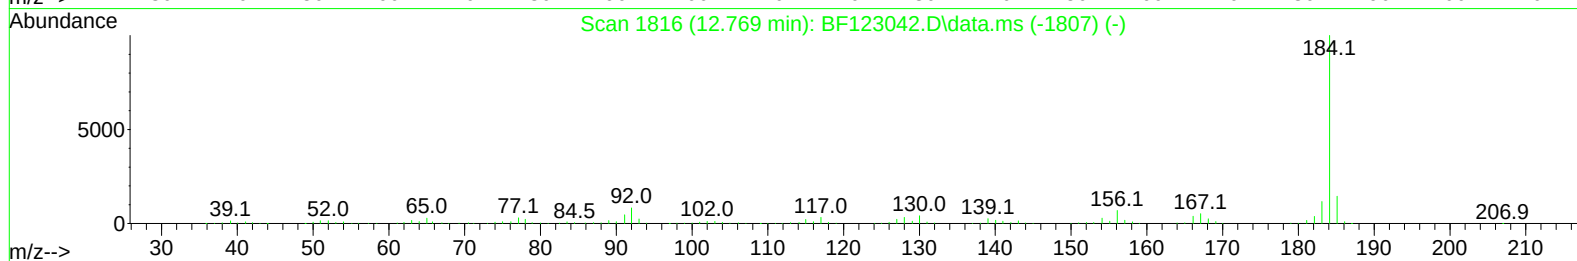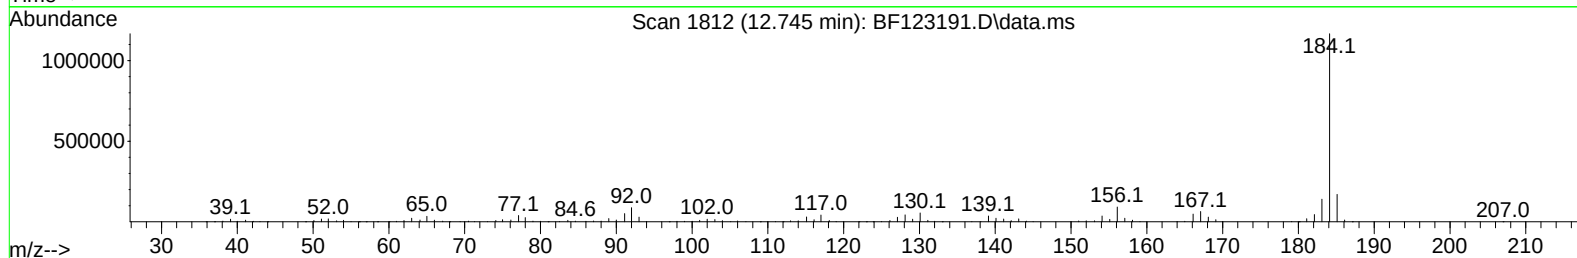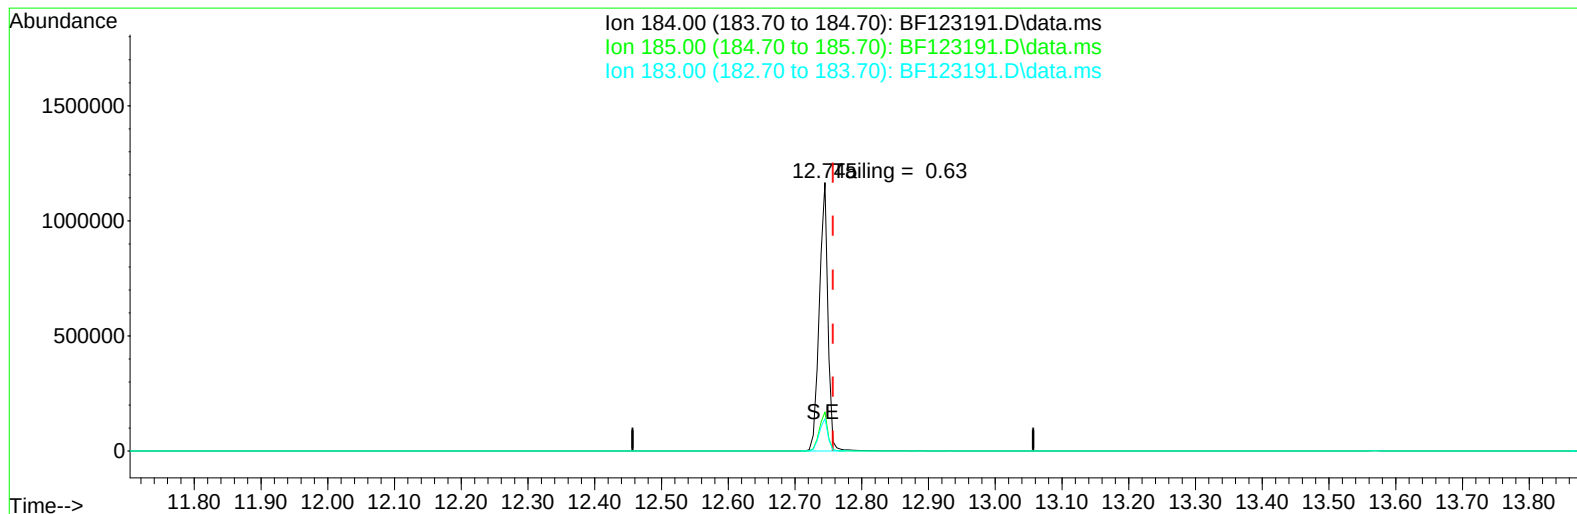

TIC: BF123191.D\data.ms

(77) Benzidine

12.745min (-0.012) 0.00 ng

response 1044070

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.55
183.00	12.10	12.07
0.00	0.00	0.00