
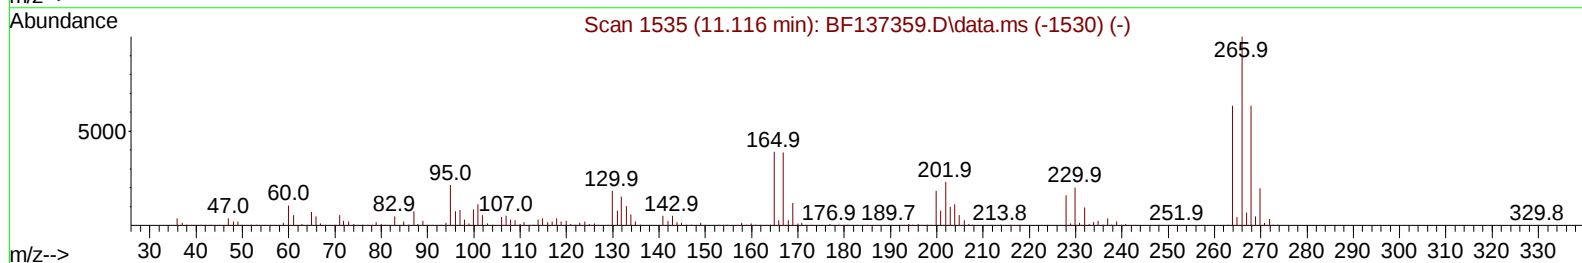
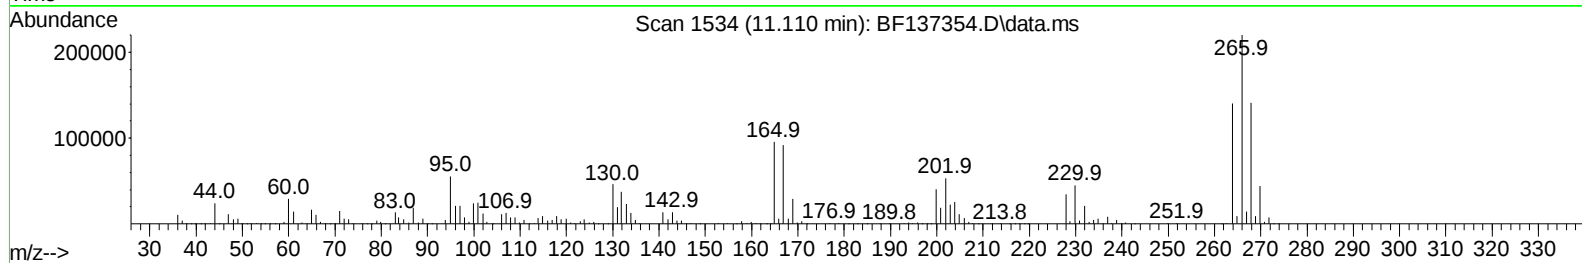


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021224\
Data File : BF137354.D
Acq On : 12 Feb 2024 14:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 02:56:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 13 02:26:13 2024
Response via : Initial Calibration

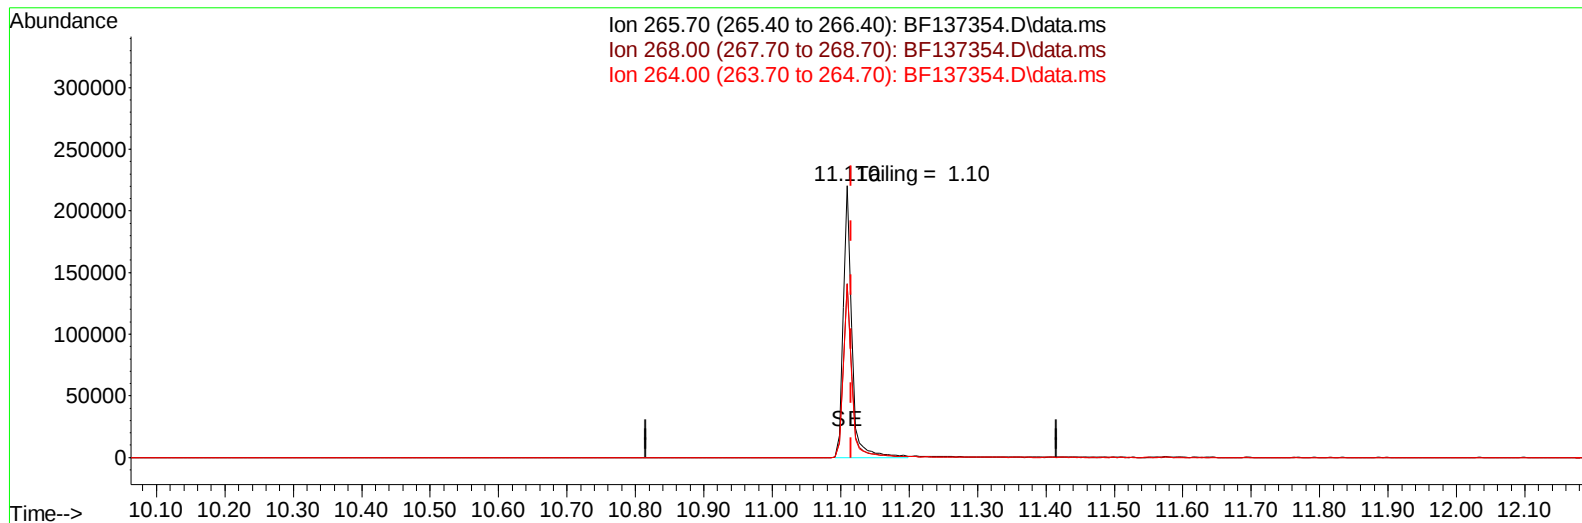




TIC: BF137354.D\data.ms

(70) Pentachlorophenol (C)**11.110min (-0.006) 375768.16 ng****response 189407**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.05
264.00	63.50	63.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021224\
Data File : BF137354.D
Acq On : 12 Feb 2024 14:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 02:56:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 13 02:26:13 2024
Response via : Initial Calibration

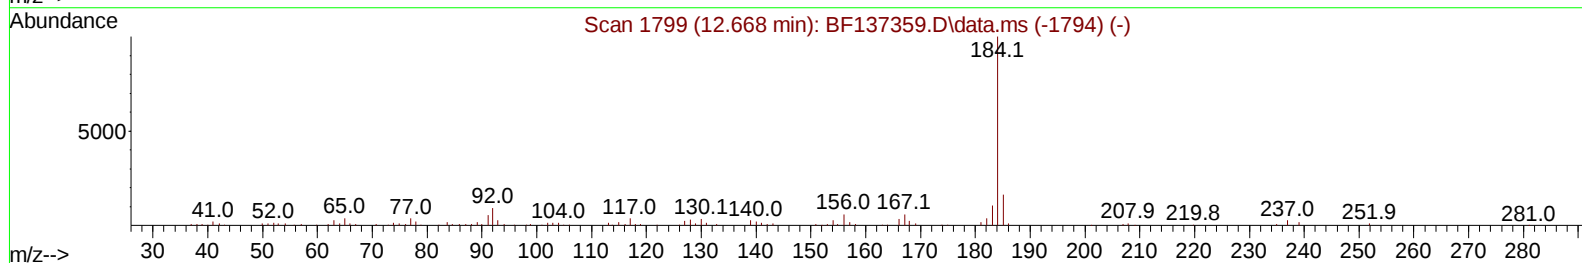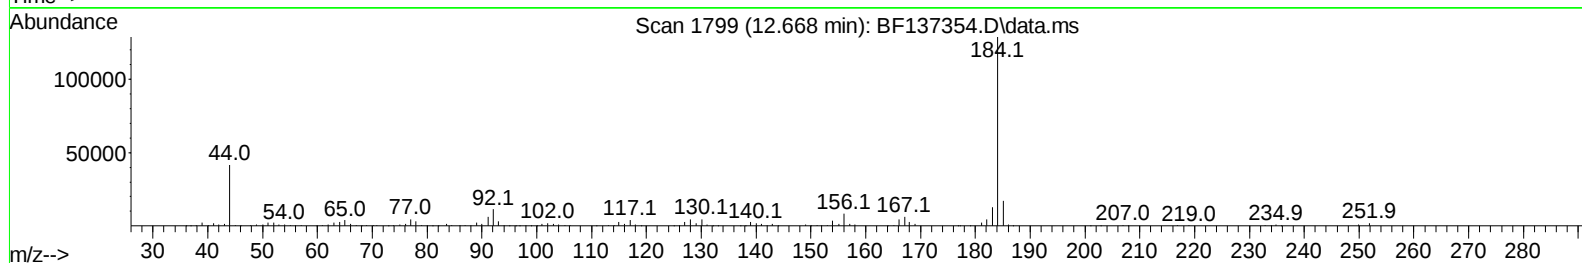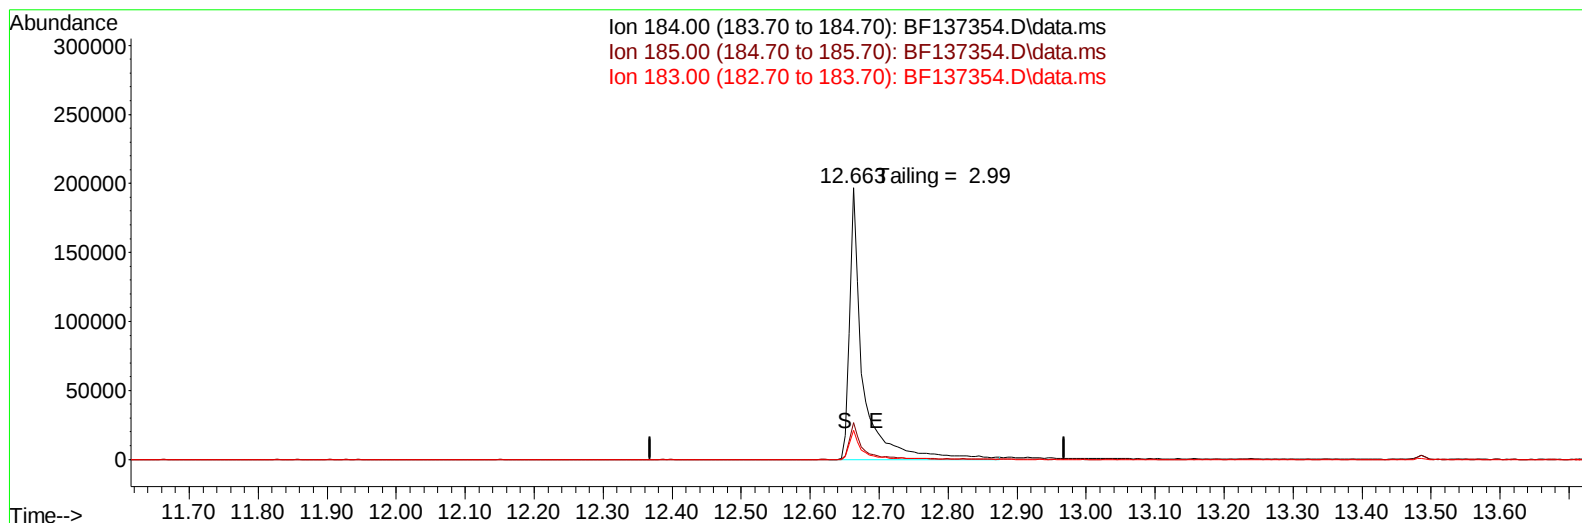

TIC: BF137354.D\data.ms

(77) Benzidine**12.668min (-12.668) 0.00 ng****response 0**

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	16.40	0.00#
183.00	10.40	0.00#
0.00	0.00	0.00