


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021224\
Data File : BF137354.D
Acq On : 12 Feb 2024 14:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 13 02:26:13 2024

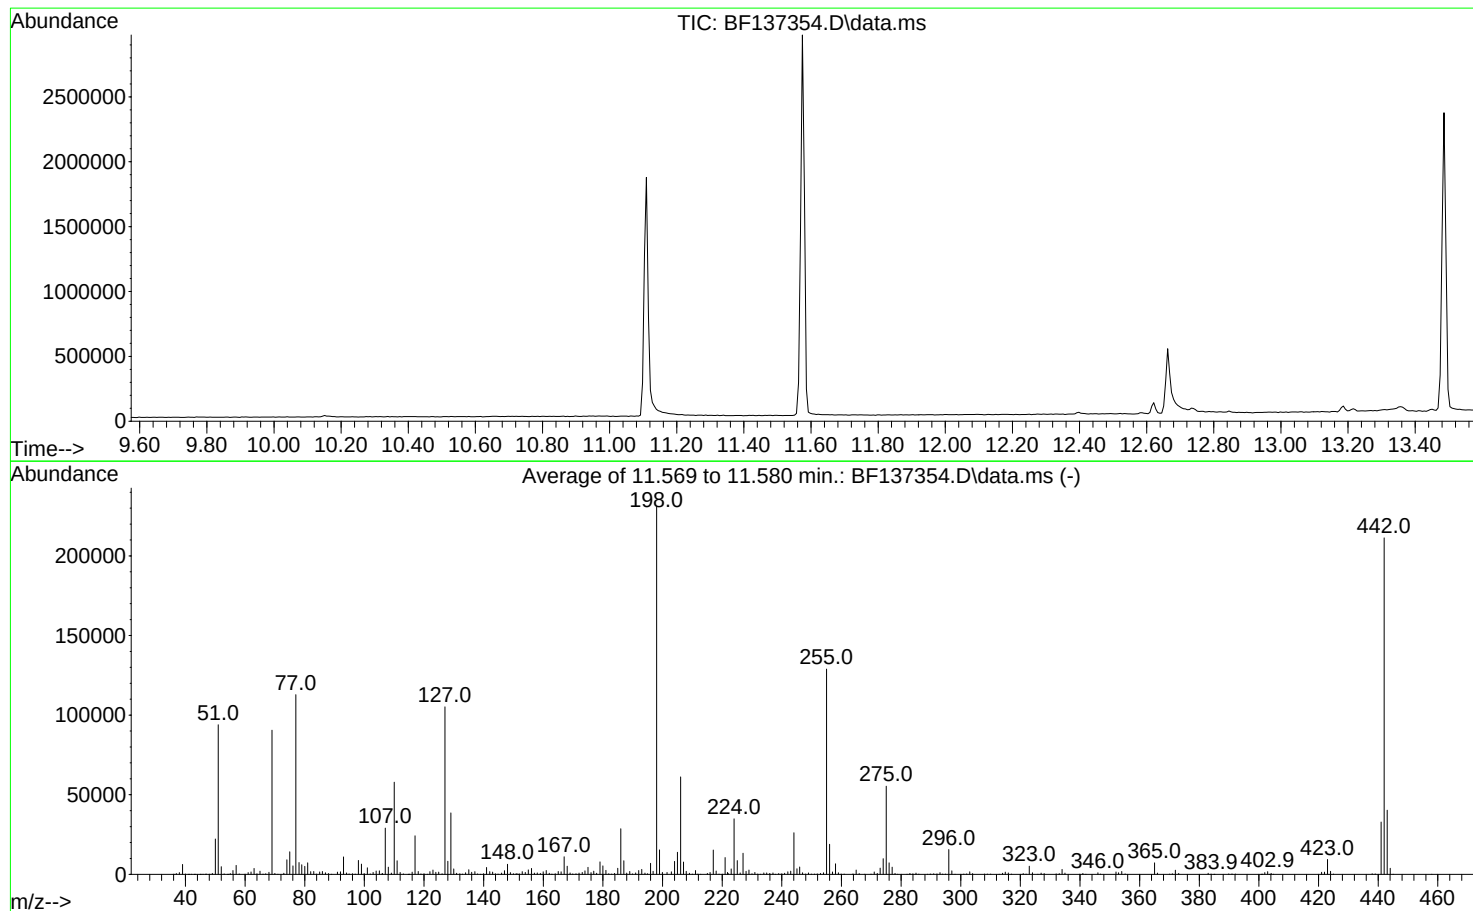




AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	93952	PASS
68	69	0.00	2	1.4	1282	PASS
69	198	0.00	100	39.2	90523	PASS
70	69	0.00	2	0.7	633	PASS
127	198	10	80	45.5	105216	PASS
197	198	0.00	2	0.8	1921	PASS
198	198	100	100	100.0	231040	PASS
199	198	5	9	6.7	15420	PASS
275	198	10	60	24.0	55384	PASS
365	198	1	100	3.1	7209	PASS
441	198	0.01	100	14.2	32913	PASS
442	442	50	100	100.0	211331	PASS
443	442	15	24	19.1	40287	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021224\
Data File : BF137354.D
Acq On : 12 Feb 2024 14:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 13 02:56:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 13 02:26:13 2024
Response via : Initial Calibration

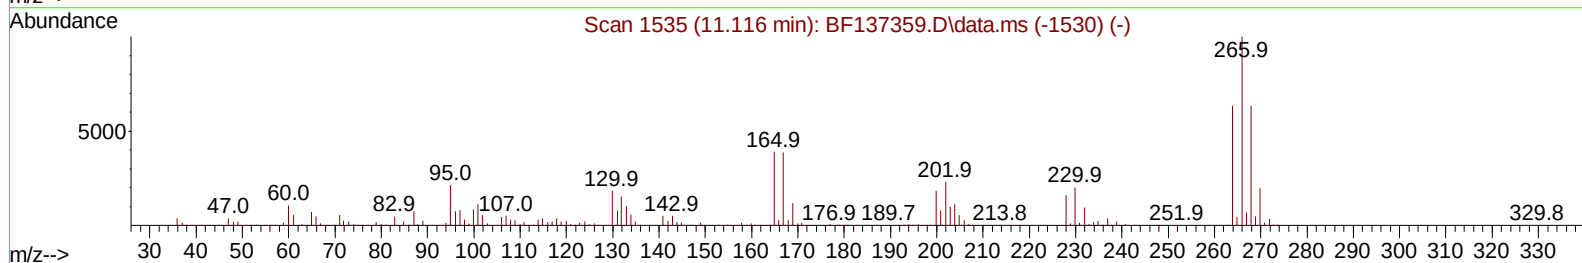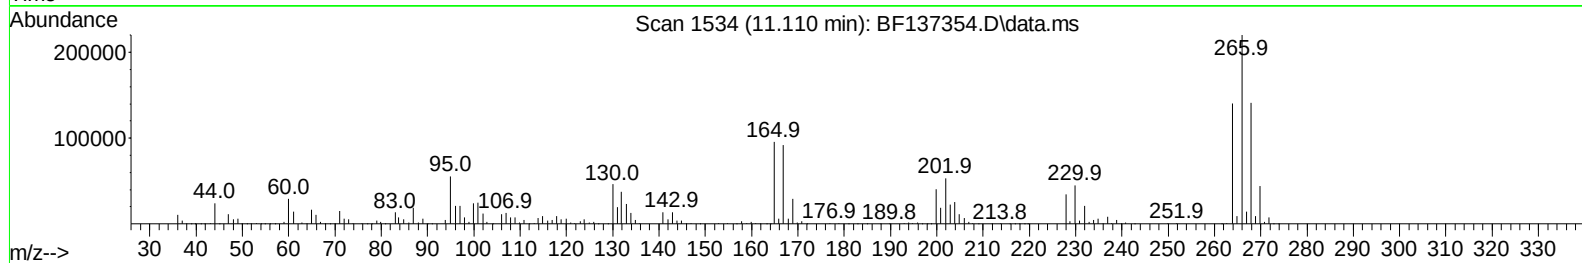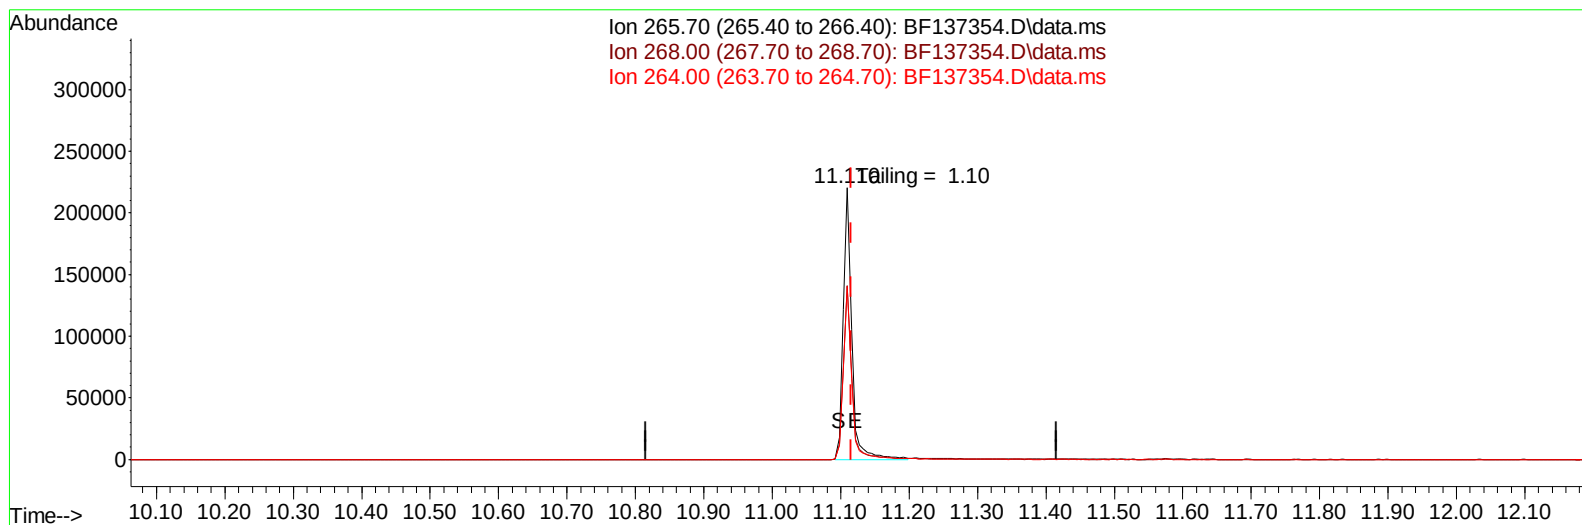

TIC: BF137354.D\data.ms

(70) Pentachlorophenol (C)

11.110min (-0.006) 375768.16 ng




response 189407

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.05
264.00	63.50	63.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021224\
Data File : BF137354.D
Acq On : 12 Feb 2024 14:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 13 02:56:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 13 02:26:13 2024
Response via : Initial Calibration

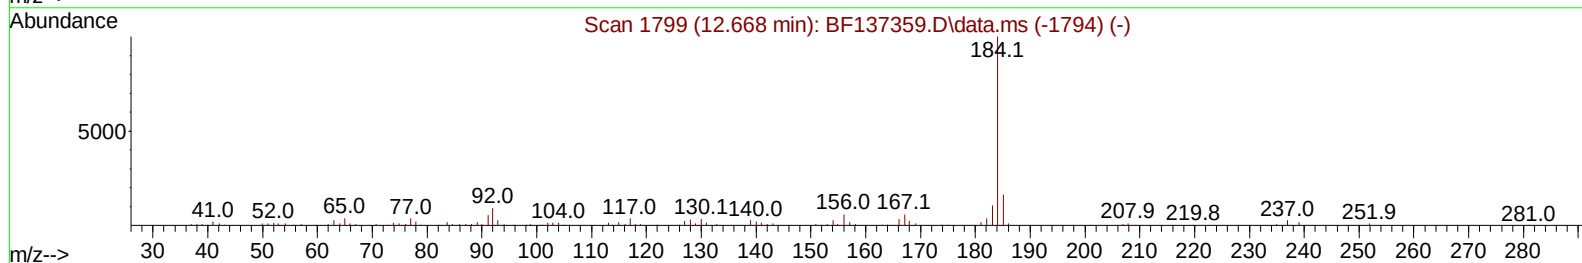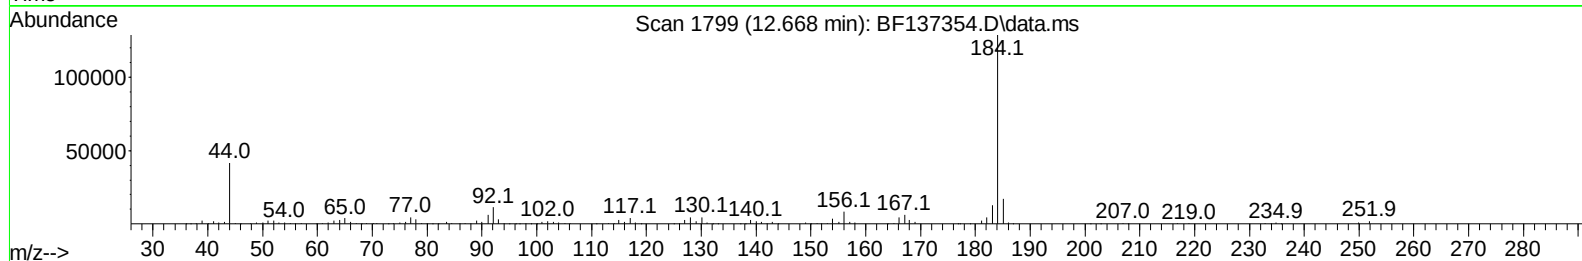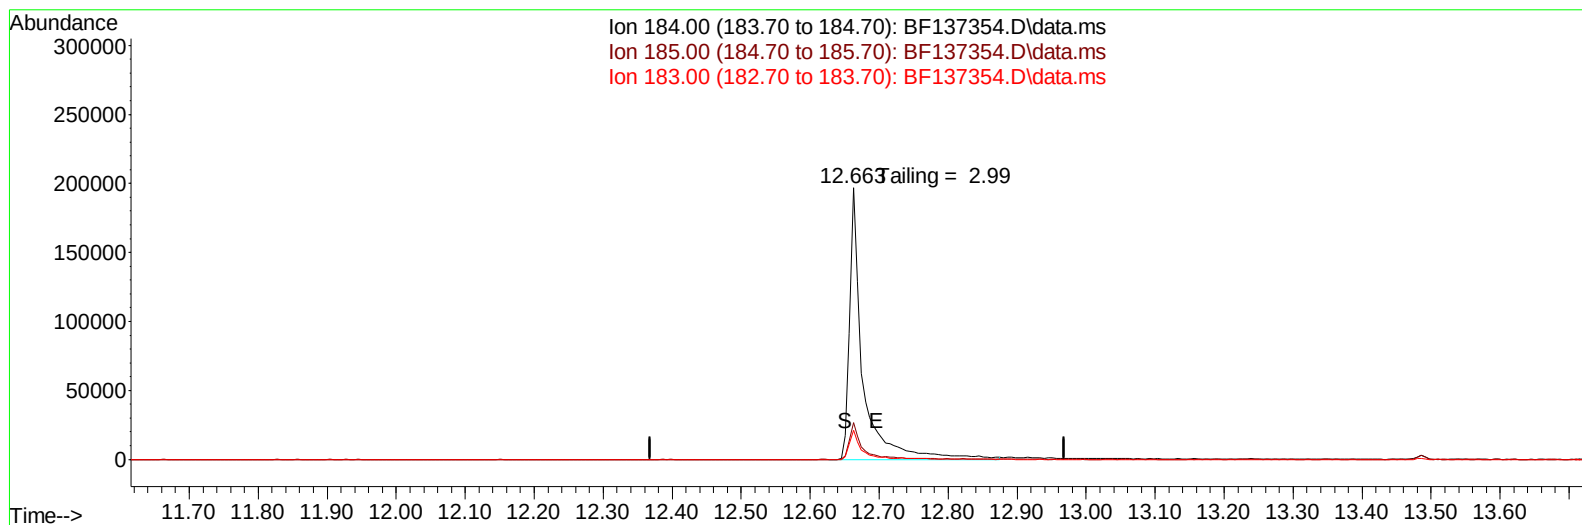

TIC: BF137354.D\data.ms

(77) Benzidine

12.668min (-12.668) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	16.40	0.00#
183.00	10.40	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/12/2024	BNA_F	<u>BF137354.D</u>
Compound Name	Response	Retention Time
DDT	255532	13.486
DDD	7783	13.186
DDE	1021	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8804	264336	3.33

Instrument :
BNA_F
ClientSampleId :
DFTPP