

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021225\
 Data File : BF141578.D
 Acq On : 12 Feb 2025 09:59
 Operator : RC/JU
 Sample : PB166665BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB166665BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141578.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.416	560	565	587	rBV	2107599	2926107	72.22%	13.196%
2	6.428	731	737	768	rBV	2107466	2980100	73.55%	13.440%
3	6.787	793	798	809	rBV	447024	550489	13.59%	2.483%
4	7.351	887	894	910	rBV	1387497	1981618	48.91%	8.937%
5	8.069	1010	1016	1028	rBV	524613	725549	17.91%	3.272%
6	9.145	1192	1199	1204	rBV	2664574	3608938	89.07%	16.276%
7	9.822	1308	1314	1333	rVB	647467	838654	20.70%	3.782%
8	10.616	1442	1449	1473	rBV	1607511	2292236	56.57%	10.337%
9	11.310	1561	1567	1588	rBV	656127	883830	21.81%	3.986%
10	12.898	1831	1837	1842	rBV	3029585	4051734	100.00%	18.272%
11	13.951	2010	2016	2028	rBV	537176	727926	17.97%	3.283%
12	15.404	2257	2263	2280	rBV	333298	556509	13.74%	2.510%
13	16.845	2499	2508	2509	rBV7	21444	50346	1.24%	0.227%




Sum of corrected areas: 22174036

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021225\
Data File : BF141578.D
Acq On : 12 Feb 2025 09:59
Operator : RC/JU
Sample : PB166665BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166665BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

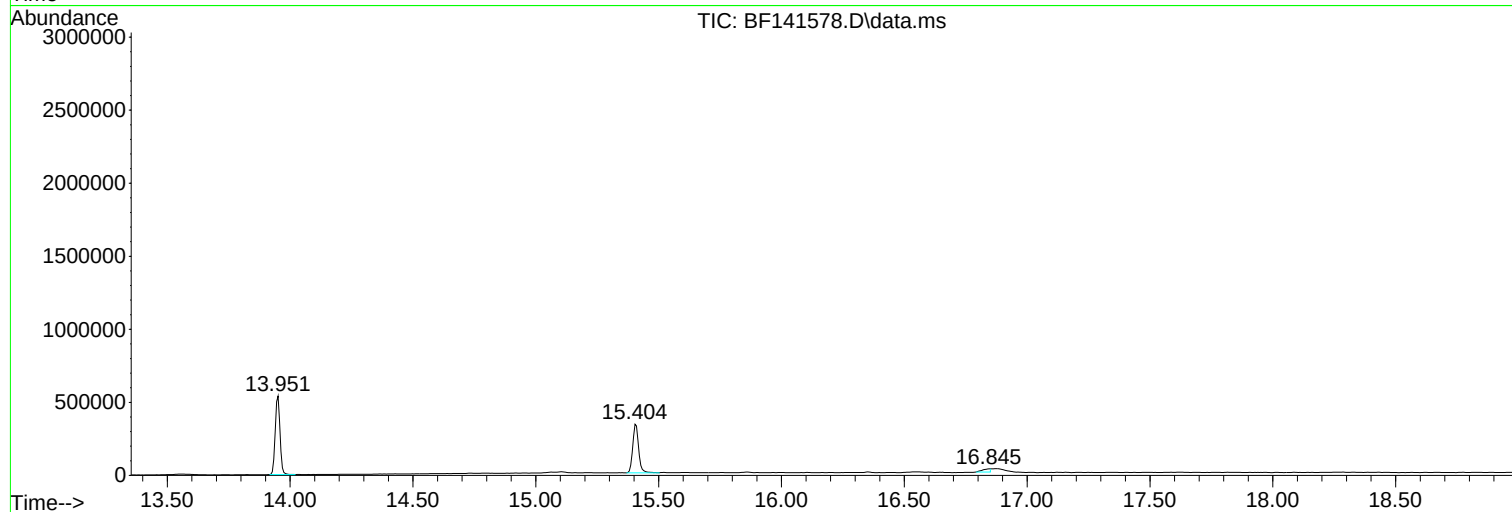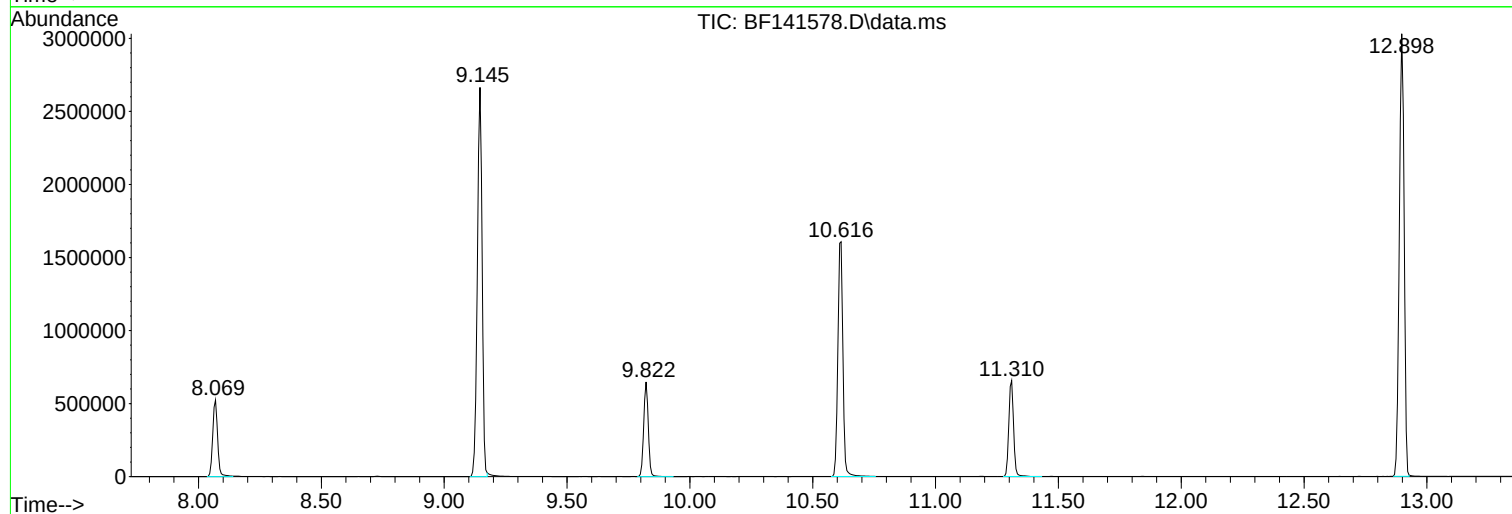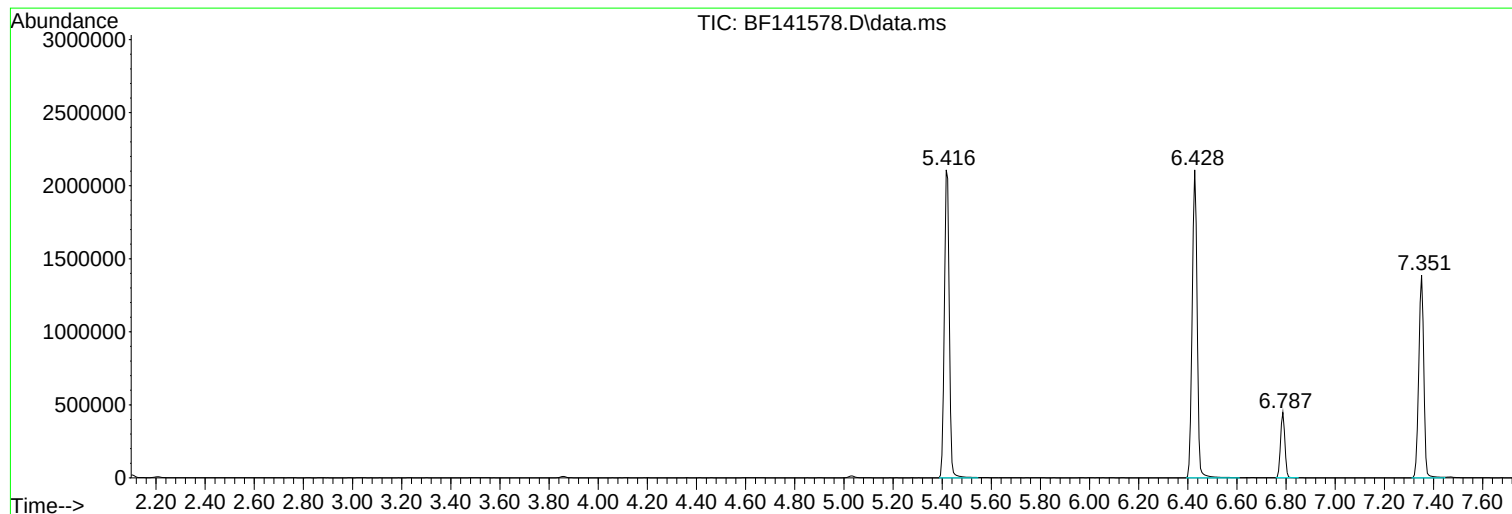

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021225\
Data File : BF141578.D
Acq On : 12 Feb 2025 09:59
Operator : RC/JU
Sample : PB166665BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166665BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021225\
Data File : BF141578.D
Acq On : 12 Feb 2025 09:59
Operator : RC/JU
Sample : PB166665BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166665BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------