

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021225\
Data File : BF141580.D
Acq On : 12 Feb 2025 10:51
Operator : RC/JU
Sample : PB166679BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166679BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141580.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.416	560	565	587	rBV	2081372	2851667	70.84%	13.022%
2	6.428	731	737	765	rBV	2036691	2901266	72.07%	13.249%
3	6.787	793	798	816	rVB	444075	556400	13.82%	2.541%
4	7.351	887	894	911	rBV	1322197	1928202	47.90%	8.805%
5	8.069	1010	1016	1030	rBV	531752	741737	18.43%	3.387%
6	9.145	1192	1199	1225	rBV	2594926	3576479	88.85%	16.332%
7	9.822	1308	1314	1330	rBV	652598	856542	21.28%	3.911%
8	10.616	1442	1449	1473	rBV	1601298	2271634	56.43%	10.374%
9	11.310	1561	1567	1589	rBV	673146	908757	22.57%	4.150%
10	12.898	1831	1837	1842	rBV	3018867	4025524	100.00%	18.383%
11	13.951	2010	2016	2029	rBV	535436	733181	18.21%	3.348%
12	15.404	2257	2263	2278	rBV	342332	546729	13.58%	2.497%




Sum of corrected areas: 21898118

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021225\
Data File : BF141580.D
Acq On : 12 Feb 2025 10:51
Operator : RC/JU
Sample : PB166679BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166679BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

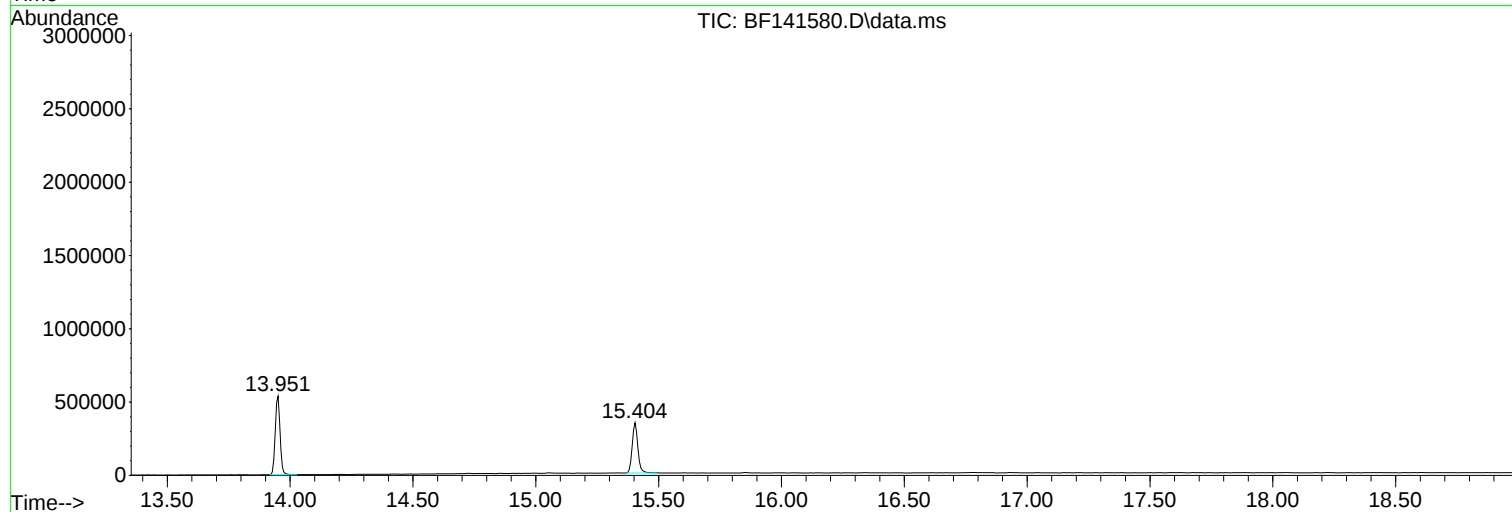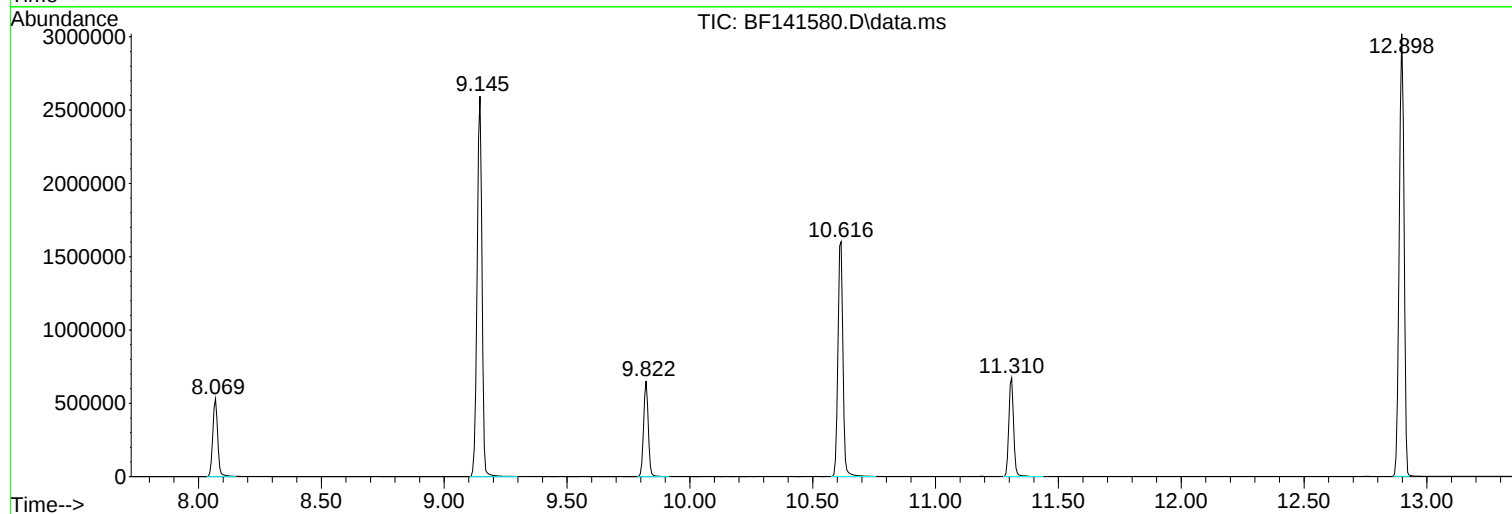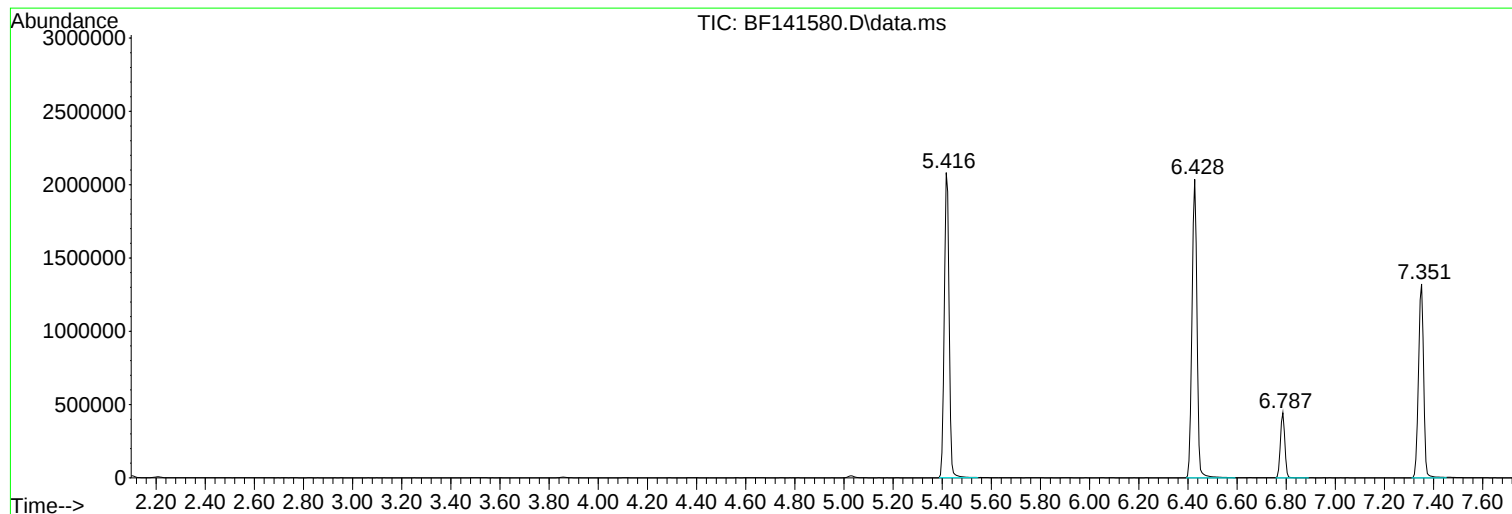

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021225\
Data File : BF141580.D
Acq On : 12 Feb 2025 10:51
Operator : RC/JU
Sample : PB166679BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166679BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021225\
Data File : BF141580.D
Acq On : 12 Feb 2025 10:51
Operator : RC/JU
Sample : PB166679BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166679BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------