

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021225\
Data File : BF141582.D
Acq On : 12 Feb 2025 11:43
Operator : RC/JU
Sample : PB166681BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166681BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141582.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.422	560	566	587	rBV	2149965	2990936	73.09%	13.113%
2	6.428	731	737	760	rBV	2134137	3036097	74.19%	13.311%
3	6.787	793	798	809	rVB	485067	602753	14.73%	2.643%
4	7.351	887	894	908	rBV	1390632	2019501	49.35%	8.854%
5	8.069	1010	1016	1037	rBV	568904	801148	19.58%	3.512%
6	9.145	1192	1199	1226	rBV	2742720	3733040	91.23%	16.366%
7	9.822	1307	1314	1335	rBV	699173	926336	22.64%	4.061%
8	10.616	1443	1449	1479	rBV	1648846	2324653	56.81%	10.192%
9	11.310	1561	1567	1584	rBV	710129	972977	23.78%	4.266%
10	12.898	1831	1837	1842	rBV	3041921	4092123	100.00%	17.940%
11	13.951	2010	2016	2028	rBV	534230	748293	18.29%	3.281%
12	15.410	2257	2264	2276	rBV	335337	561809	13.73%	2.463%




Sum of corrected areas: 22809666

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021225\
Data File : BF141582.D
Acq On : 12 Feb 2025 11:43
Operator : RC/JU
Sample : PB166681BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166681BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

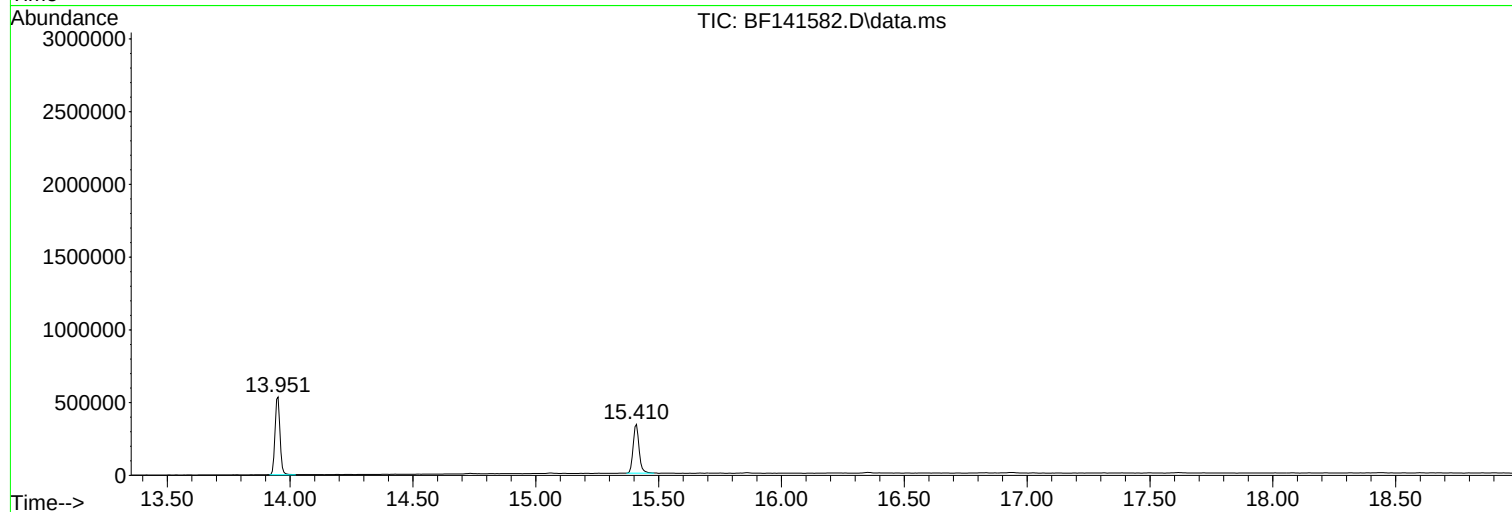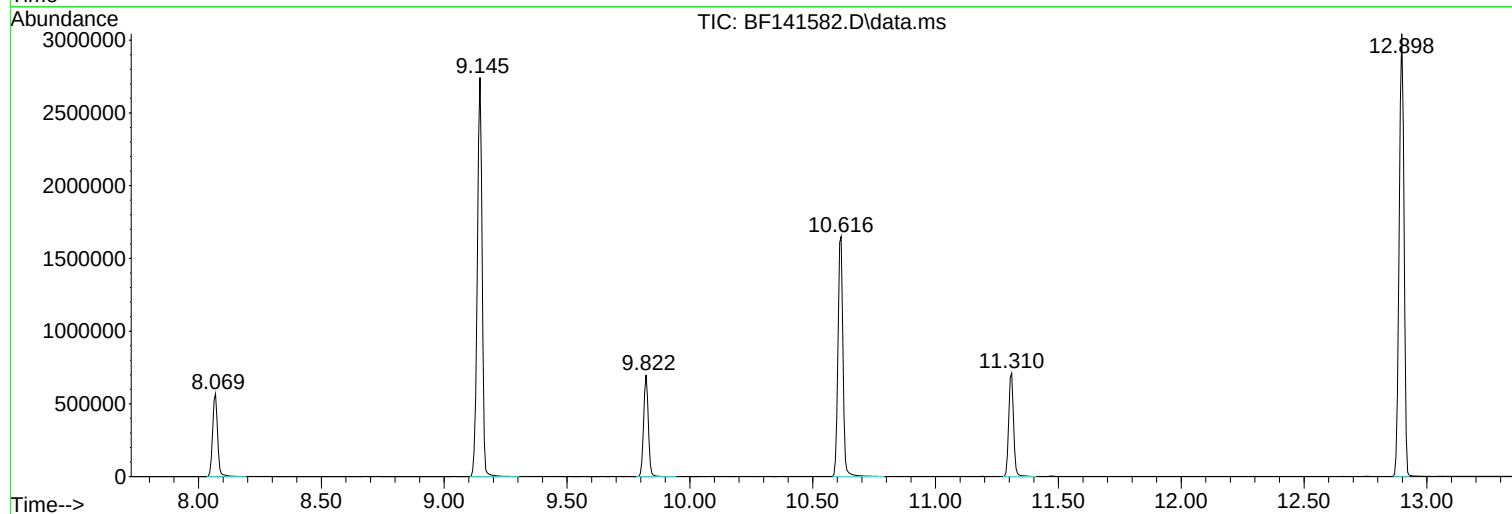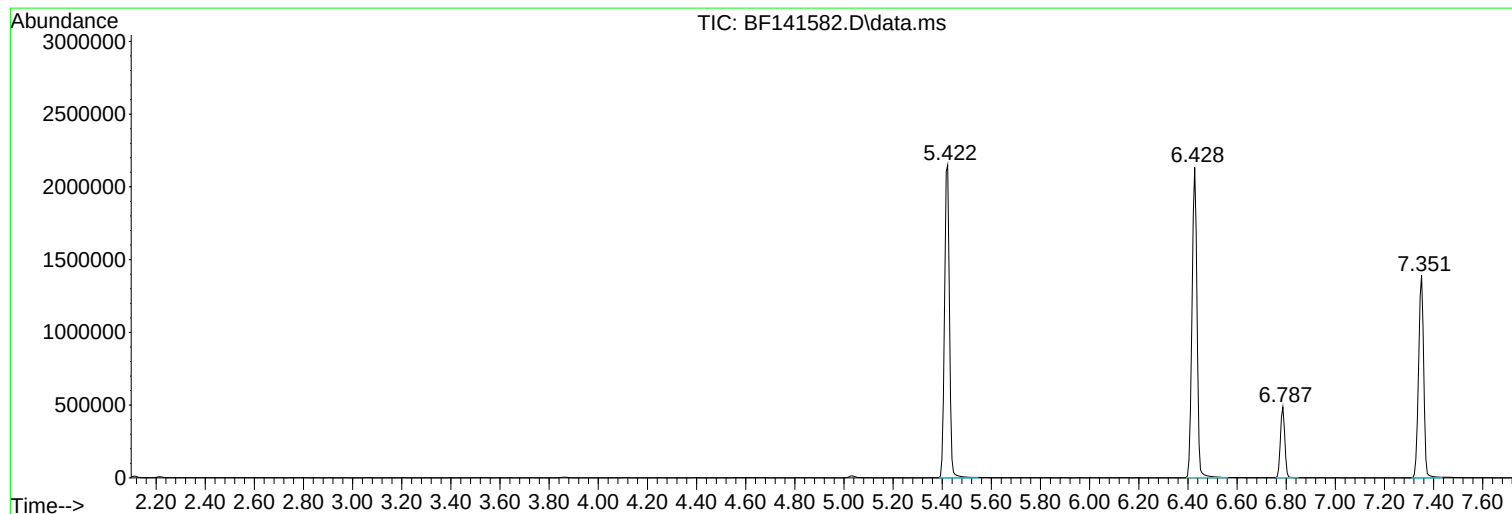

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021225\
Data File : BF141582.D
Acq On : 12 Feb 2025 11:43
Operator : RC/JU
Sample : PB166681BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166681BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021225\
Data File : BF141582.D
Acq On : 12 Feb 2025 11:43
Operator : RC/JU
Sample : PB166681BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166681BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------