
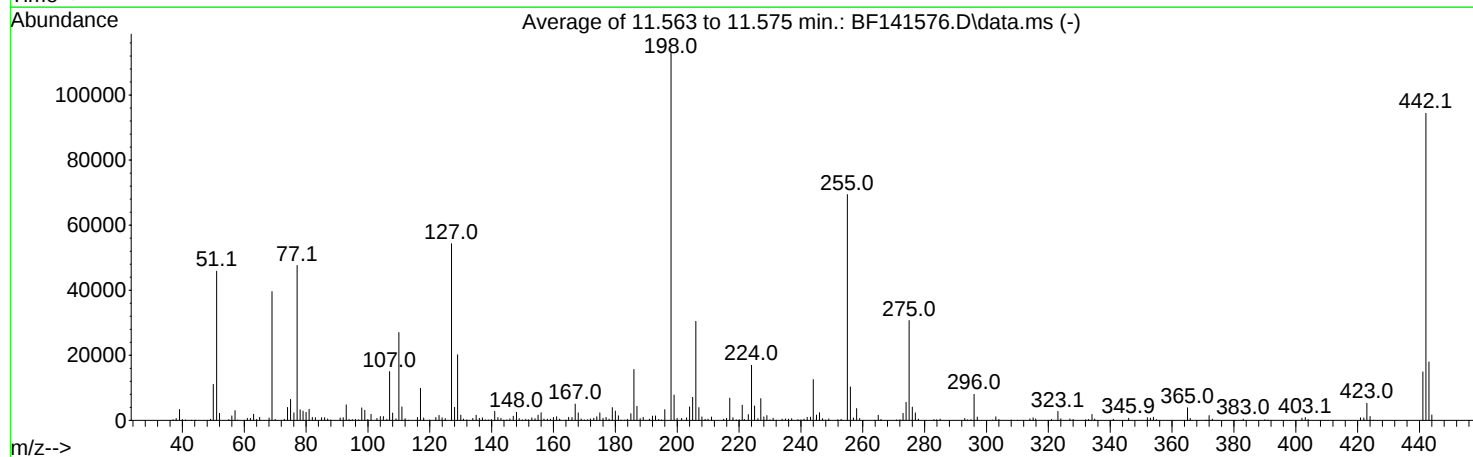


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021225\
Data File : BF141576.D
Acq On : 12 Feb 2025 09:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 06 16:58:59 2025

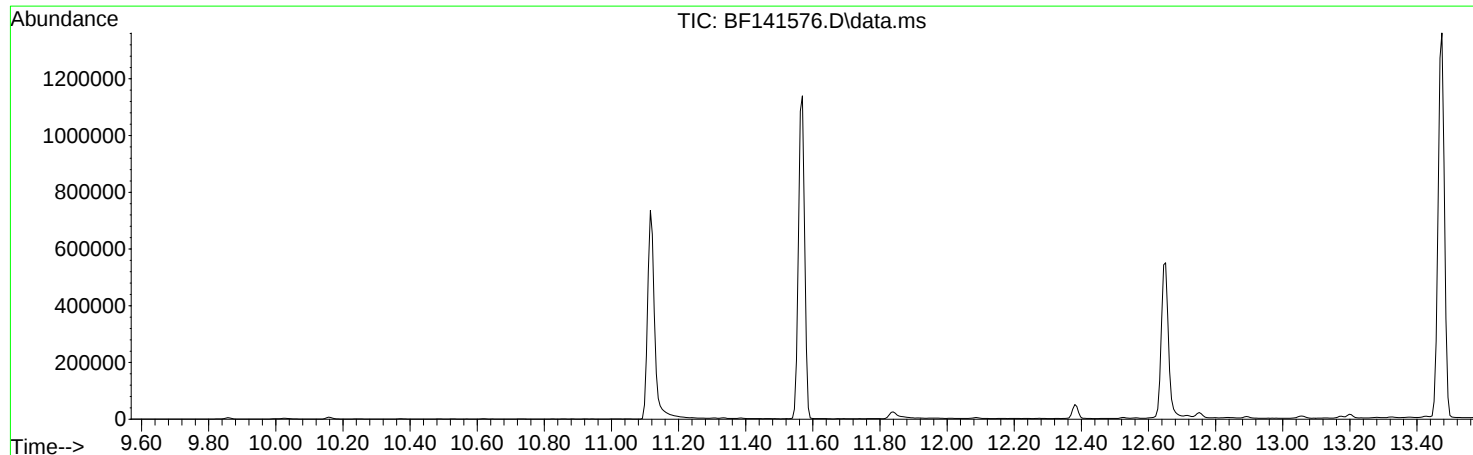

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1603

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	40.5	45816	PASS
68	69	0.00	2	1.9	733	PASS
69	198	0.00	100	35.0	39577	PASS
70	69	0.00	2	0.7	295	PASS
127	198	10	80	48.0	54299	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	113075	PASS
199	198	5	9	6.9	7771	PASS
275	198	10	60	27.1	30696	PASS
365	198	1	100	3.4	3878	PASS
441	198	0.01	100	13.2	14889	PASS
442	442	50	100	100.0	94400	PASS
443	442	15	24	19.0	17945	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/12/2025	BNA_F	<u>BF141576.D</u>
Compound Name	Response	Retention Time
DDT	354959	13.474
DDD	6935	13.198
DDE	623	12.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7558	362517	2.08

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021225\
Data File : BF141576.D
Acq On : 12 Feb 2025 09:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 12 10:33:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

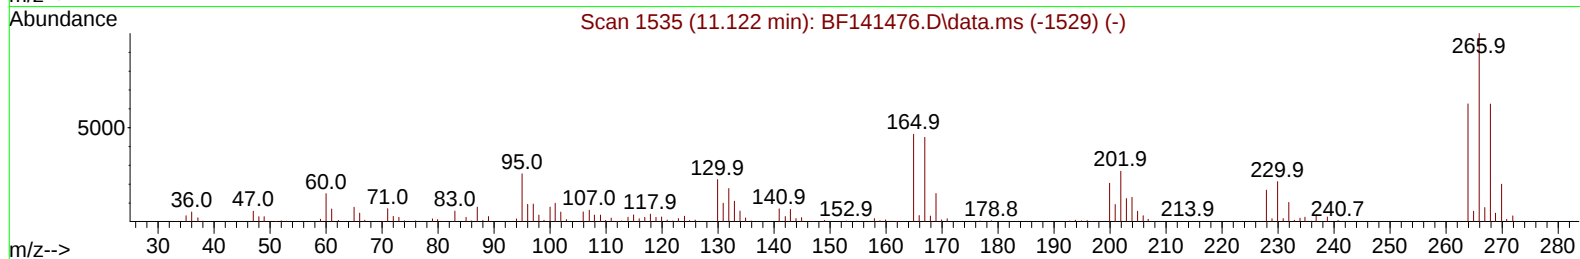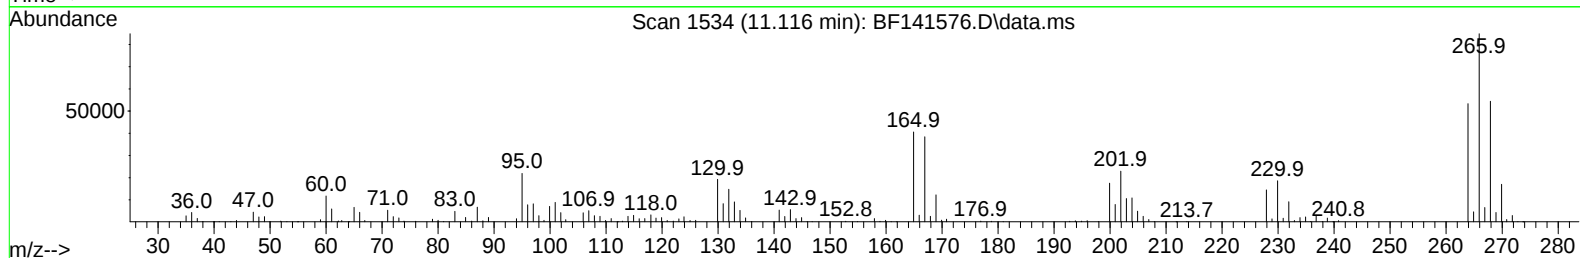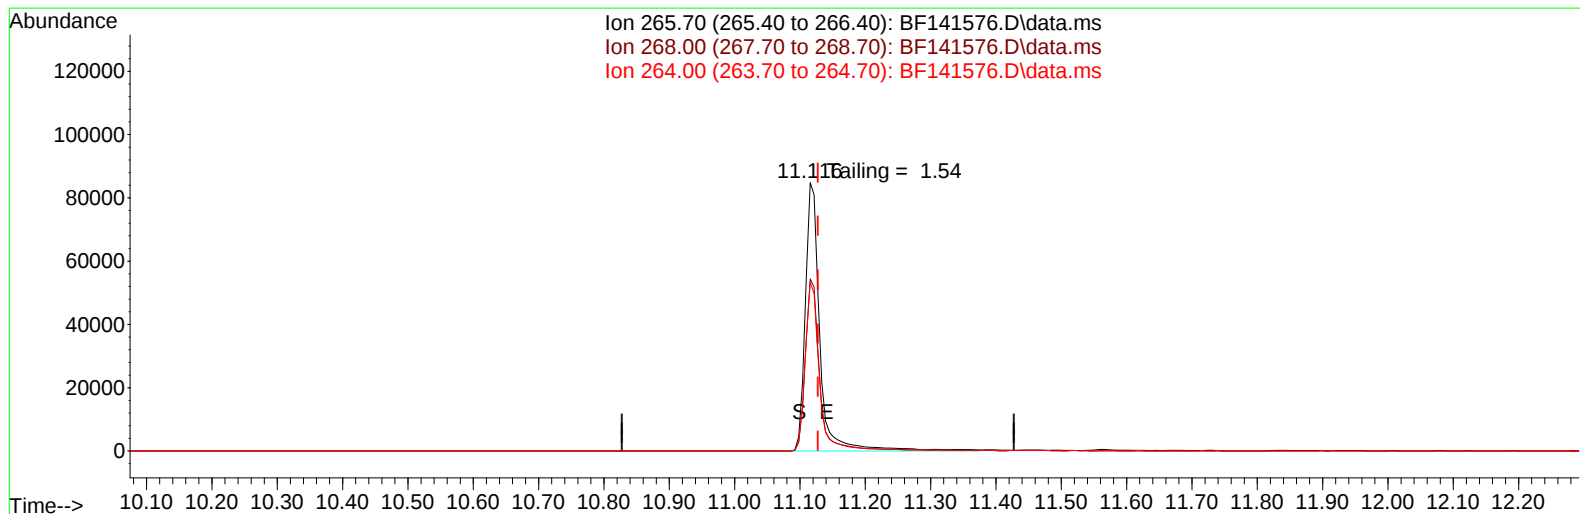

TIC: BF141576.D\data.ms

(70) Pentachlorophenol (C)

11.116min (-0.012) 17103.54 ng




response 131022

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.17
264.00	62.60	62.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021225\
Data File : BF141576.D
Acq On : 12 Feb 2025 09:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 12 10:33:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

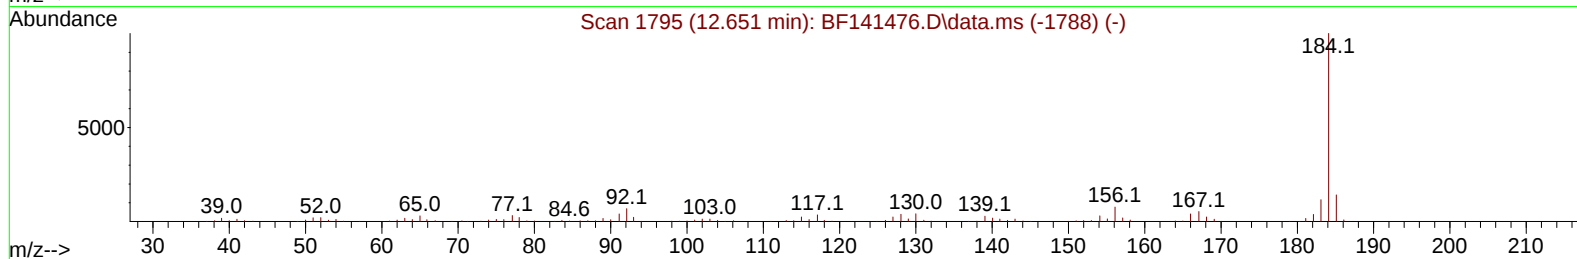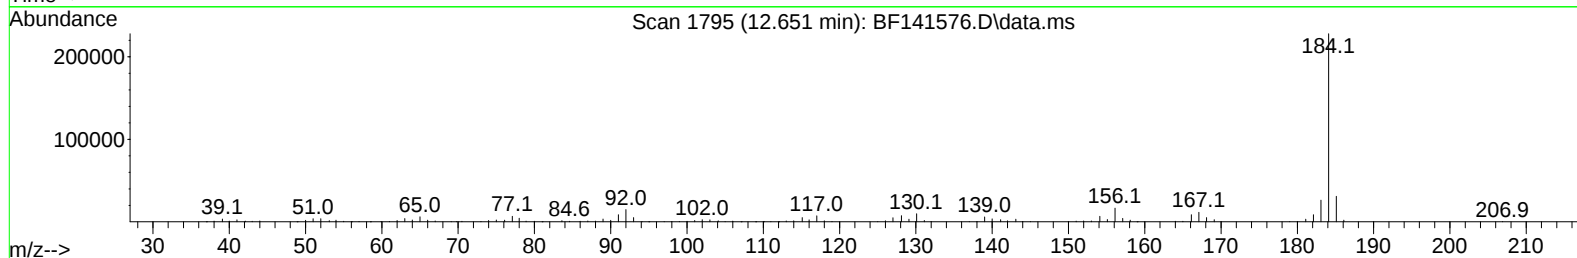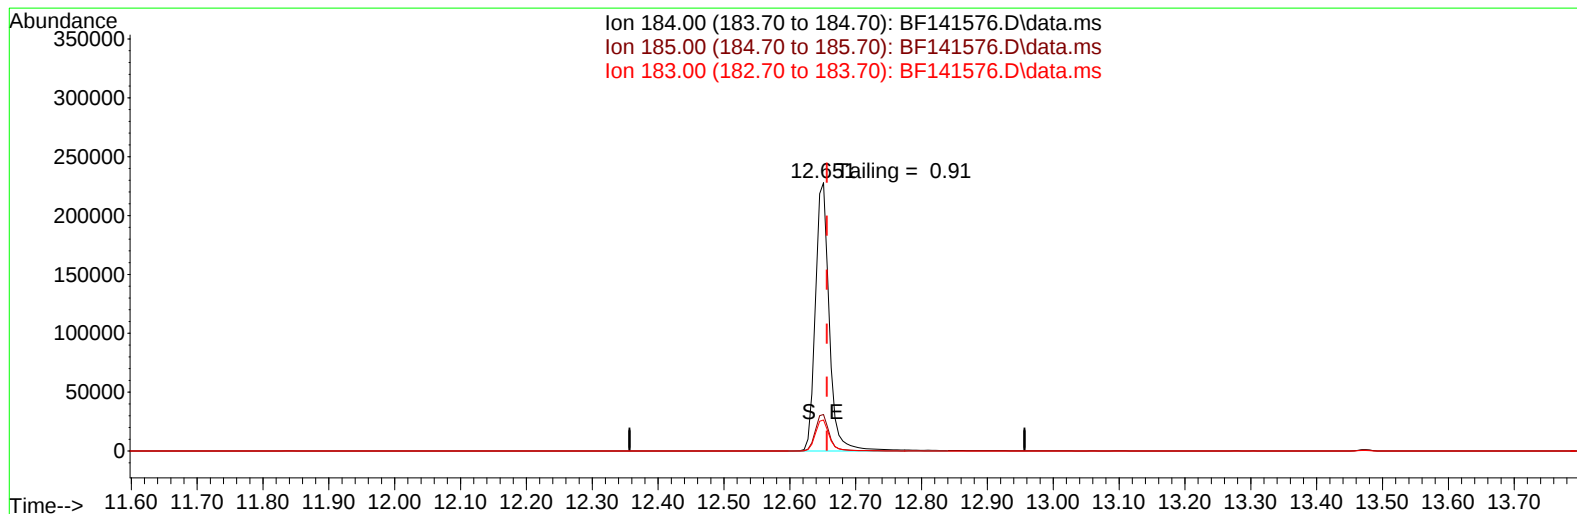

TIC: BF141576.D\data.ms

(77) Benzidine

12.651min (-0.006) 16095.31 ng

response 335448

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.63
183.00	11.60	11.58
0.00	0.00	0.00