
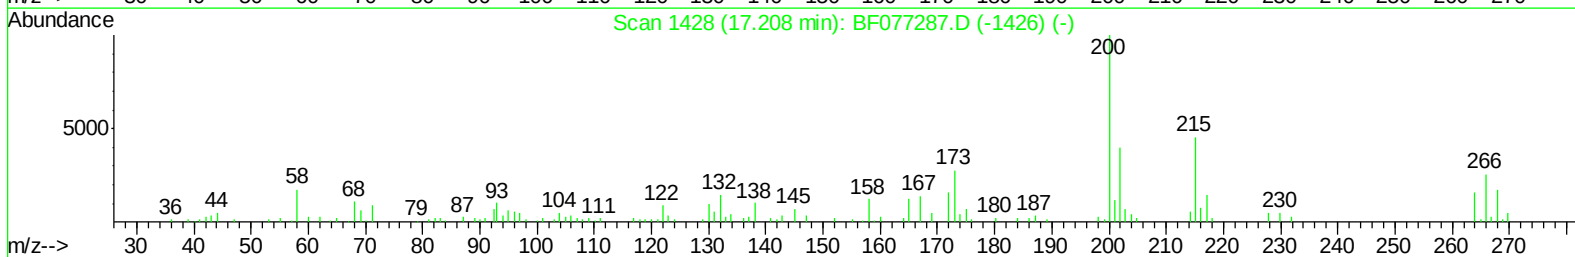
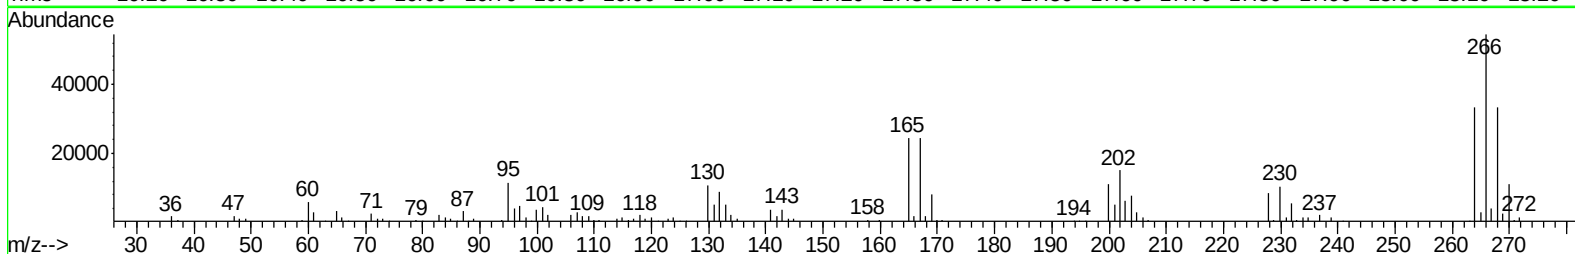


Data Path : Z:\HPCHEM1\BNA_F\Data\BF021315\
Data File : BF077304.D
Acq On : 13 Feb 2015 10:49
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 04:20:31 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 13 13:10:36 2015
Response via : Initial Calibration

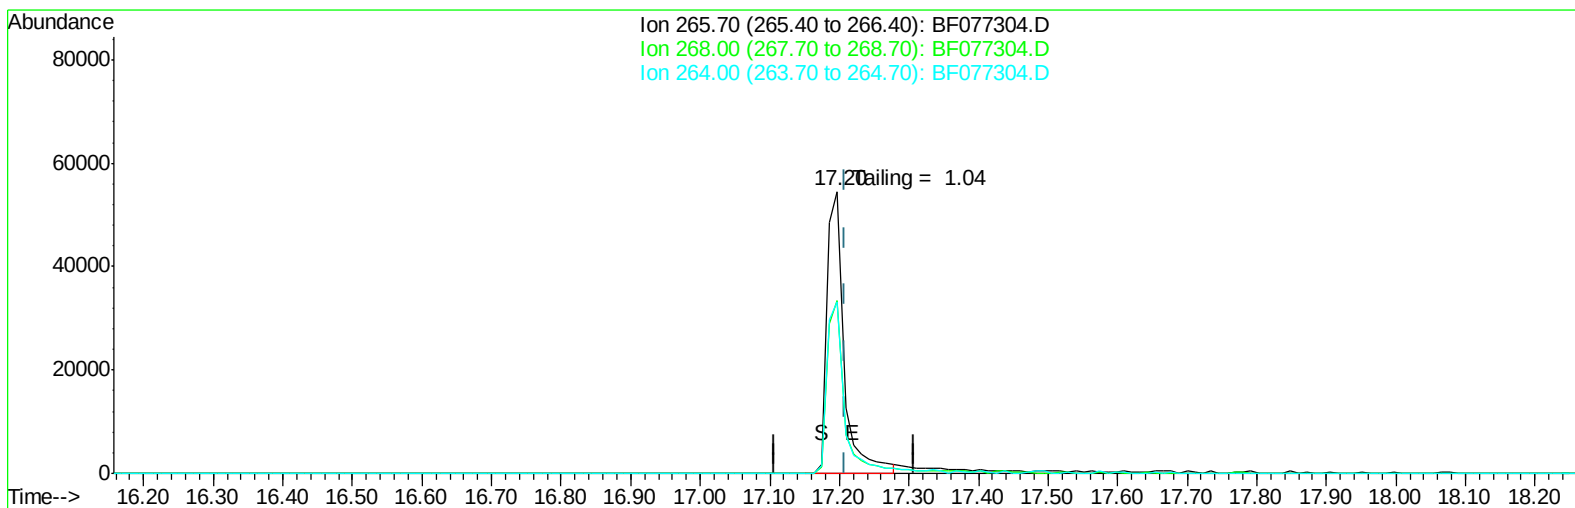

TIC: BF077304.D

(69) Pentachlorophenol (C)




17.197min (-0.011) 0.00ng

response 91464

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	61.47
264.00	61.90	60.97
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF021315\
Data File : BF077304.D
Acq On : 13 Feb 2015 10:49
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 04:20:31 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 13 13:10:36 2015
Response via : Initial Calibration

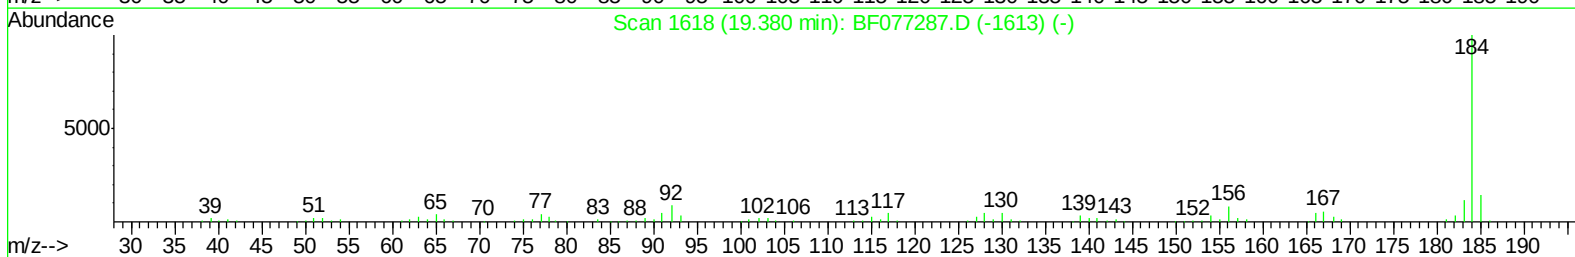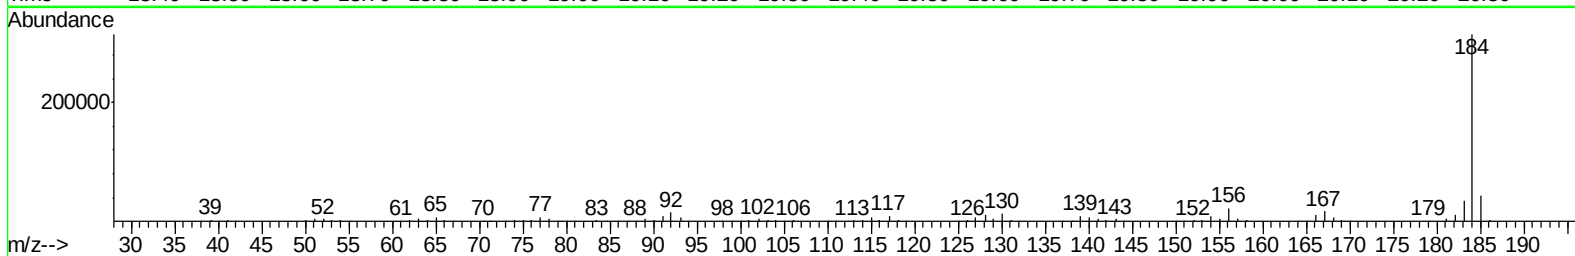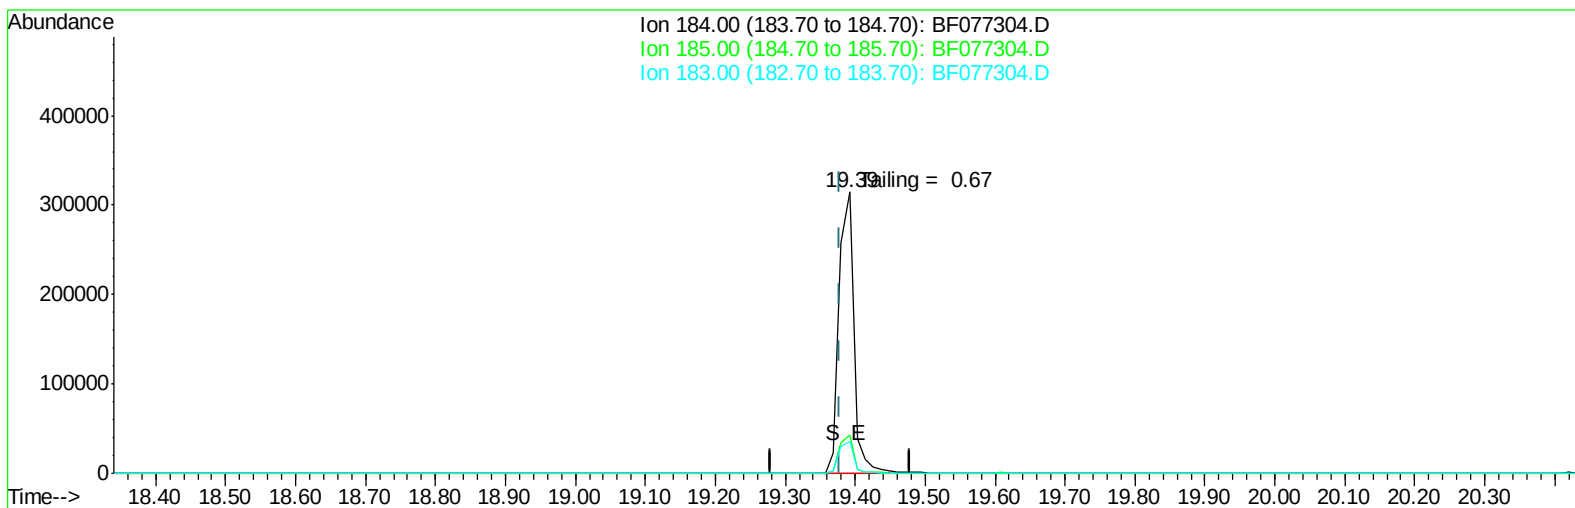

TIC: BF077304.D

(76) Benzidine

19.392min (+0.013) 43273.58ng

response 452564

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.54
183.00	11.60	11.27
0.00	0.00	0.00