

Data Path : Z:\HPCHEM1\BNA F\DATA\BF021315\
 Data File : BF077316.D
 Acq On : 13 Feb 2015 19:41
 Operator : TP/IZ
 Sample : G1294-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 1003-20(0-2)

Quant Time: Feb 16 10:26:47 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 13 13:10:36 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.50	152	28941	20.00	ng	0.01
21) Naphthalene-d8	10.41	136	121671	20.00	ng	0.00
38) Acenaphthene-d10	14.52	164	58681	20.00	ng	0.00
63) Phenanthrene-d10	17.43	188	101226	20.00	ng	-0.01
75) Chrysene-d12	20.95	240	97048	20.00	ng	-0.01
86) Perylene-d12	22.58	264	90507	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	4.49	112	194261	104.80	ng	0.00
7) Phenol-d6	6.92	99	245756	107.29	ng	-0.01
23) Nitrobenzene-d5	8.81	82	151709	71.22	ng	-0.01
41) 2,4,6-Tribromophenol	16.29	330	47646	99.57	ng	-0.01
44) 2-Fluorobiphenyl	13.06	172	297176	76.22	ng	-0.01
78) Terphenyl-d14	19.69	244	271408	62.82	ng	-0.01
Target Compounds						
49) Dimethylphthalate	14.15	163	25230	5.95	ng	# 98
79) Butylbenzylphthalate	20.36	149	14870	4.54	ng	# 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF021315\
Data File : BF077316.D
Acq On : 13 Feb 2015 19:41
Operator : TP/IZ
Sample : G1294-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
1003-20(0-2)

Quant Time: Feb 16 10:26:47 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 13 13:10:36 2015
Response via : Initial Calibration

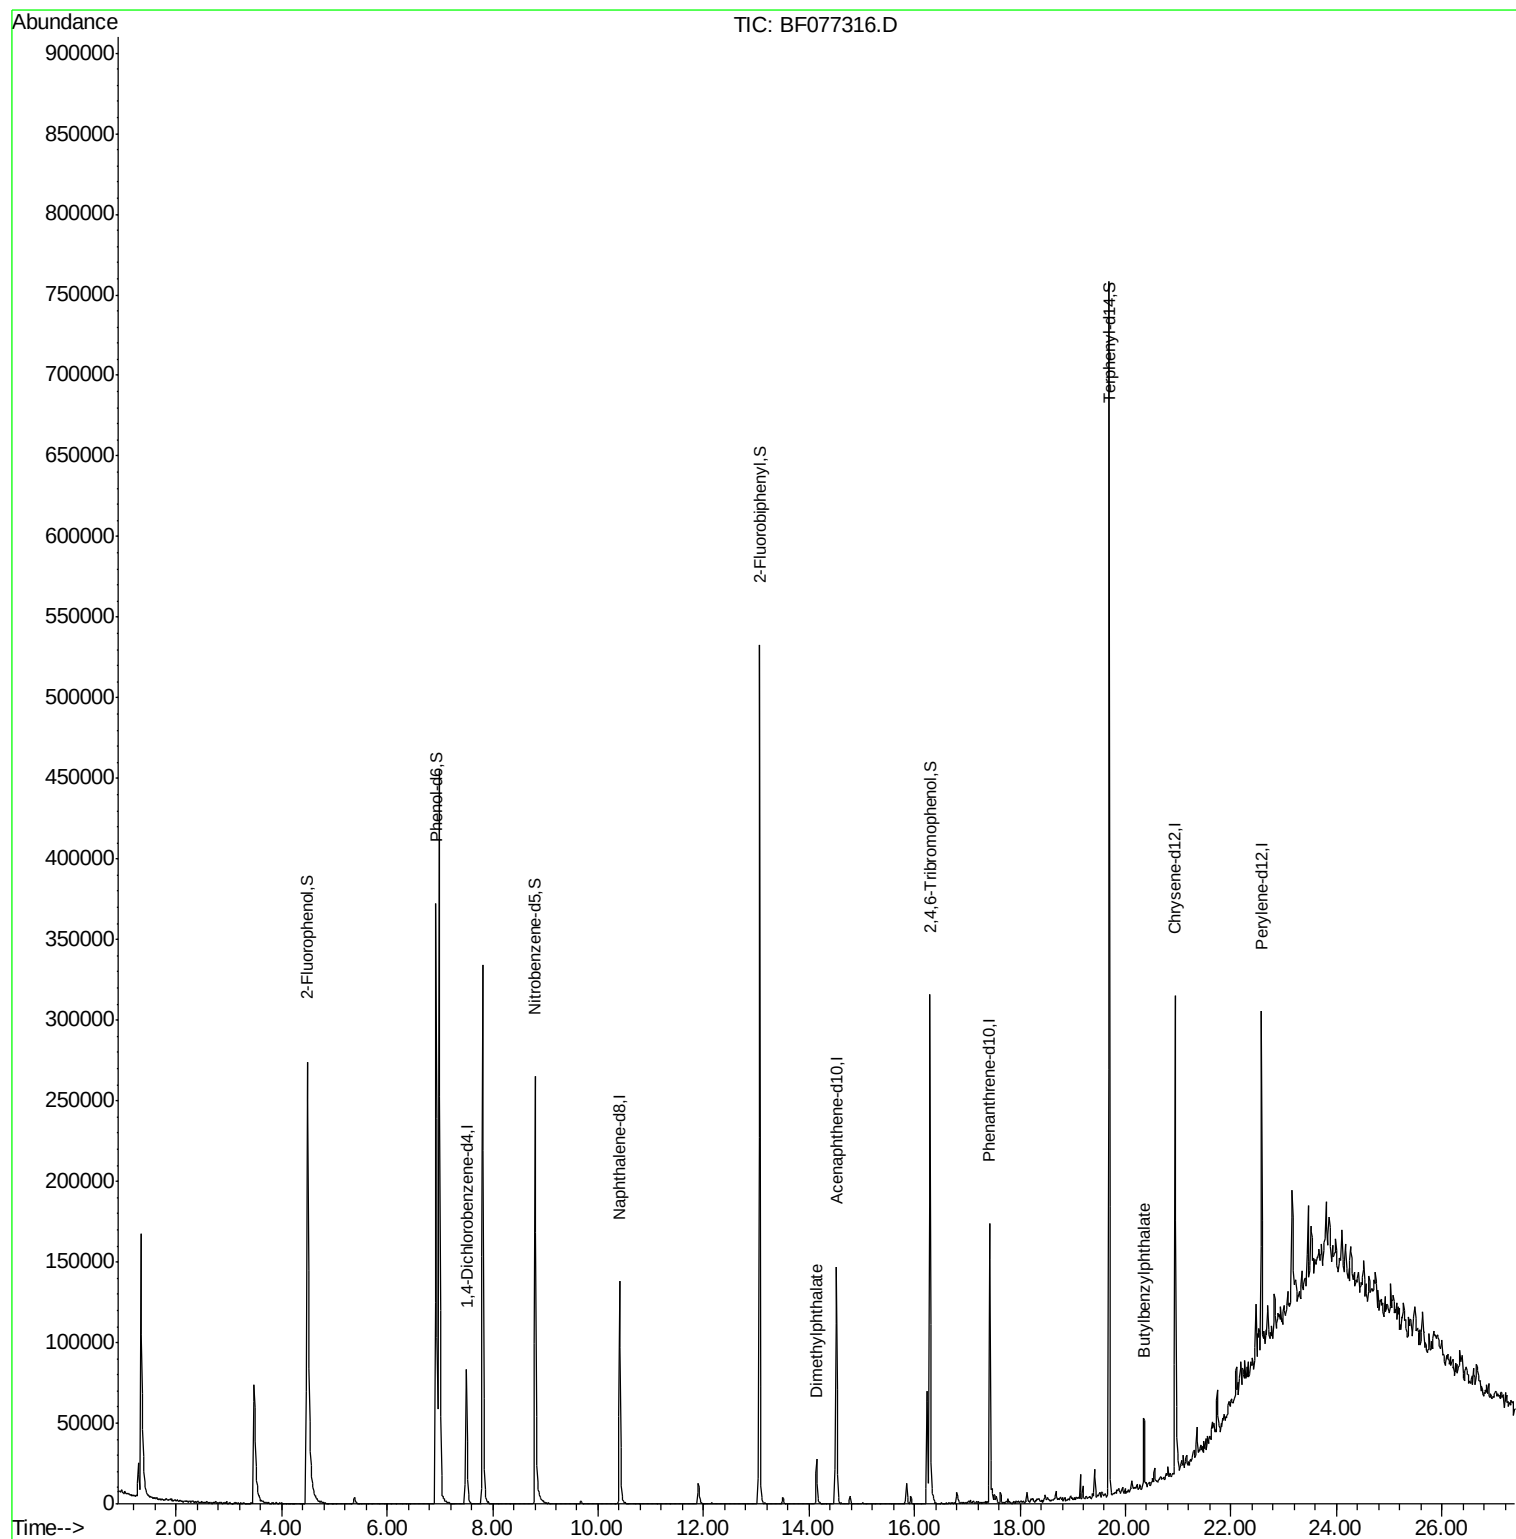

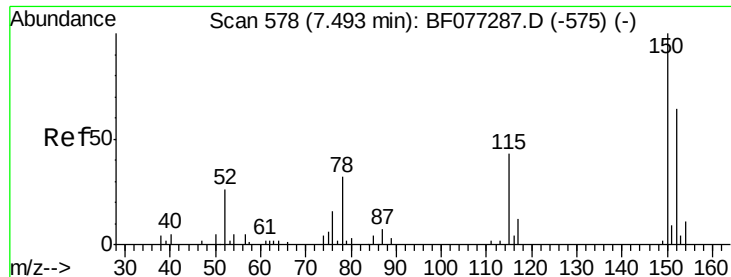


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.50 min Scan# 579
Delta R.T. 0.01 min
Lab File: BF077316.D
Acq: 13 Feb 2015 19:41

Instrument :
BNA_F
ClientSampleId :
1003-20(0-2)

Tot Ion:152 Resp: 28941
Ion Ratio Lower Upper
152 100
150 168.4 124.9 187.3
115 64.9 54.1 81.1

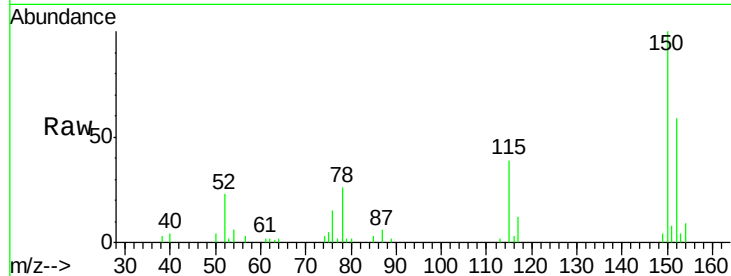


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

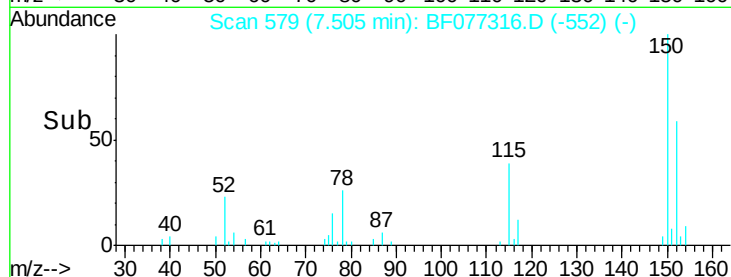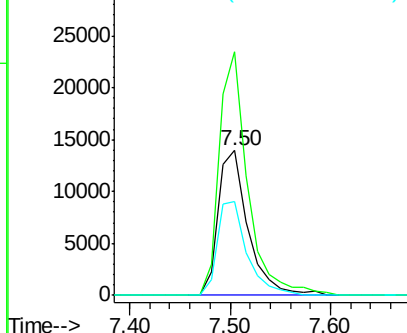



#5


2-Fluorophenol
Concen: 104.80 ng
RT: 4.49 min Scan# 315
Delta R.T. 0.00 min
Lab File: BF077316.D
Acq: 13 Feb 2015 19:41

Tgt Ion:112 Resp: 194261
Ion Ratio Lower Upper
112 100
64 67.9 55.0 82.4
63 37.7 33.0 49.6



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

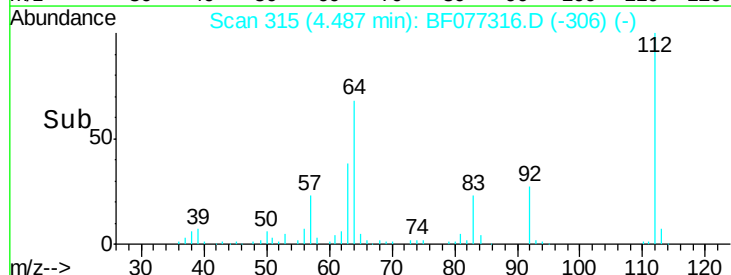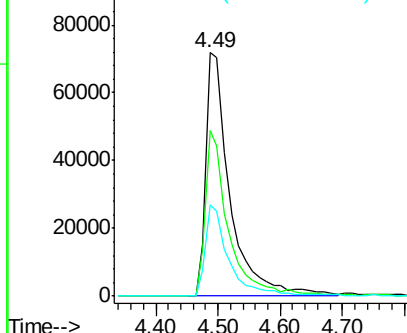

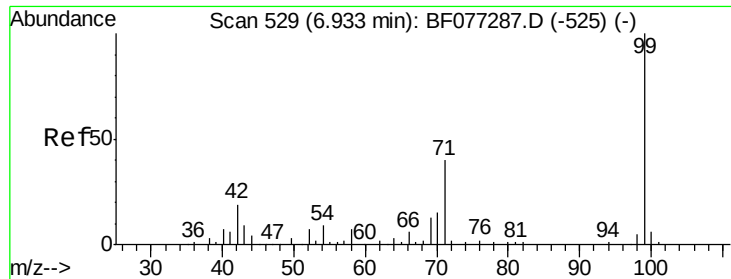

#7

Phenol-d6

Concen: 107.29 ng

RT: 6.92 min Scan# 528

Delta R.T. -0.01 min

Lab File: BF077316.D

Acq: 13 Feb 2015 19:41

Instrument :

BNA_F

ClientSampleId :

1003-20(0-2)


Tot Ion: 99 Resp: 245756

Ion Ratio Lower Upper

99 100

42 19.4 15.0 22.4




71 39.2 31.8 47.6

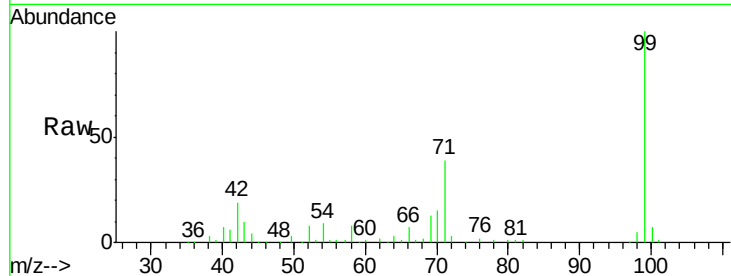

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

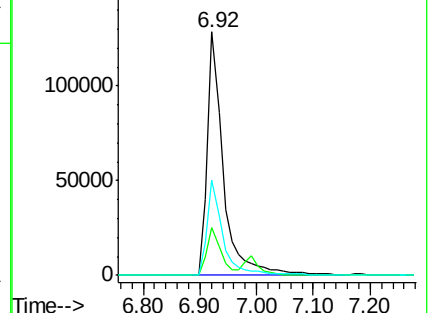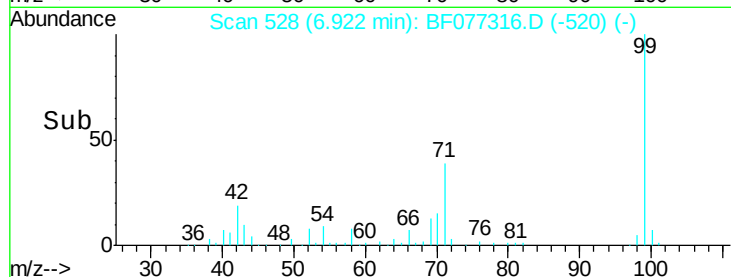

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.41 min Scan# 833

Delta R.T. 0.00 min

Lab File: BF077316.D

Acq: 13 Feb 2015 19:41

Tgt Ion: 136 Resp: 121671


Ion Ratio Lower Upper

136 100

137 10.8 8.7 13.1

54 8.0 8.2 12.2#

68 5.0 3.1 4.7#






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

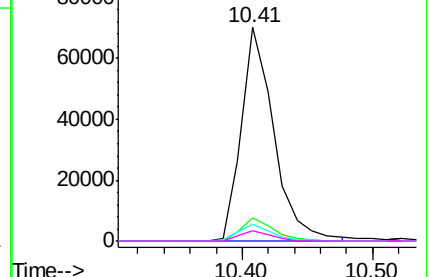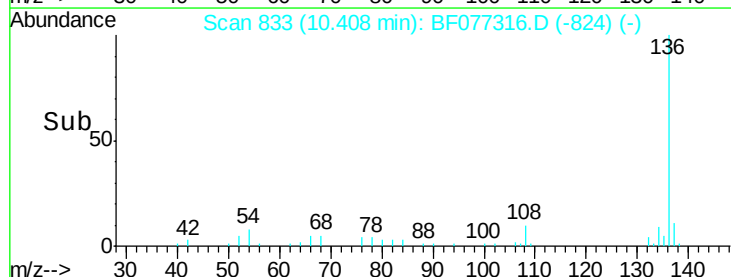


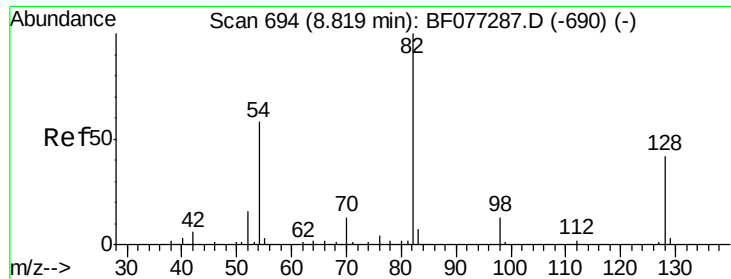




#23
 Nitrobenzene-d5
 Concen: 71.22 ng
 RT: 8.81 min Scan# 693
 Delta R.T. -0.01 min
 Lab File: BF077316.D
 Acq: 13 Feb 2015 19:41

Instrument :
 BNA_F
 ClientSampleId :
 1003-20(0-2)

Tot Ion	82	Resp	151709
Ion Ratio	100	Lower	Upper
128	39.0	33.6	50.4
54	60.9	46.2	69.2

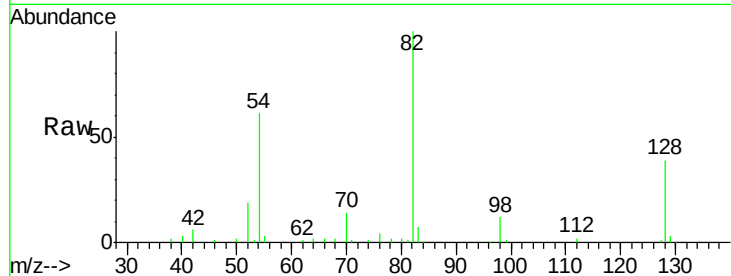


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

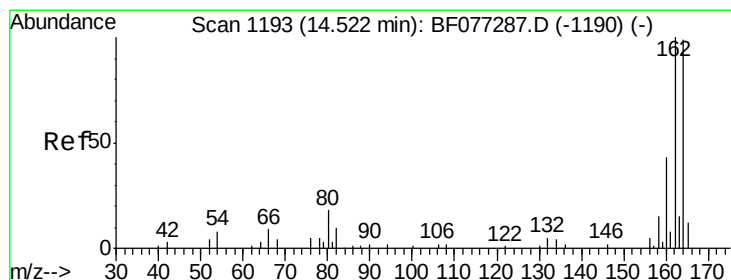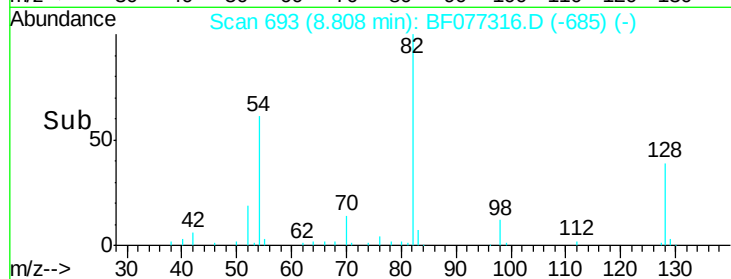
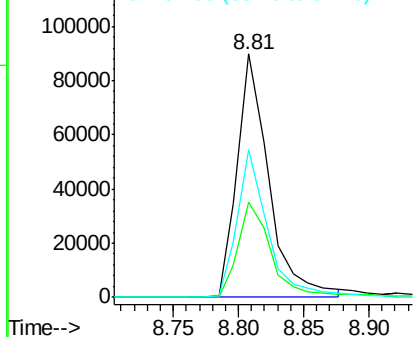



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.52 min Scan# 1193
 Delta R.T. 0.00 min
 Lab File: BF077316.D
 Acq: 13 Feb 2015 19:41

Tgt Ion	164	Resp	58681
Ion Ratio	100	Lower	Upper
162	100.8	81.0	121.4
160	44.6	35.2	52.8



Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

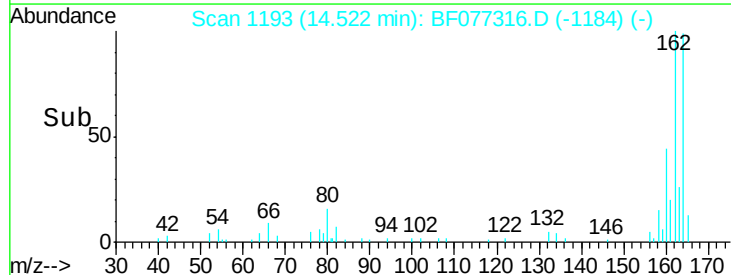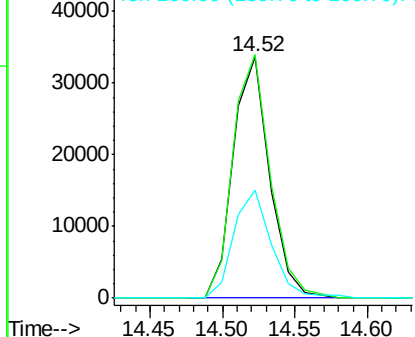


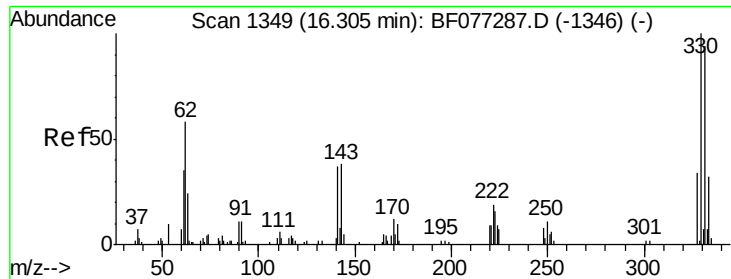




#41
 2,4,6-Tribromophenol
 Concen: 99.57 ng
 RT: 16.29 min Scan# 1348
 Delta R.T. -0.01 min
 Lab File: BF077316.D
 Acq: 13 Feb 2015 19:41

Instrument :
 BNA_F
 ClientSampleId :
 1003-20(0-2)

Tot Ion	Ratio	Lower	Upper
330	100		
332	100.6	0.0	0.0#
141	52.6	0.0	0.0#

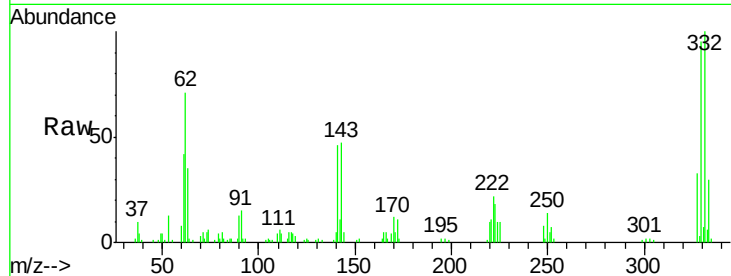


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

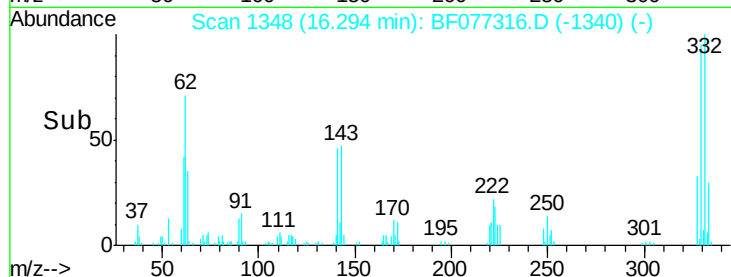
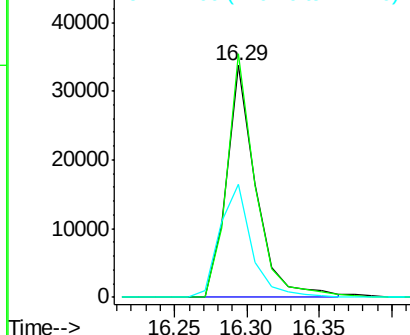



#44
 2-Fluorobiphenyl
 Concen: 76.22 ng
 RT: 13.06 min Scan# 1065
 Delta R.T. -0.01 min
 Lab File: BF077316.D
 Acq: 13 Feb 2015 19:41

Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.4	27.8	41.8
170	23.1	18.3	27.5



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

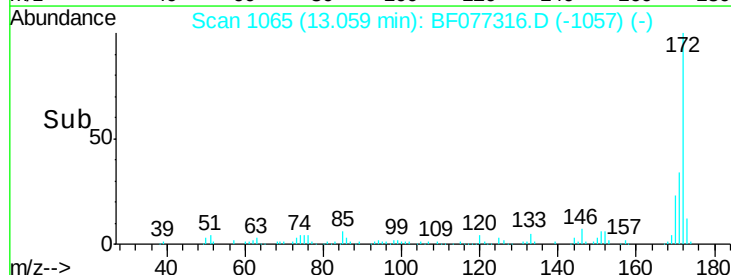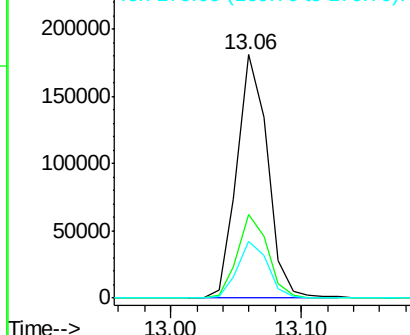

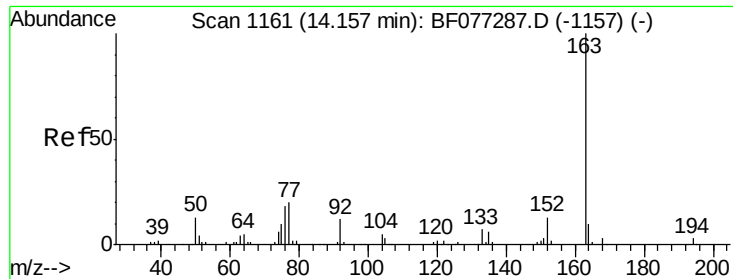

#49

Dimethylphthalate

Concen: 5.95 ng

RT: 14.15 min Scan# 1160

Delta R.T. -0.01 min

Lab File: BF077316.D

Acq: 13 Feb 2015 19:41

Instrument :

BNA_F

ClientSampleId :

1003-20(0-2)


Tot Ion:163 Resp: 25230

Ion Ratio Lower Upper

163 100

194 3.9 2.3 3.5#




164 8.8 7.6 11.4

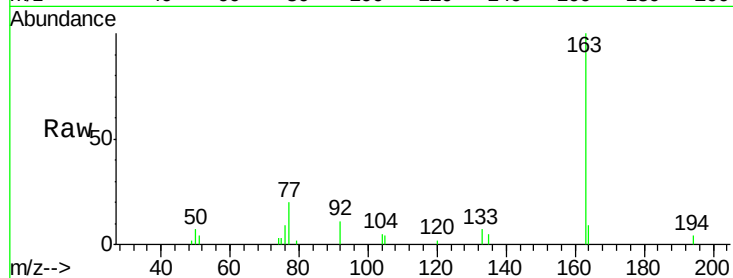

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

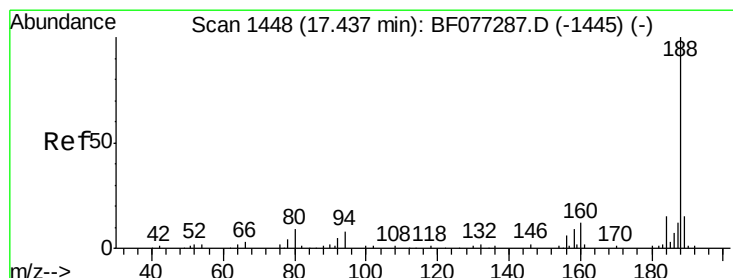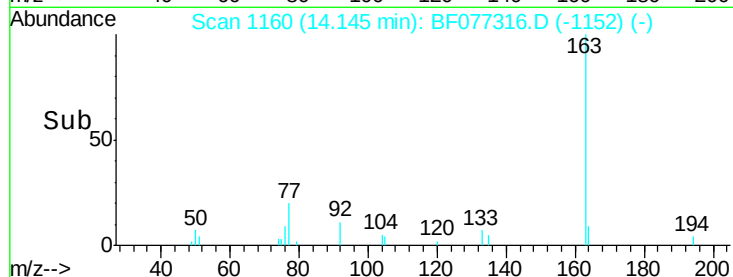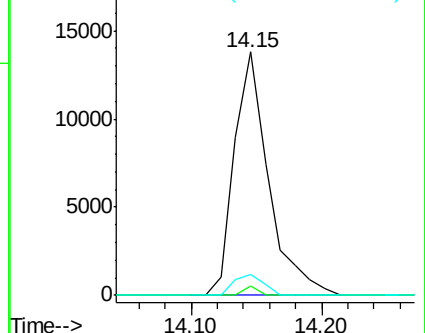

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.43 min Scan# 1447

Delta R.T. -0.01 min

Lab File: BF077316.D

Acq: 13 Feb 2015 19:41


Tgt Ion:188 Resp: 101226

Ion Ratio Lower Upper

188 100

94 10.9 6.5 9.7#



80 11.3 7.1 10.7#

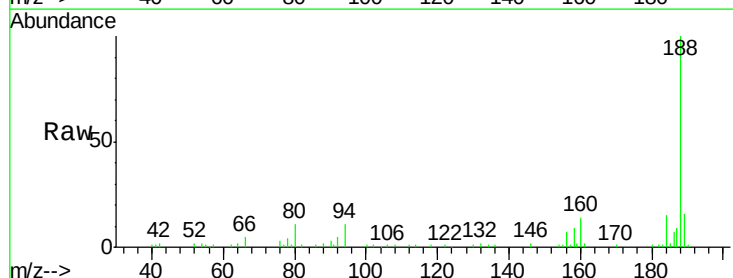


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

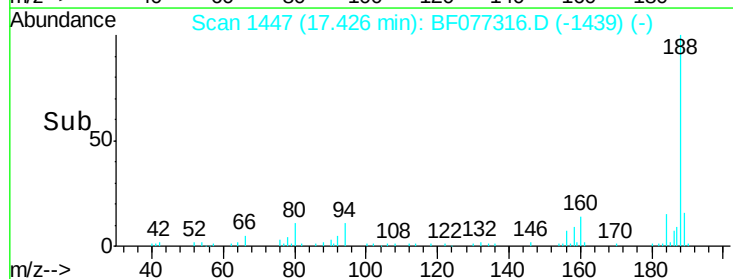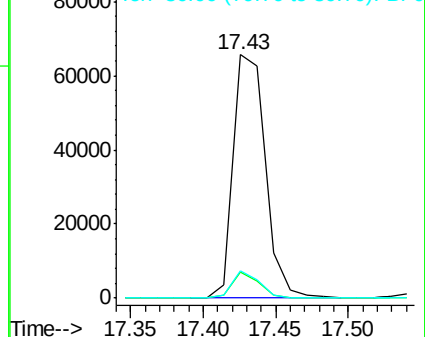

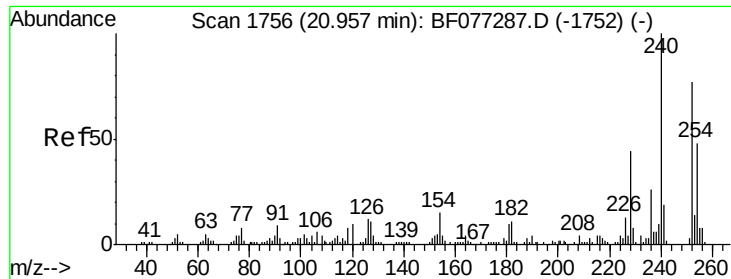

#75

Chrysene-d12

Concen: 20.00 ng

RT: 20.95 min Scan# 1755

Delta R.T. -0.01 min

Lab File: BF077316.D

Acq: 13 Feb 2015 19:41

Instrument :

BNA_F

ClientSampleId :

1003-20(0-2)


Tot Ion:240 Resp: 97048

Ion Ratio Lower Upper

240 100

120 11.1 7.8 11.8




236 25.2 20.4 30.6



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

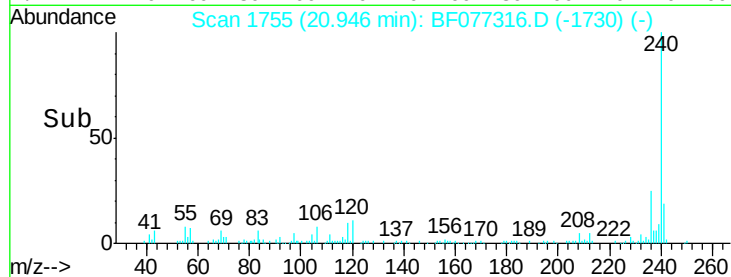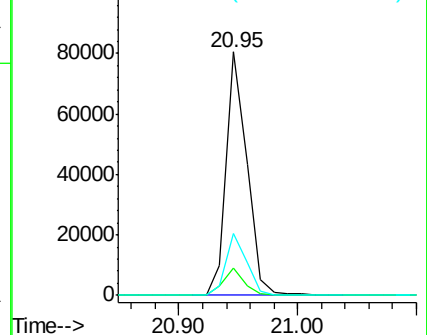

#78

Terphenyl-d14

Concen: 62.82 ng

RT: 19.69 min Scan# 1645

Delta R.T. -0.01 min

Lab File: BF077316.D

Acq: 13 Feb 2015 19:41


Tgt Ion:244 Resp: 271408

Ion Ratio Lower Upper

244 100

212 7.2 5.6 8.4



122 11.1 7.0 10.4#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E



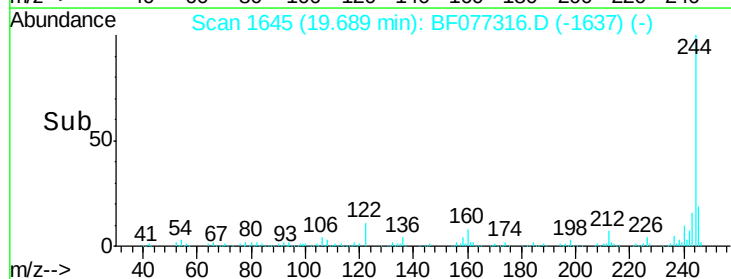
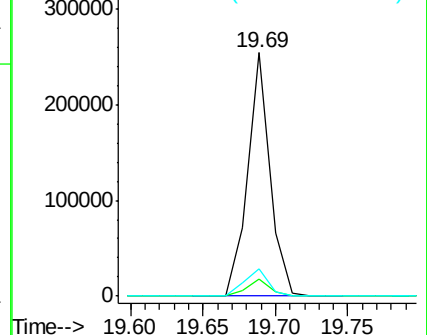


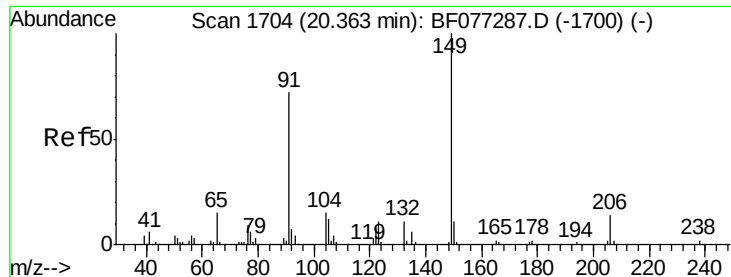

#79
Butylbenzylphthalate
Concen: 4.54 ng
RT: 20.36 min Scan# 1704
Delta R.T. 0.00 min
Lab File: BF077316.D
Acq: 13 Feb 2015 19:41

Instrument :
BNA_F
ClientSampleId :
1003-20(0-2)

Tot Ion:149 Resp: 14870
Ion Ratio Lower Upper
149 100
91 62.8 57.3 85.9
206 17.7 11.6 17.4#

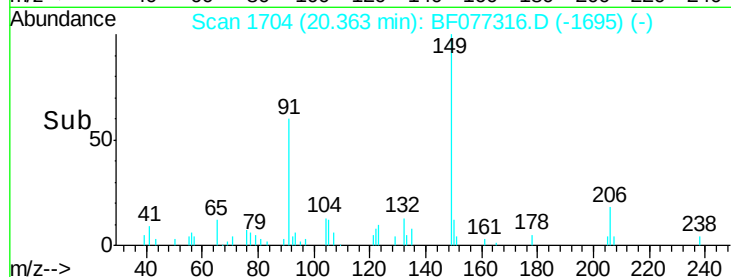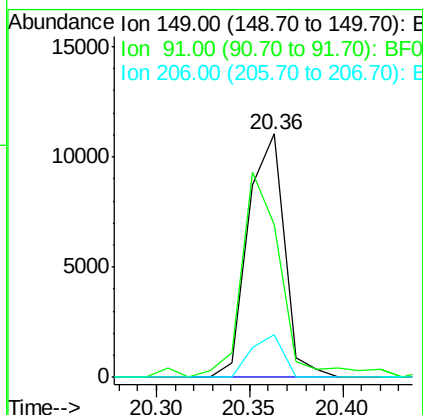

#86
Perylene-d12
Concen: 20.00 ng
RT: 22.58 min Scan# 1898
Delta R.T. -0.06 min
Lab File: BF077316.D
Acq: 13 Feb 2015 19:41

Tgt Ion:264 Resp: 90507
Ion Ratio Lower Upper
264 100
260 23.5 18.6 27.8
265 20.9 16.2 24.2

