


Data Path : Z:\HPCHEM1\BNA F\Data\BF021315\
 Data File : BF077304.D
 Acq On : 13 Feb 2015 10:49
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 13 13:10:36 2015

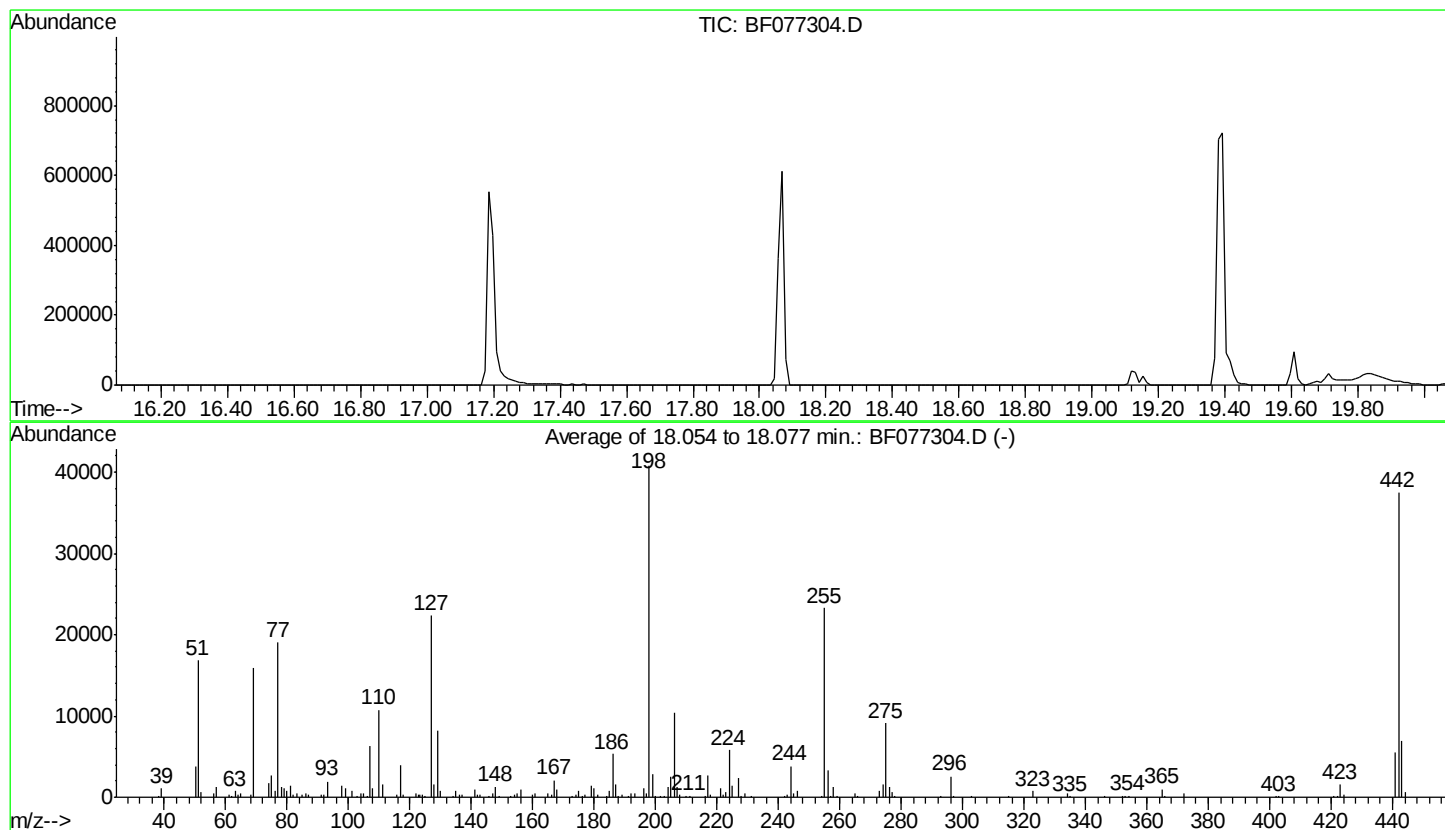

AutoFind: Scans 1502, 1503, 1504; Background Corrected with Scan 1498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	16808	PASS
68	69	0.00	2	1.6	254	PASS
69	198	0.00	100	38.8	15847	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.8	22360	PASS
197	198	0.00	2	1.0	406	PASS
198	198	100	100	100.0	40819	PASS
199	198	5	9	6.8	2768	PASS
275	198	10	60	22.4	9129	PASS
365	198	1	100	2.4	962	PASS
441	442	0.01	24	14.8	5550	PASS
442	198	50	100	91.8	37466	PASS
443	442	15	24	18.7	7000	PASS