


Aniline

Response Ratio

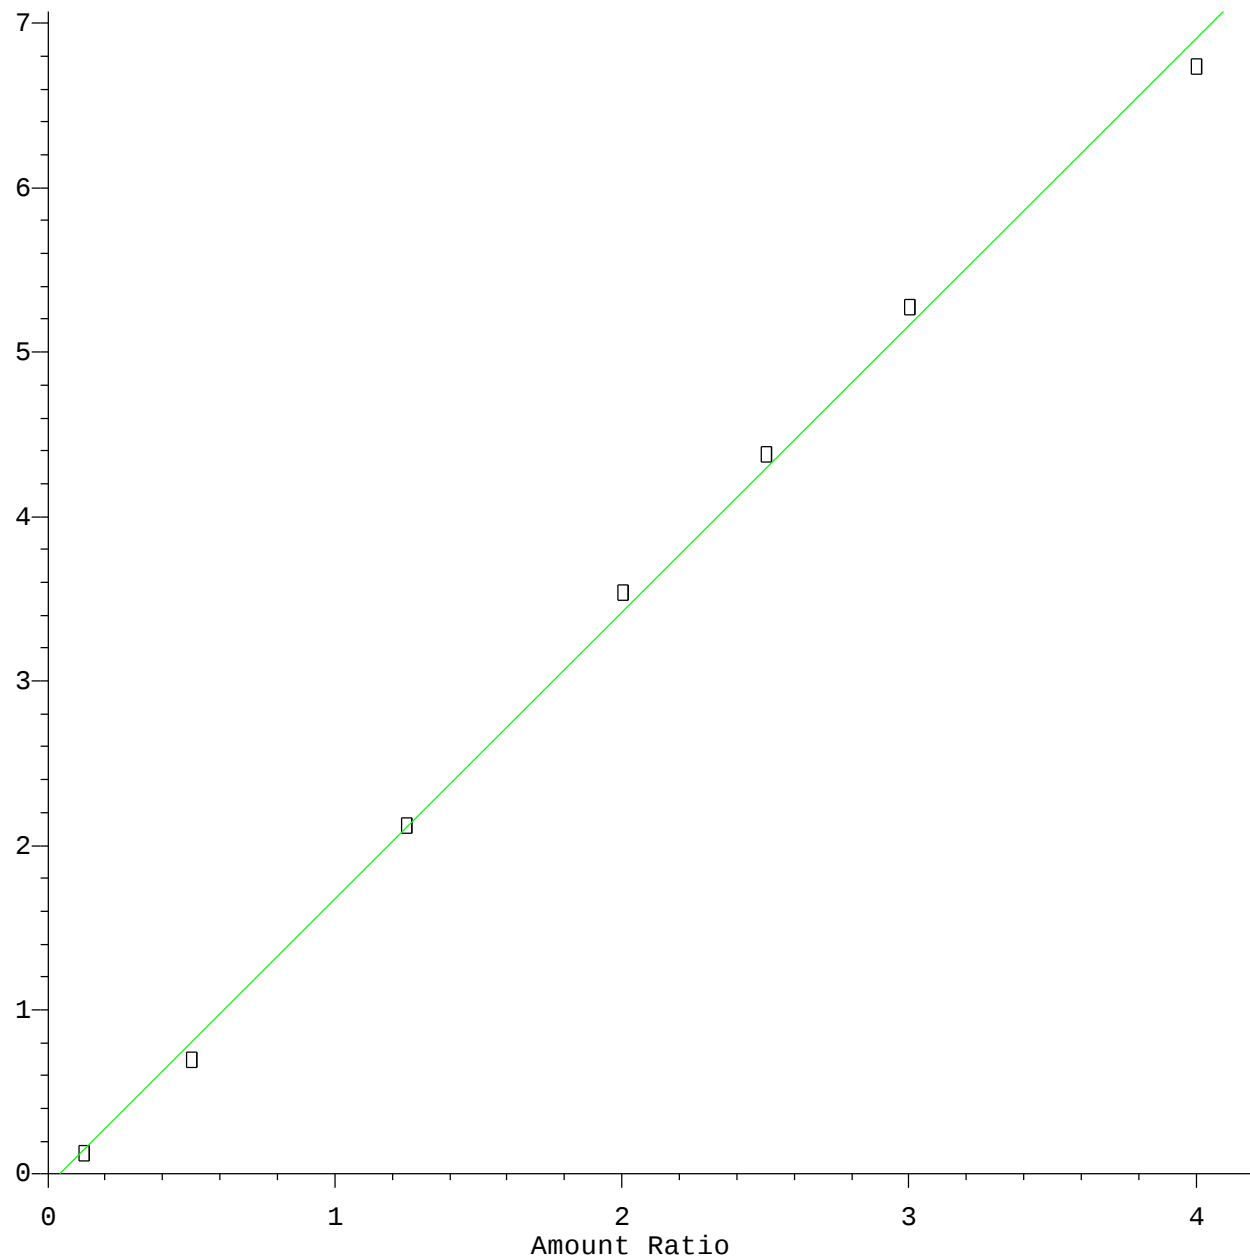


Resp Ratio = 1.74×10^0 * Amt - 6.95×10^{-2}
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF021316.M
Calibration Table Last Updated: Sat Feb 13 00:11:18 2016

bis(2-Chloroethyl)ether

Response Ratio

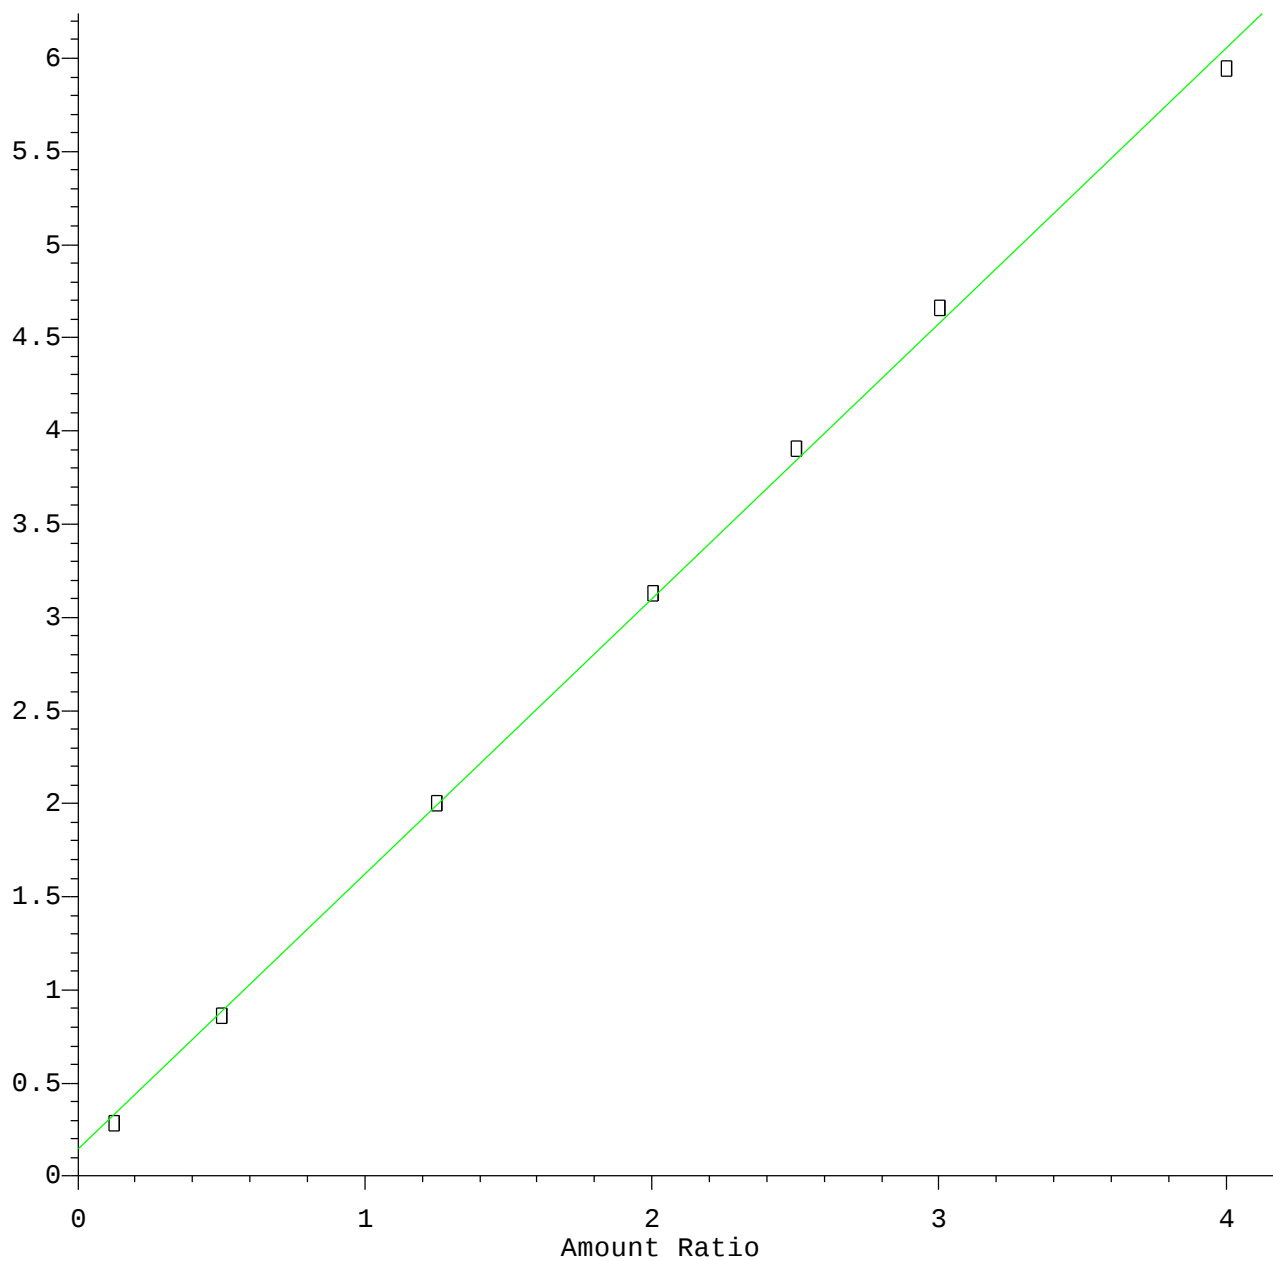


Resp Ratio = 1.48e+000 * Amt + 1.43e-001
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF021316.M
Calibration Table Last Updated: Sat Feb 13 00:11:18 2016


3+4-Methylphenols

Response Ratio

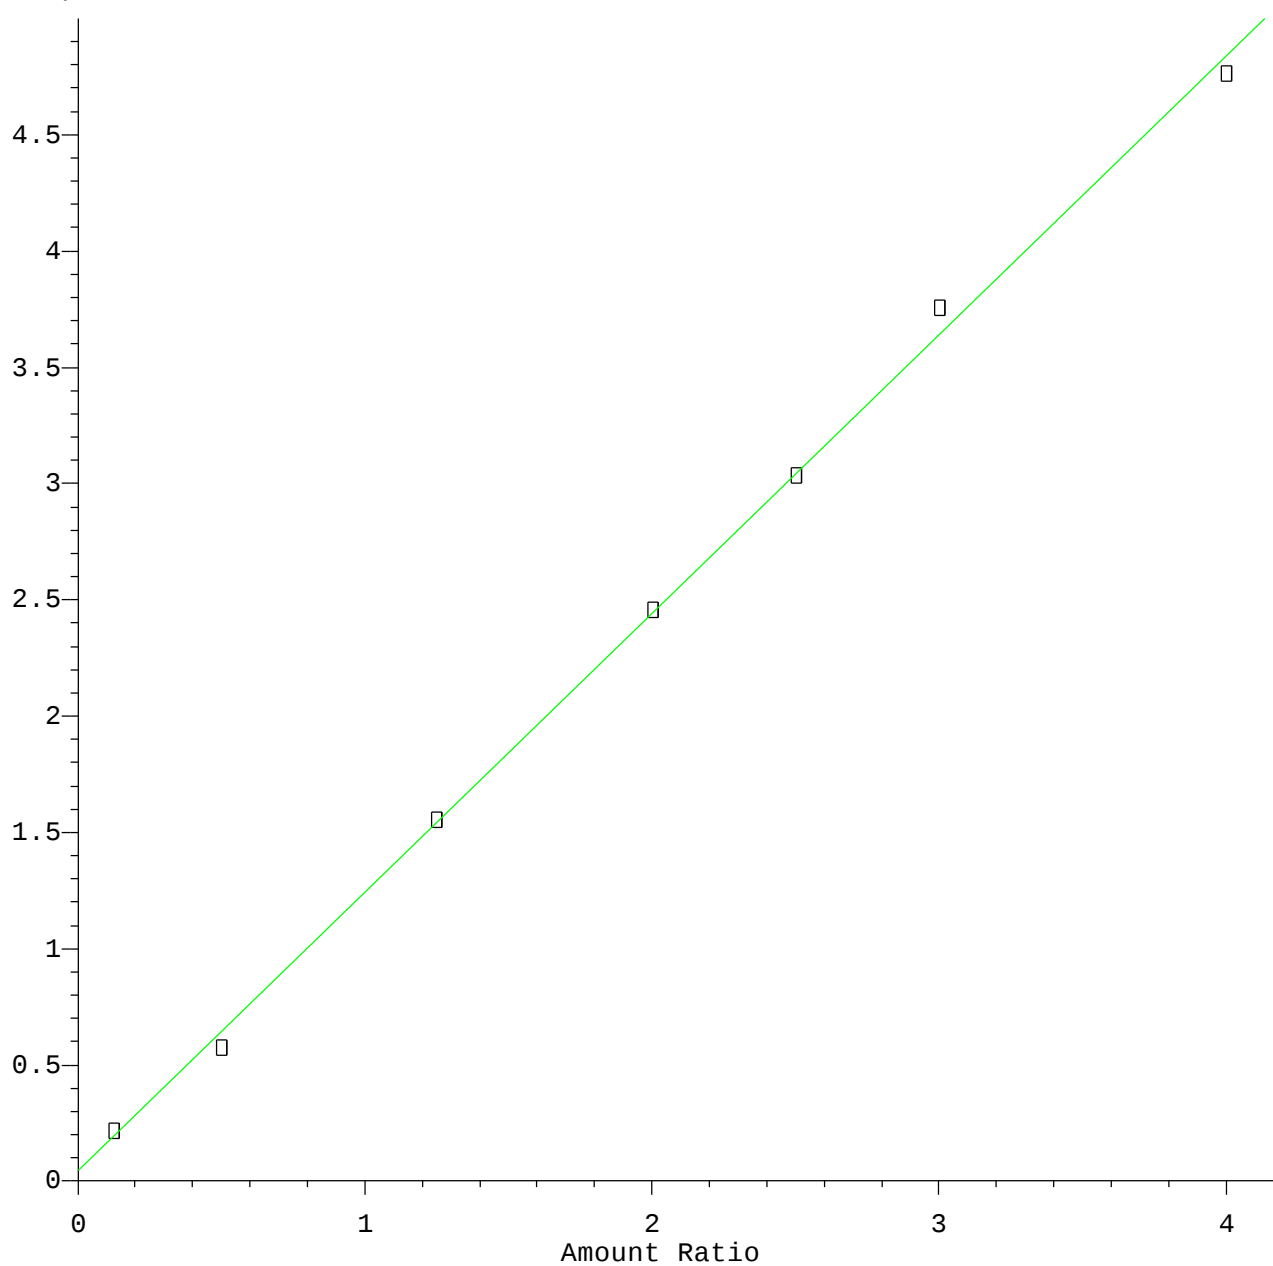

Resp Ratio = $1.20 \times 10^0 \times \text{Amt} + 4.38 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF021316.M
Calibration Table Last Updated: Sat Feb 13 00:11:18 2016

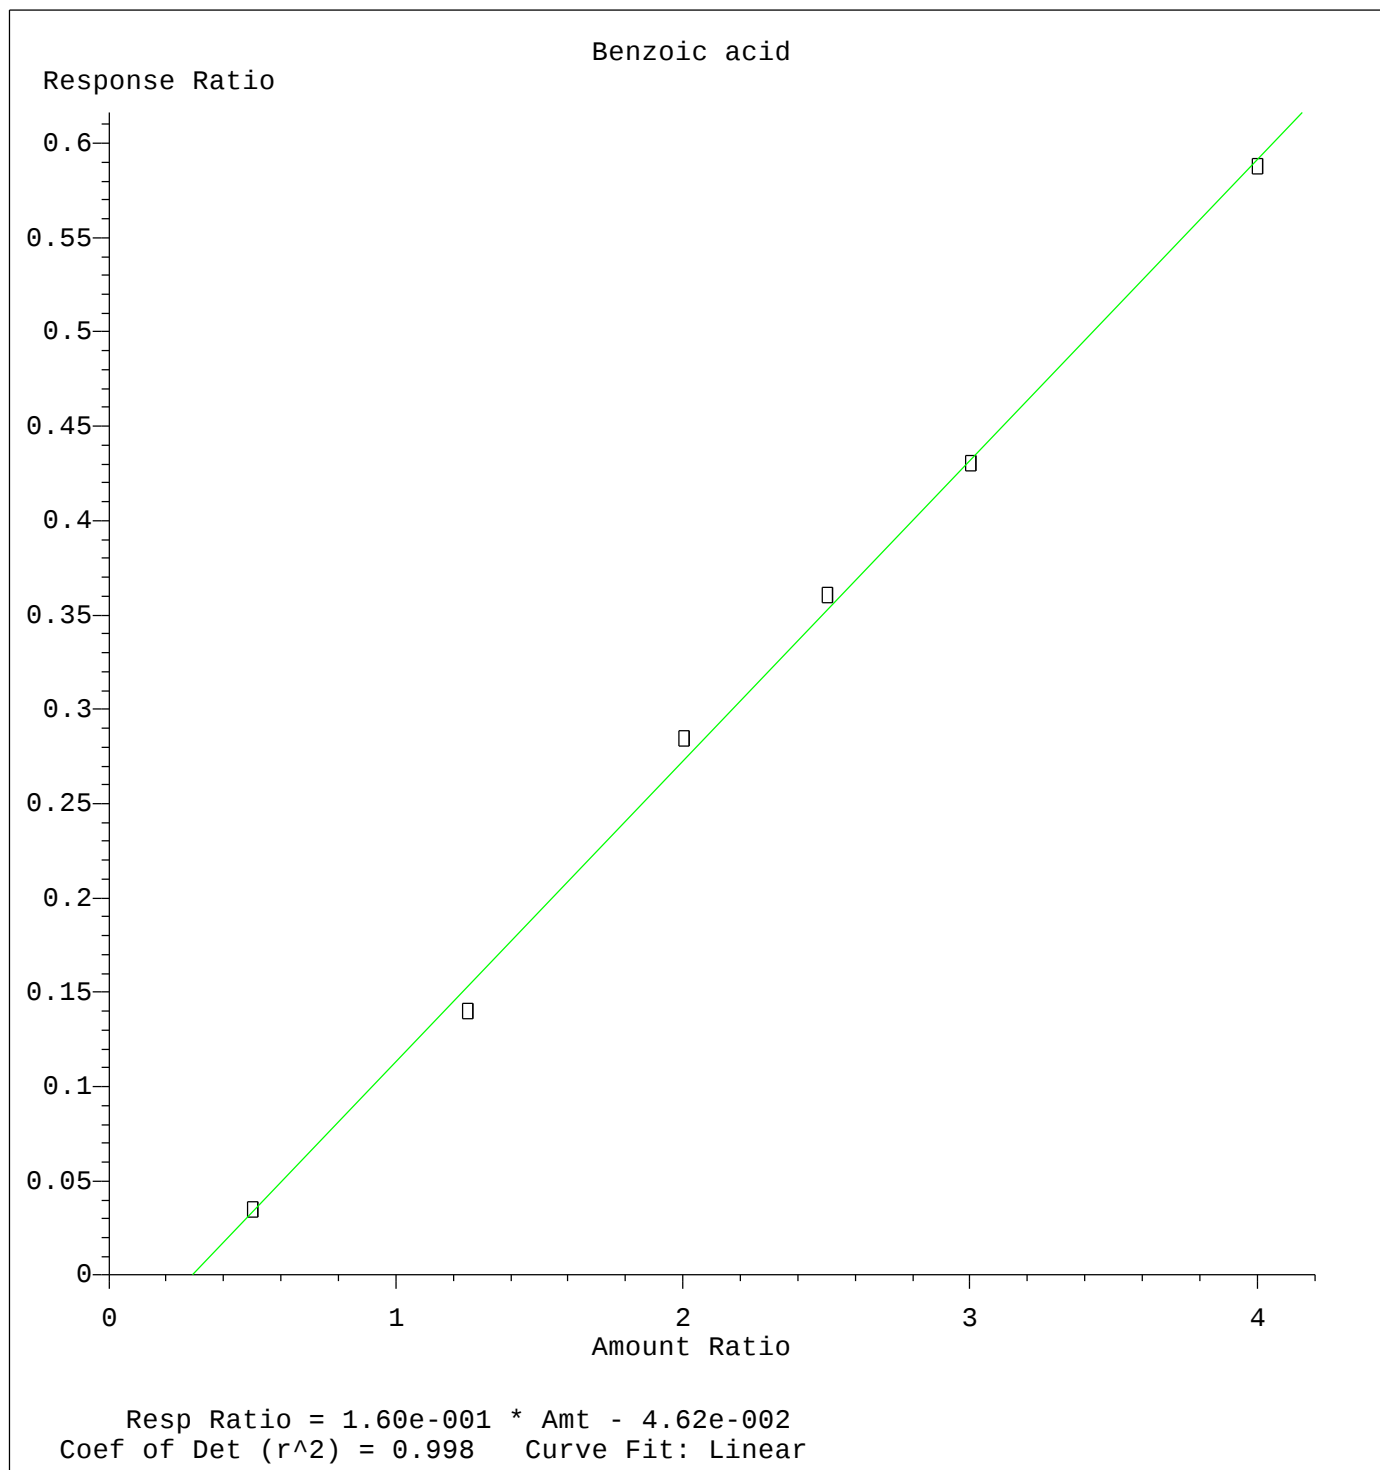

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF021316.M
Calibration Table Last Updated: Sat Feb 13 00:11:18 2016


Hexachlorocyclopentadiene

Response Ratio

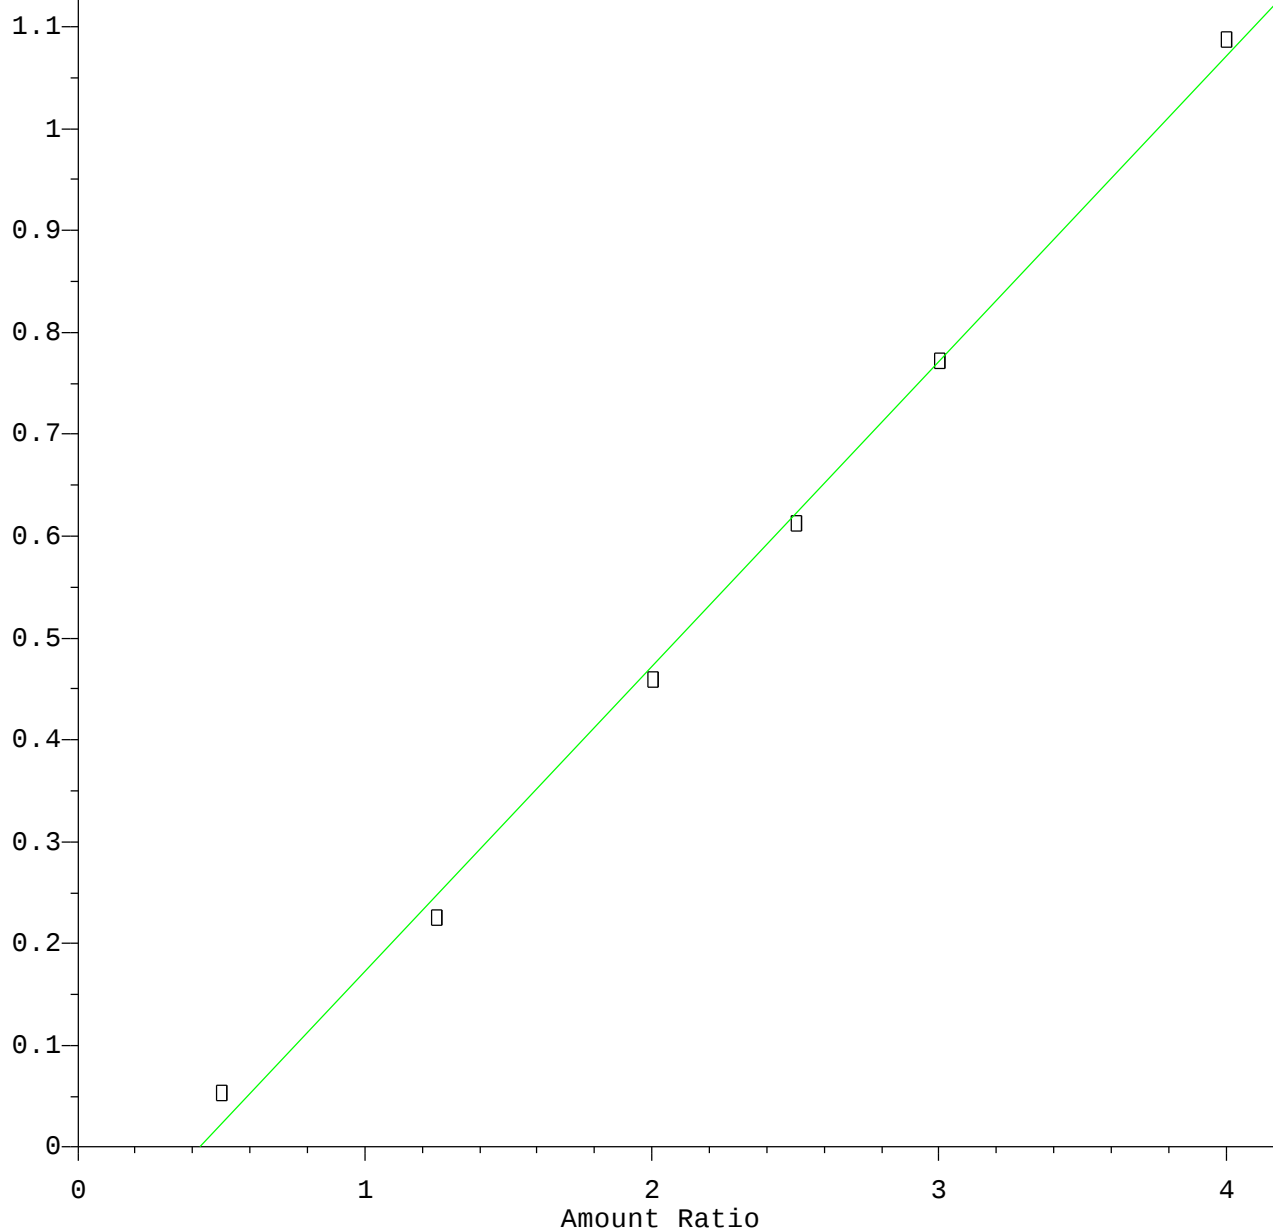


Resp Ratio = $2.99 \times 10^{-1} \times \text{Amt} - 1.26 \times 10^{-1}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF021316.M
Calibration Table Last Updated: Sat Feb 13 00:11:18 2016

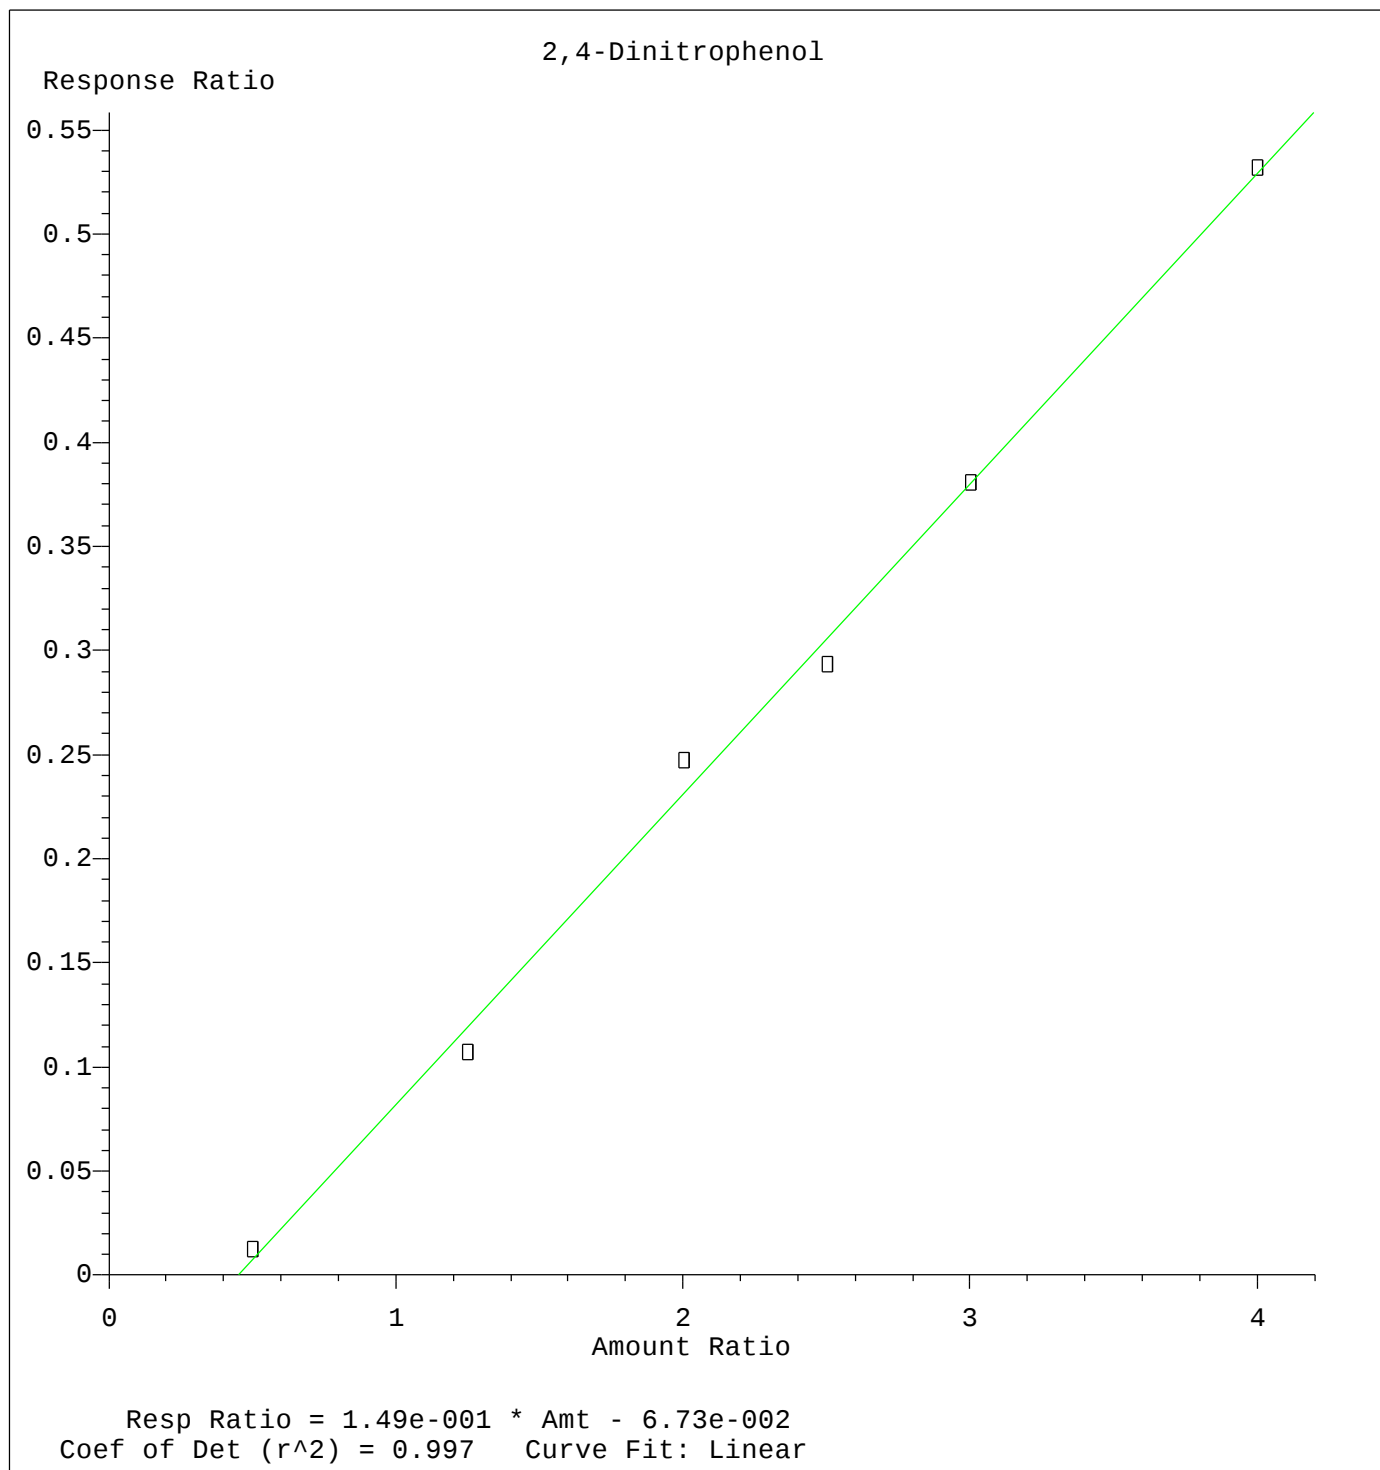


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF021316.M
Calibration Table Last Updated: Sat Feb 13 00:11:18 2016

4,6-Dinitro-2-methylphenol

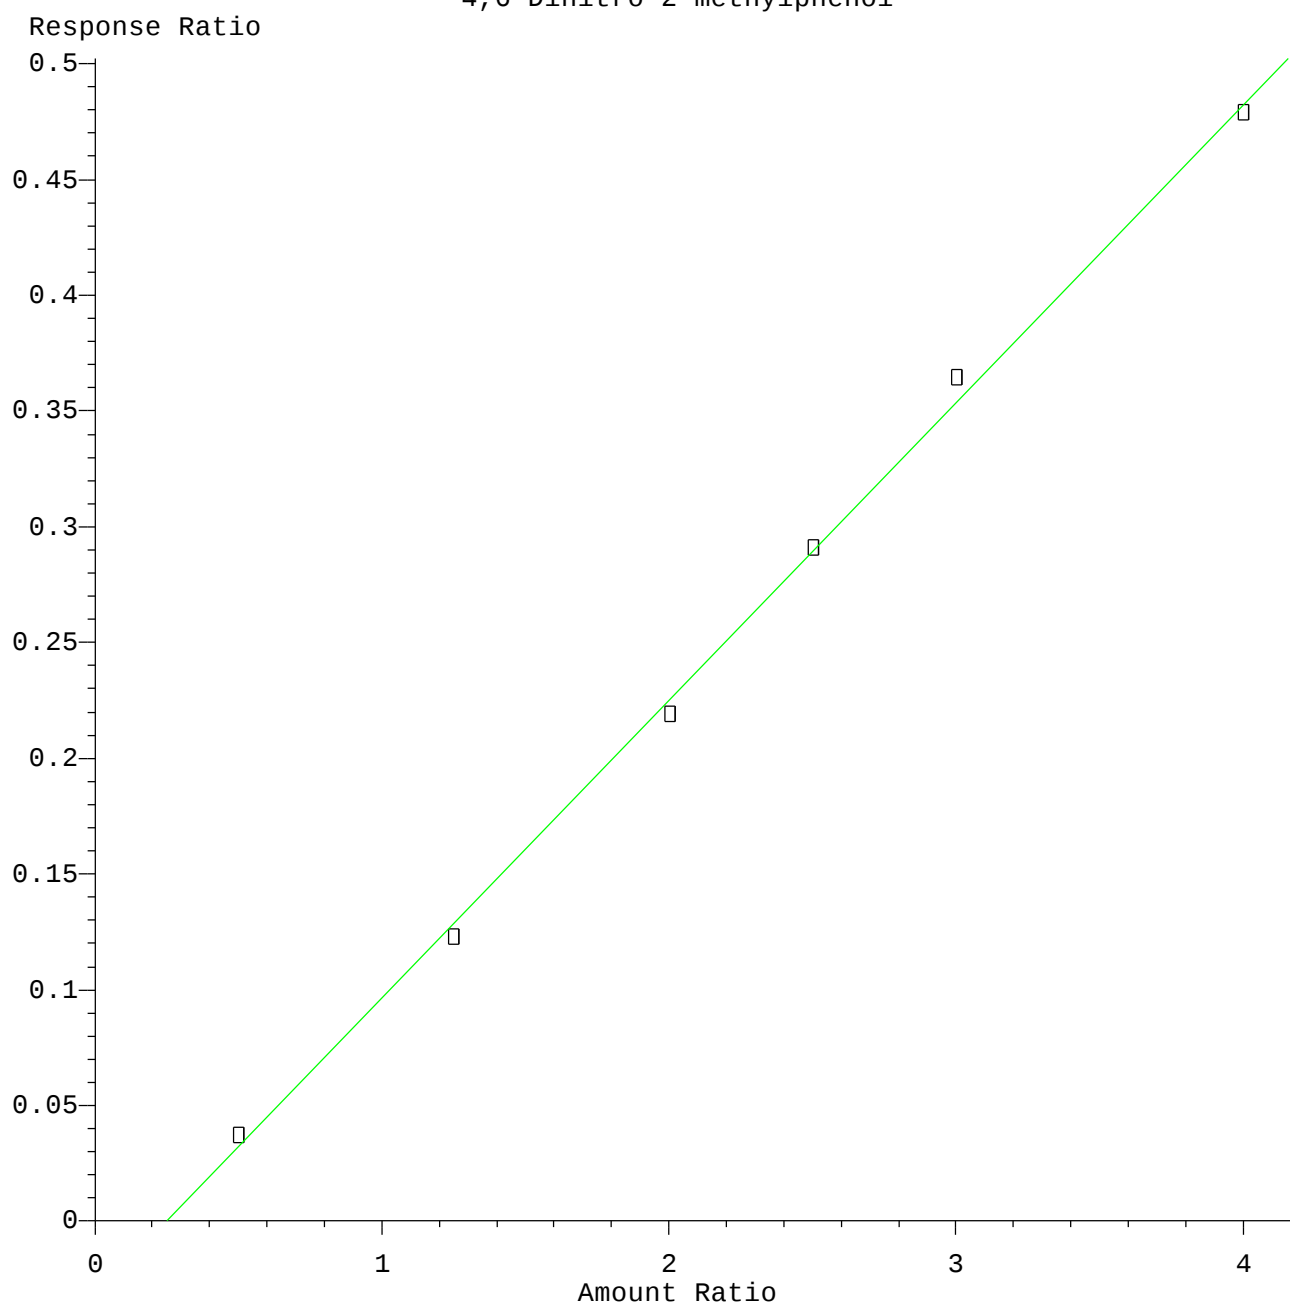


Resp Ratio = $1.29 \times 10^{-1} \times \text{Amt} - 3.23 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF021316.M
Calibration Table Last Updated: Sat Feb 13 00:11:18 2016

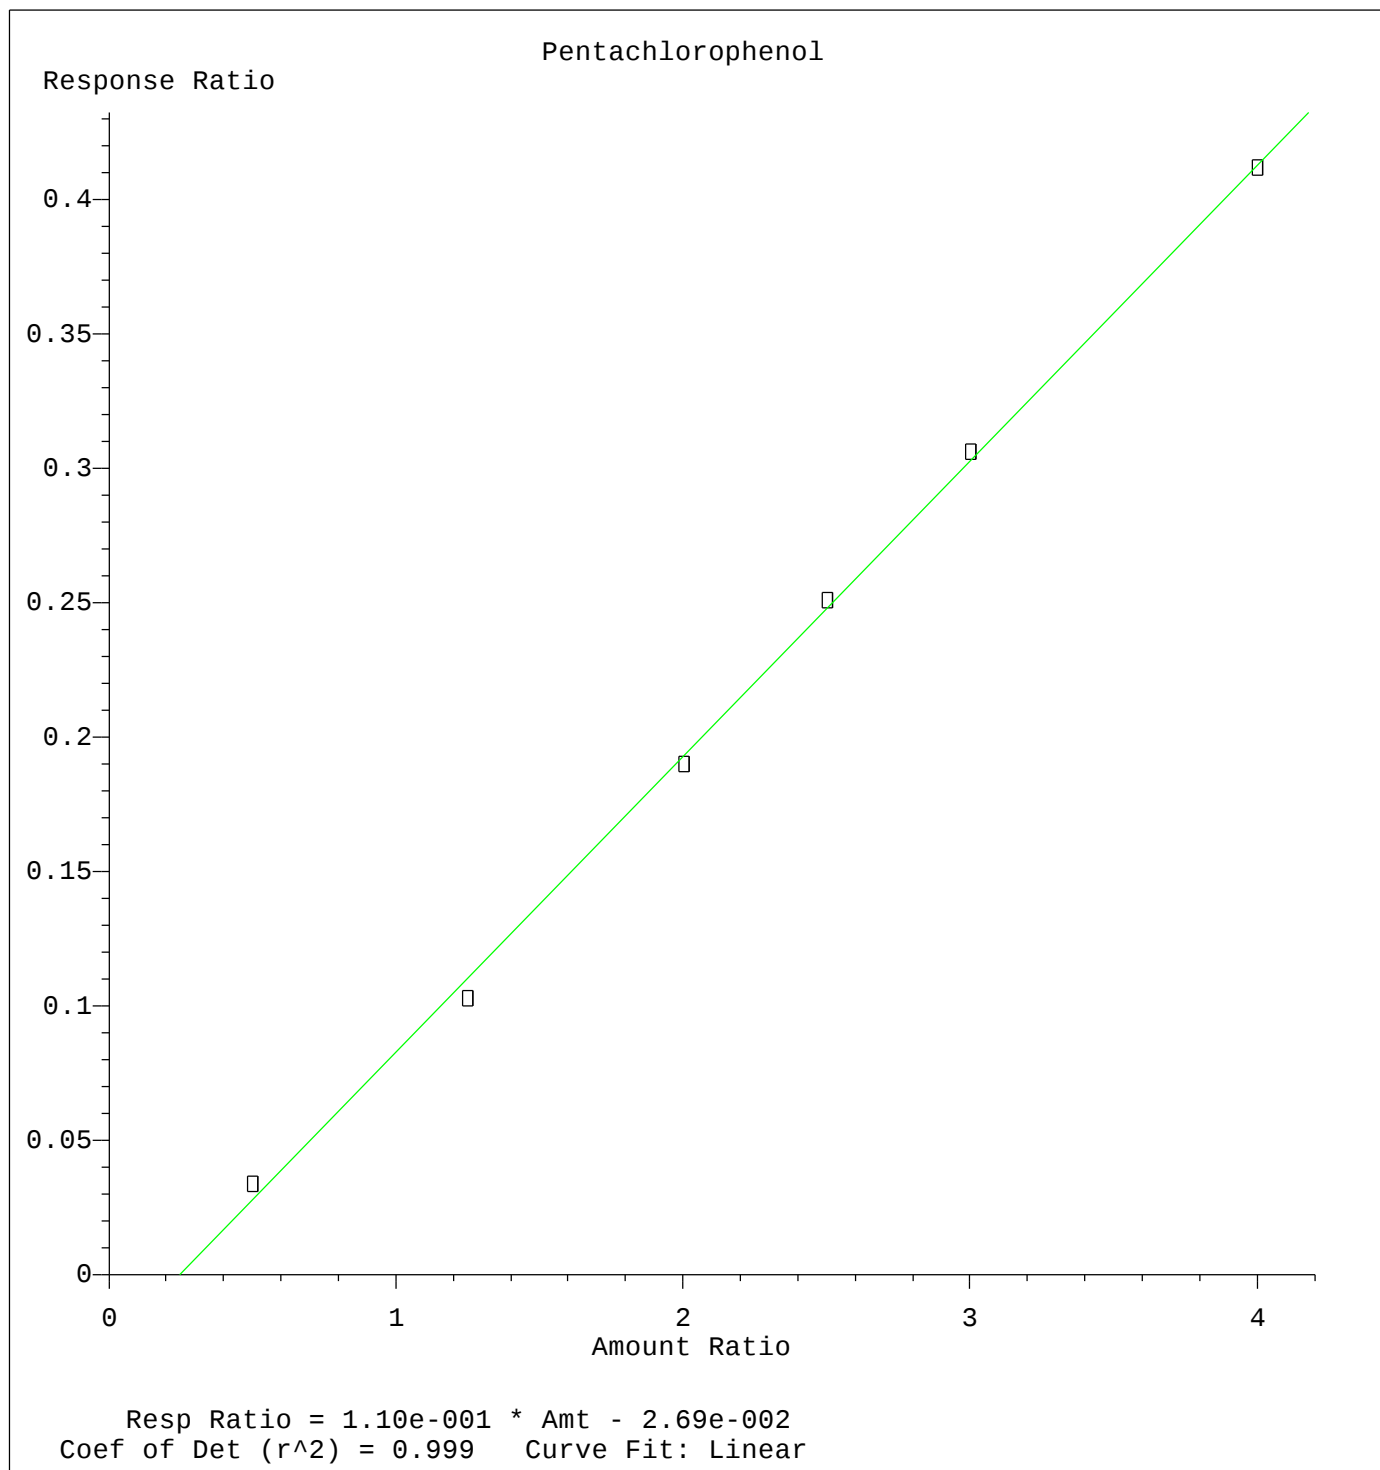

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF021316.M
Calibration Table Last Updated: Sat Feb 13 00:11:18 2016

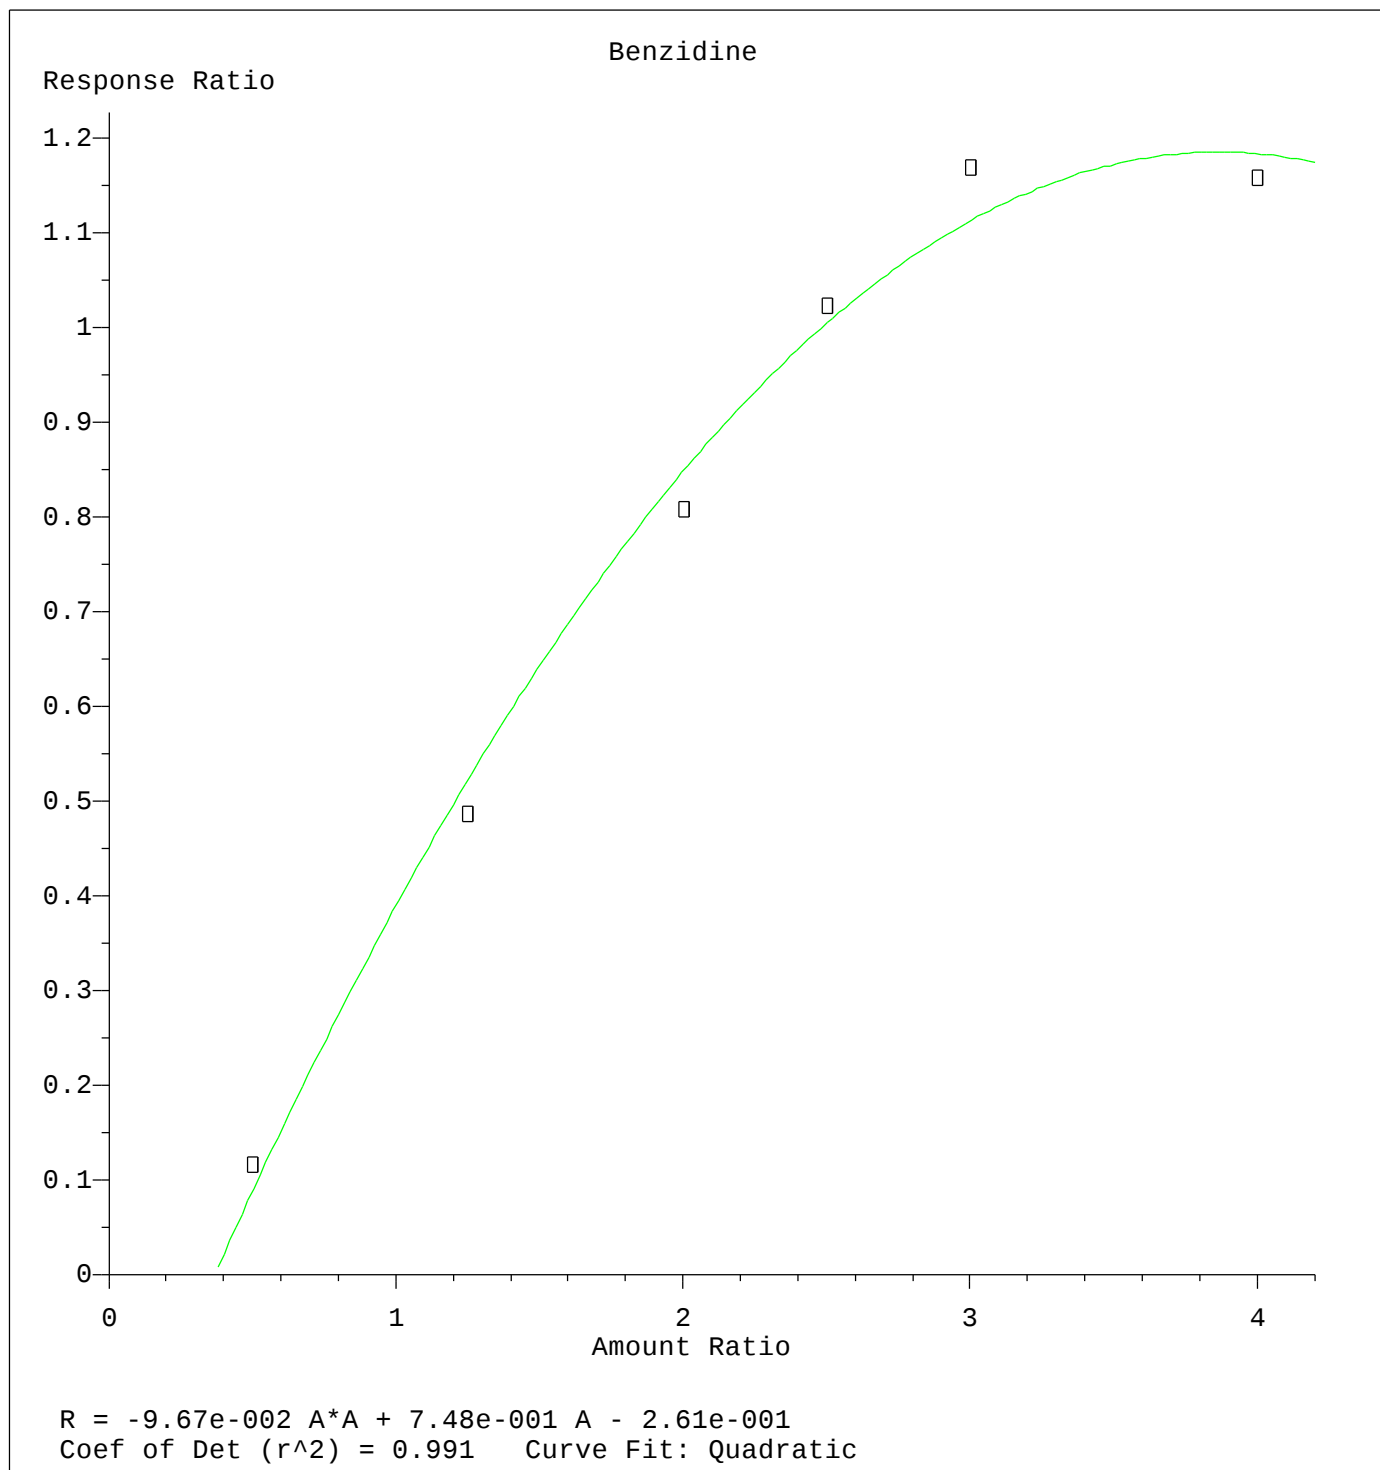

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF021316.M
Calibration Table Last Updated: Sat Feb 13 00:11:18 2016