
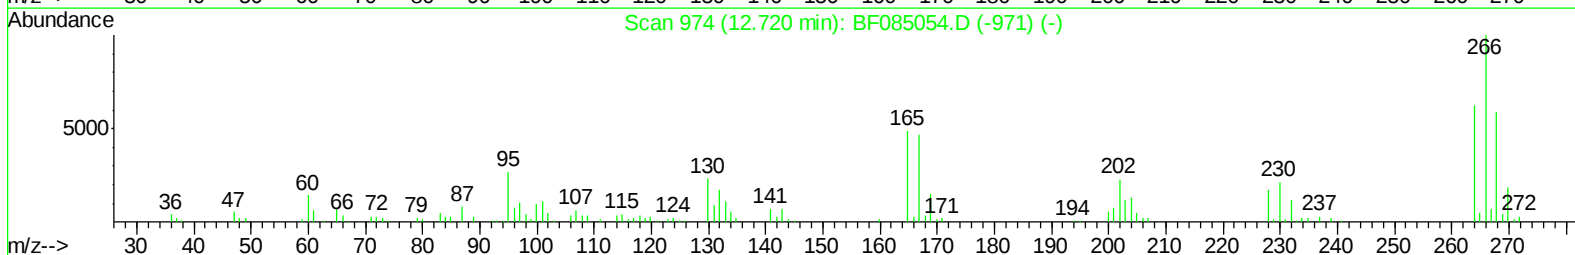
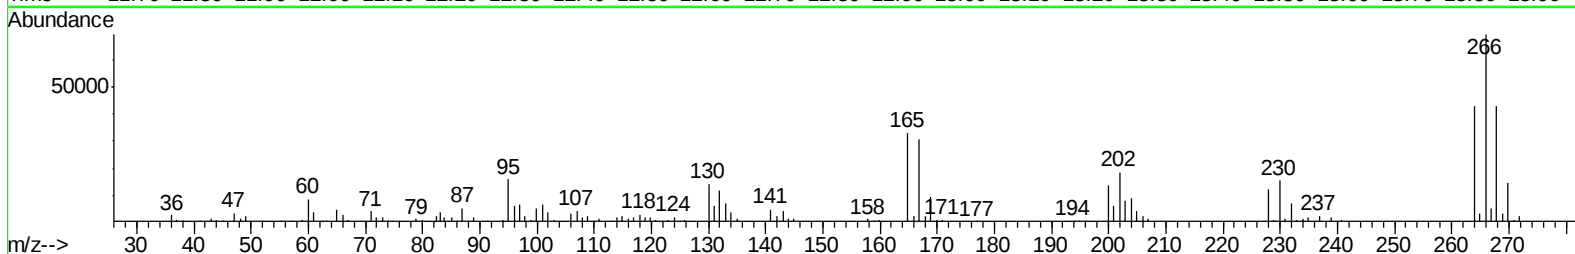


Data Path : Z:\HPCHEM1\BNA_F\Data\BF021316\
Data File : BF085050.D
Acq On : 12 Feb 2016 16:19
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 15 08:39:39 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 13 00:11:18 2016
Response via : Initial Calibration

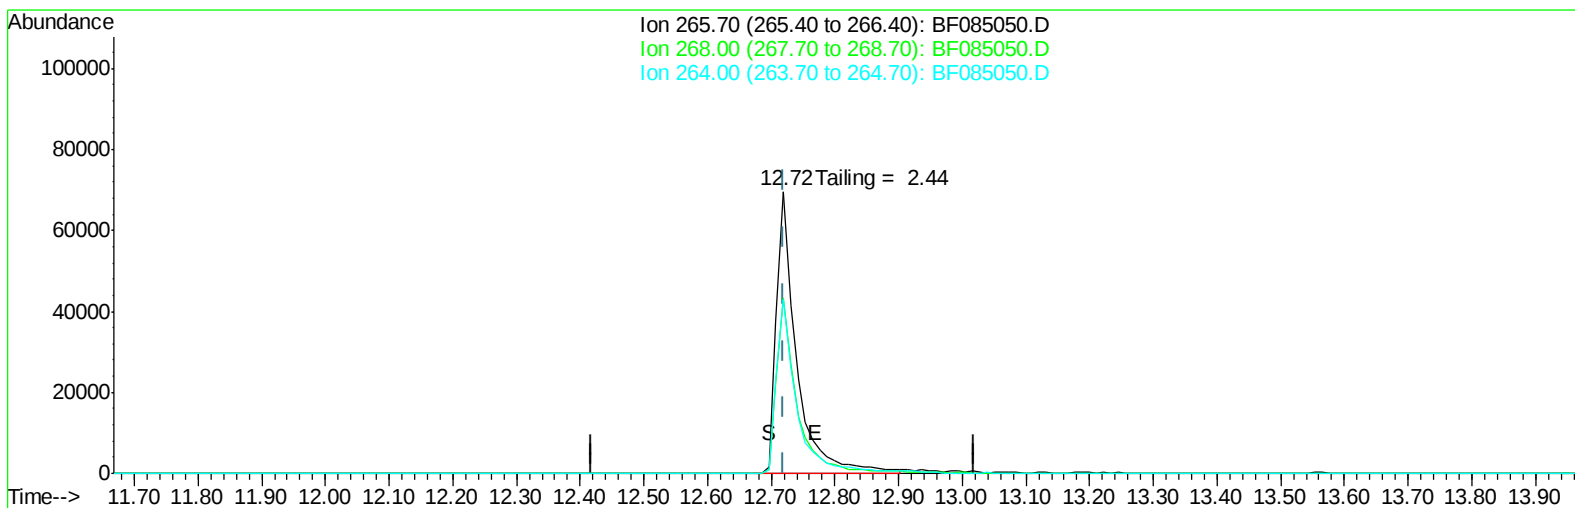

TIC: BF085050.D

(69) Pentachlorophenol (C)




12.719min (+0.000) 85088.81ng

response 154696

Ion	Exp%	Act%
265.70	100	100
268.00	59.10	62.11
264.00	62.20	61.98
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF021316\
Data File : BF085050.D
Acq On : 12 Feb 2016 16:19
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 15 08:39:39 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 13 00:11:18 2016
Response via : Initial Calibration

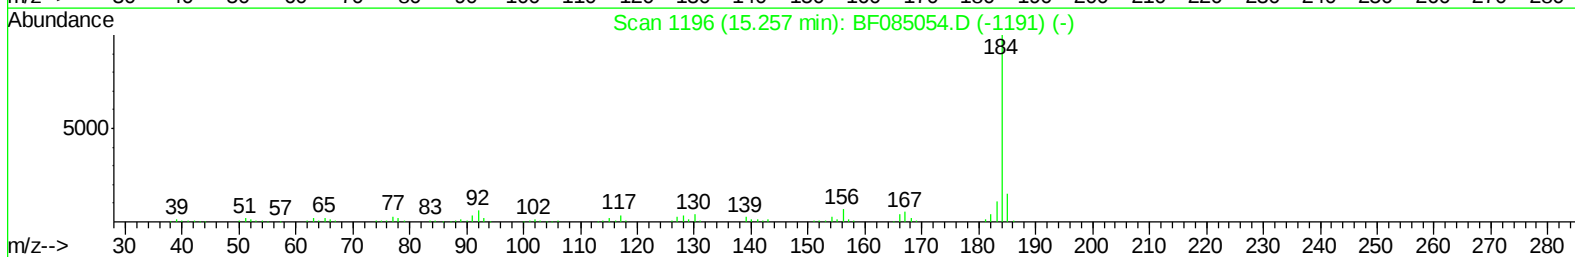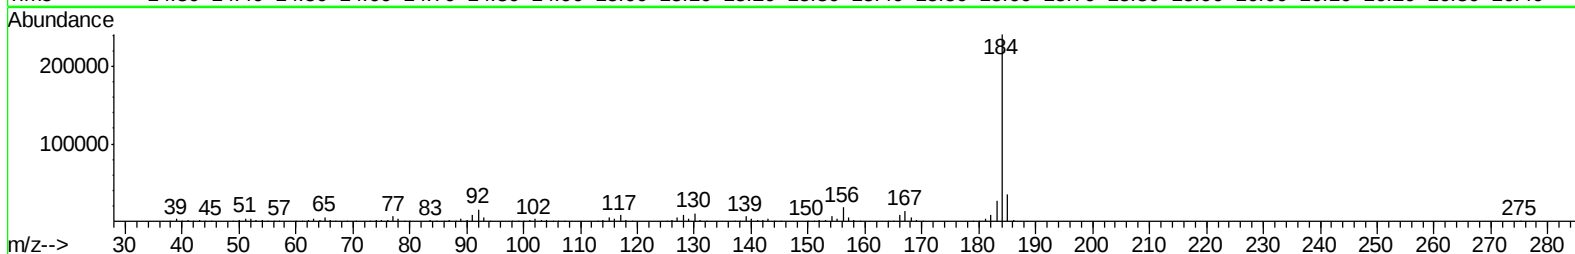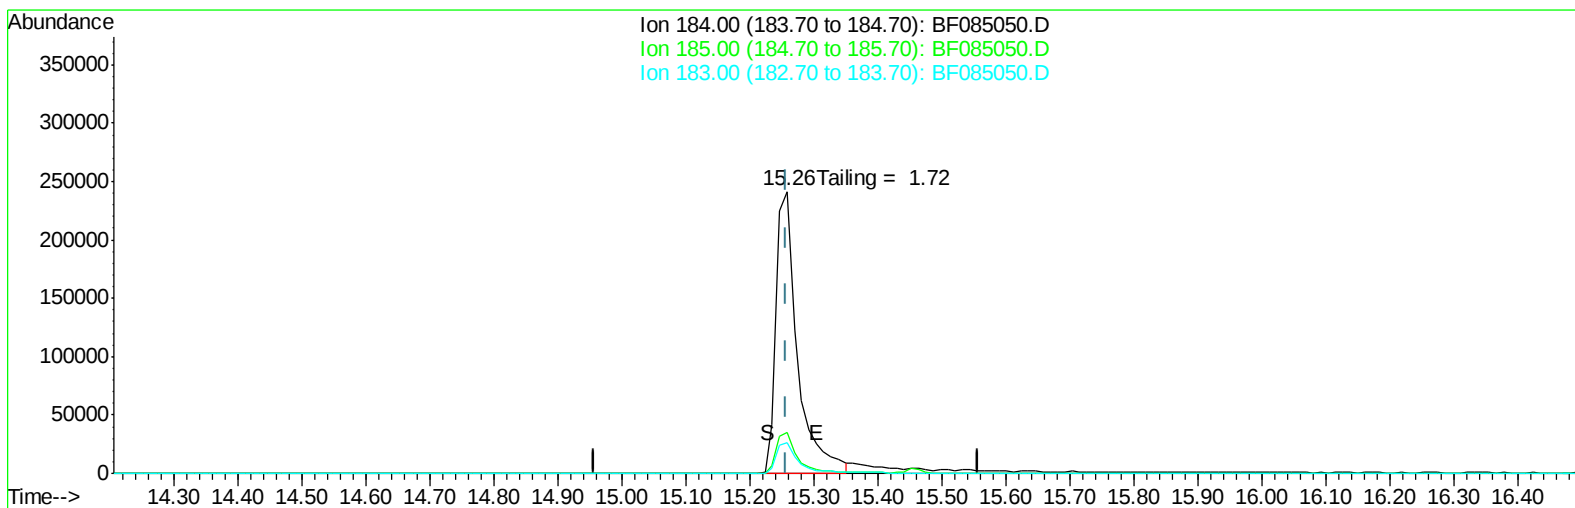

TIC: BF085050.D

(76) Benzidine

15.257min (+0.001) -20.00ng

response 598298

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.37
183.00	10.70	10.89
0.00	0.00	0.00