


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021316\
 Data File : BF085050.D
 Acq On : 12 Feb 2016 16:19
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Feb 13 00:11:18 2016

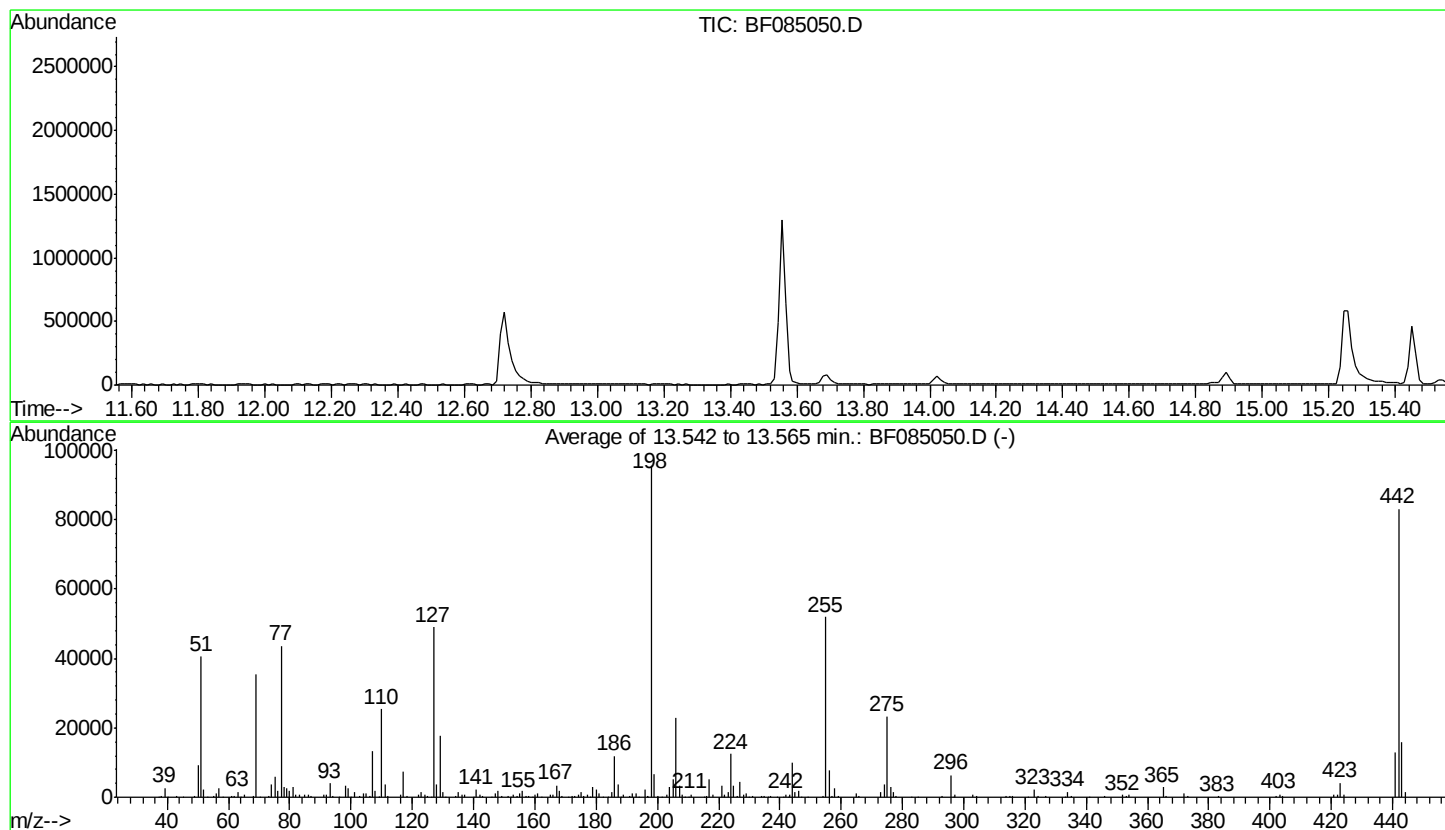

AutoFind: Scans 1046, 1047, 1048; Background Corrected with Scan 1041

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	40557	PASS
68	69	0.00	2	1.3	469	PASS
69	198	0.00	100	37.0	35330	PASS
70	69	0.00	2	0.4	129	PASS
127	198	10	80	51.2	48928	PASS
197	198	0.00	2	0.3	303	PASS
198	198	100	100	100.0	95584	PASS
199	198	5	9	6.9	6597	PASS
275	198	10	60	24.2	23138	PASS
365	198	1	100	3.1	2938	PASS
441	442	0.01	24	15.5	12865	PASS
442	198	50	100	86.9	83040	PASS
443	442	15	24	19.1	15846	PASS