
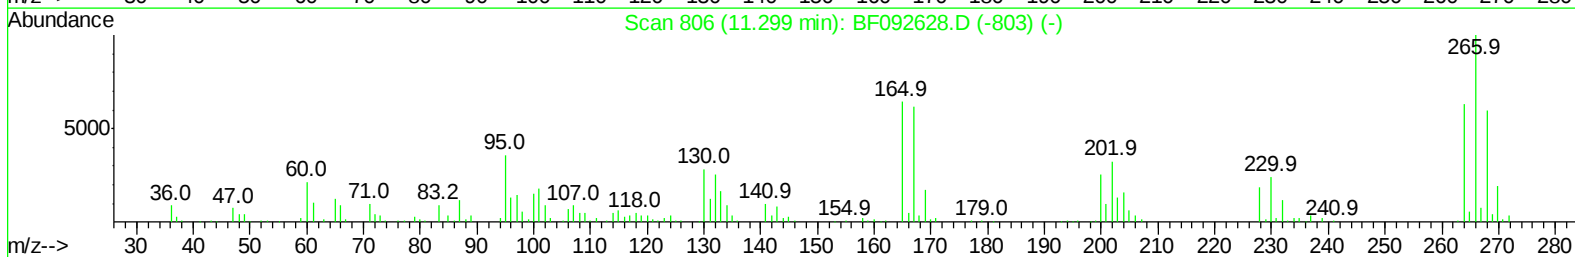
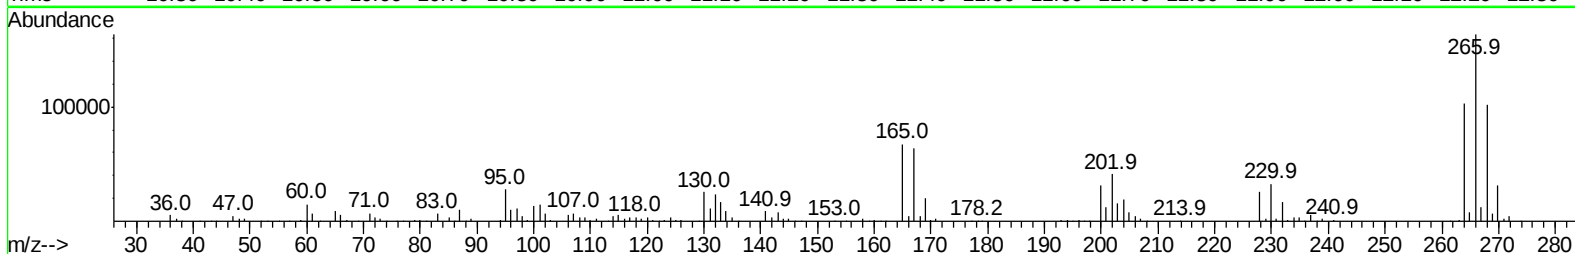


Data Path : Z:\HPCHEM1\BNA F\Data\BF021317\
Data File : BF092914.D
Acq On : 13 Feb 2017 9:54
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 12:04:49 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 30 14:50:05 2017
Response via : Initial Calibration

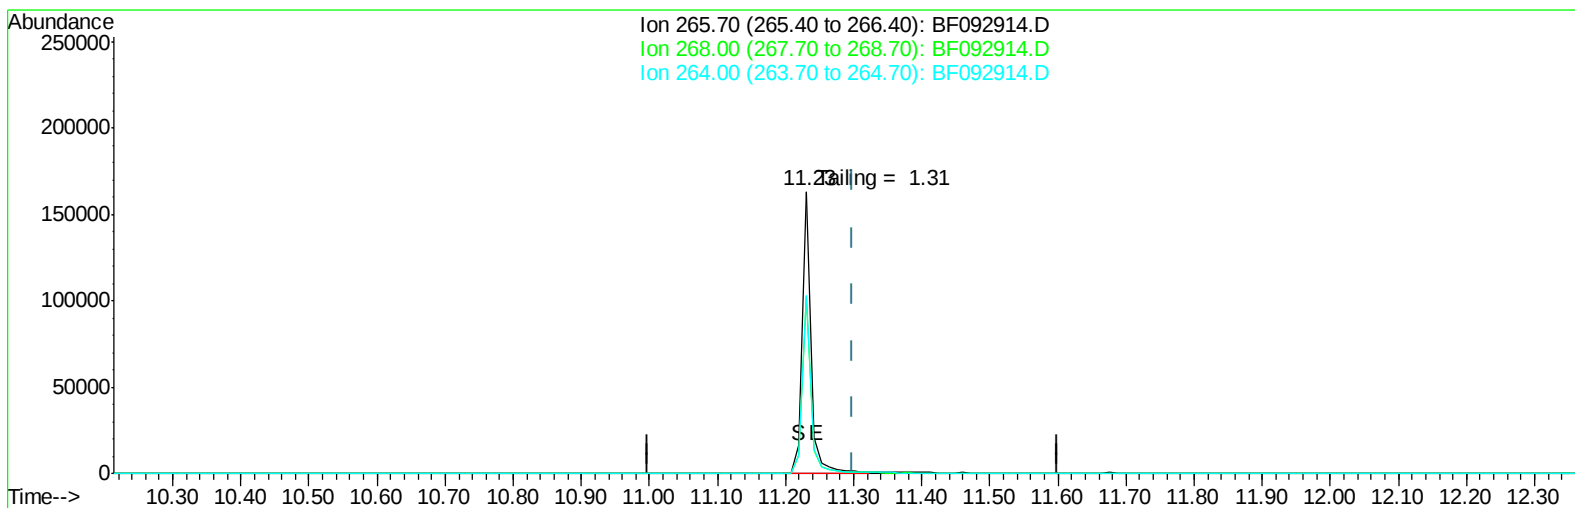

TIC: BF092914.D

(69) Pentachlorophenol (C)




11.231min (-0.068) 54434.66ng

response 150464

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	62.60
264.00	62.90	63.23
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF021317\
Data File : BF092914.D
Acq On : 13 Feb 2017 9:54
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 12:04:49 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 30 14:50:05 2017
Response via : Initial Calibration

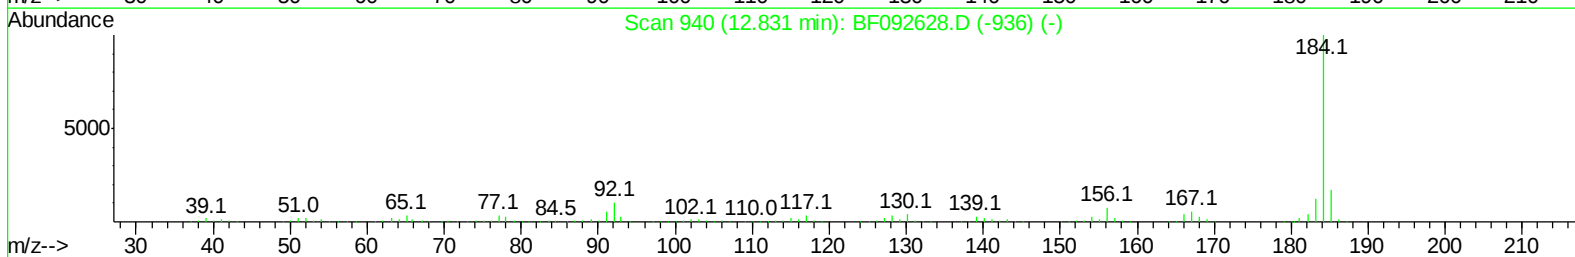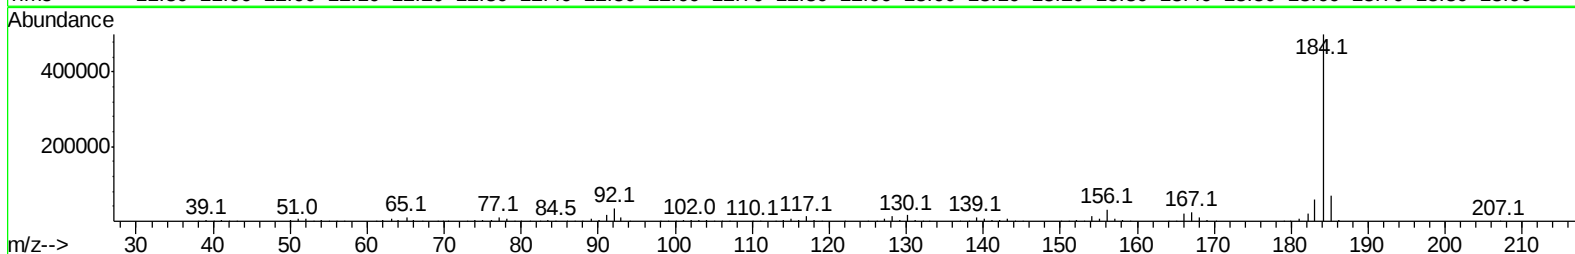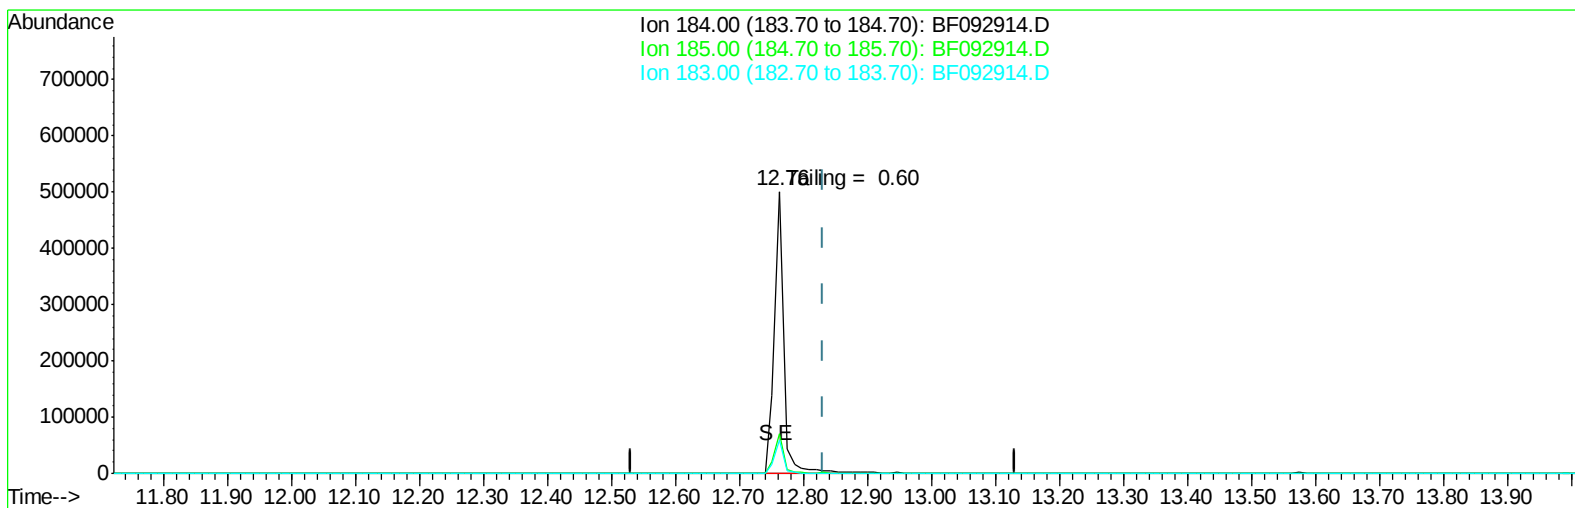

TIC: BF092914.D

(76) Benzidine

12.762min (-0.069) 0.00ng

response 515014

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	13.96
183.00	11.50	12.01
0.00	0.00	0.00