

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021317\
 Data File : BF092930.D
 Acq On : 13 Feb 2017 20:45
 Operator : SJ/MA
 Sample : I1799-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.059	258	260	271	rBV	1127336	1483348	38.03%	4.342%
2	5.481	294	297	300	rBV	3130201	3176006	81.43%	9.296%
3	6.510	384	387	390	rBV	2430768	3588499	92.01%	10.503%
4	6.647	396	399	401	rBV	3579826	3365881	86.30%	9.851%
5	6.876	417	419	422	rBV	1040930	884172	22.67%	2.588%
6	7.036	430	433	435	rBV	2863495	2633177	67.52%	7.707%
7	7.447	466	469	471	rBV	2050600	2296796	58.89%	6.722%
8	8.167	529	532	534	rBV	1079033	1165710	29.89%	3.412%
9	9.242	623	626	628	rBV	3587611	3900095	100.00%	11.415%
10	9.630	658	660	662	rBV	322677	261579	6.71%	0.766%
11	9.916	682	685	687	rBV	1599080	1384823	35.51%	4.053%
12	10.339	721	722	724	rVB	54436	64688	1.66%	0.189%
13	10.568	739	742	745	rBV	26483	48117	1.23%	0.141%
14	10.705	751	754	757	rBV	2157770	2124663	54.48%	6.219%
15	10.819	762	764	769	rVB	101621	128401	3.29%	0.376%
16	11.265	801	803	805	rBV	76159	75472	1.94%	0.221%
17	11.402	813	815	817	rBV	1495254	1375621	35.27%	4.026%
18	12.991	951	954	956	rBV	3217323	3678221	94.31%	10.766%
19	13.894	1030	1033	1041	rBV2	40203	123703	3.17%	0.362%
20	14.031	1043	1045	1048	rVB	920383	1284813	32.94%	3.760%
21	15.482	1168	1172	1174	rBV	729990	1122536	28.78%	3.286%


Sum of corrected areas: 34166321

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021317\
Data File : BF092930.D
Acq On : 13 Feb 2017 20:45
Operator : SJ/MA
Sample : I1799-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

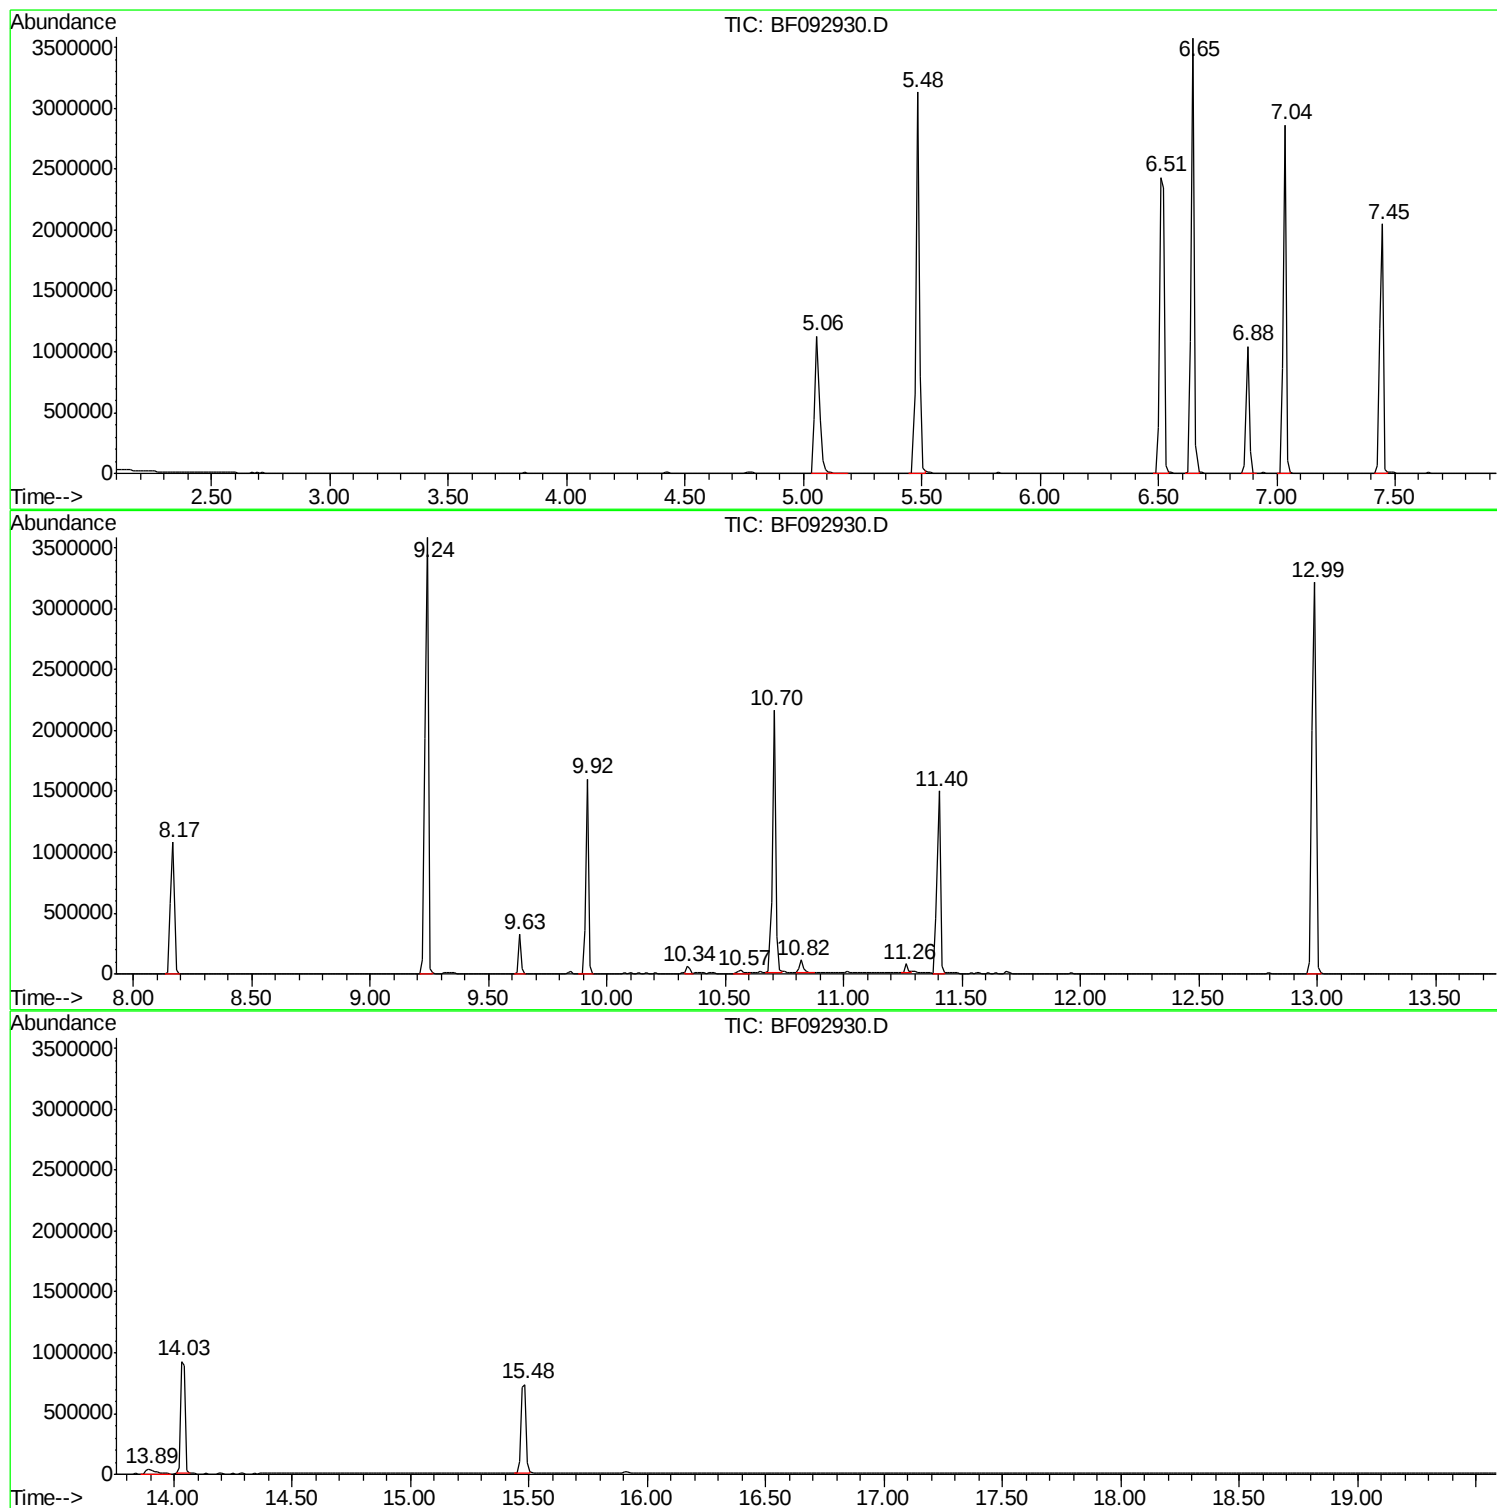

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021317\
Data File : BF092930.D
Acq On : 13 Feb 2017 20:45
Operator : SJ/MA
Sample : I1799-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-3









Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.06	33.55 ng	1483350	1,4-Dichlorobenzene-d4	6.88

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
2			3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33
3			2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	33
4			Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	33
5			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23

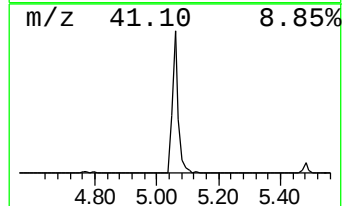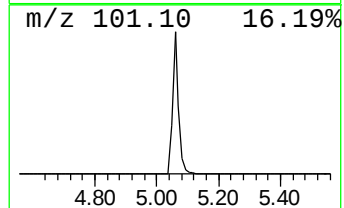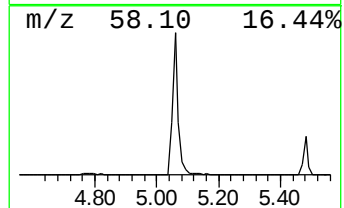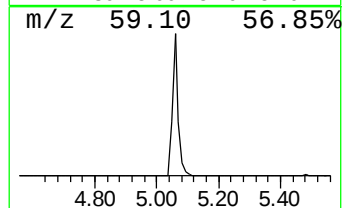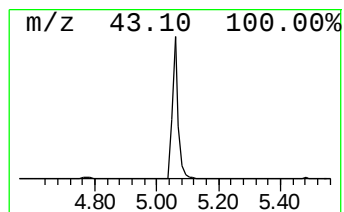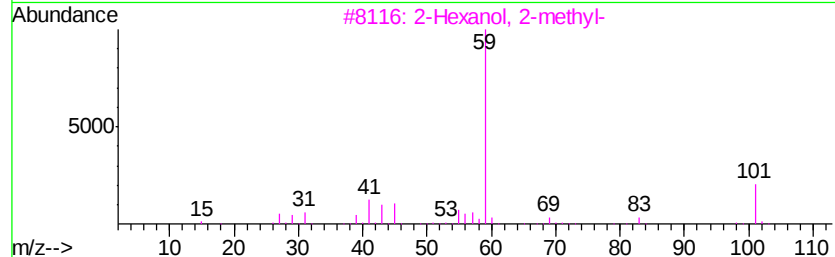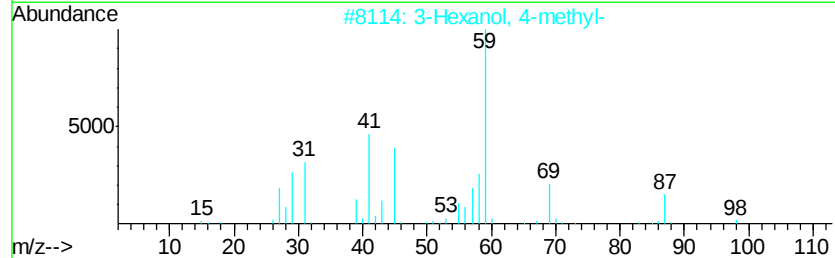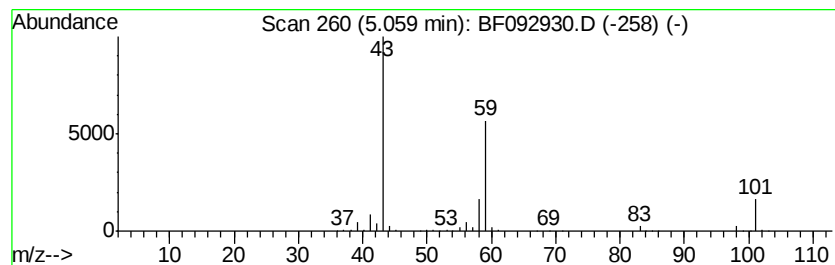

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021317\
Data File : BF092930.D
Acq On : 13 Feb 2017 20:45
Operator : SJ/MA
Sample : I1799-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-3










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.65 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.65	76.14 ng	3365880	1,4-Dichlorobenzene-d4	6.88

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		Imidazole, 4,5-dicyano-1-methyl-	132	C6H4N4	019485-35-9	9

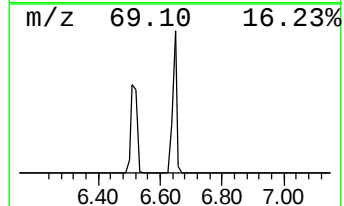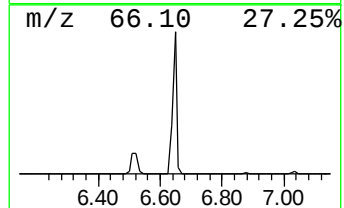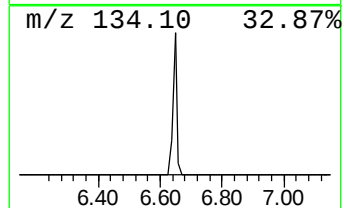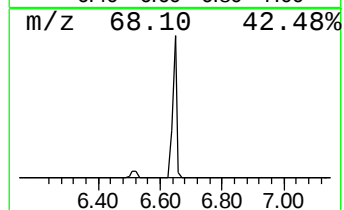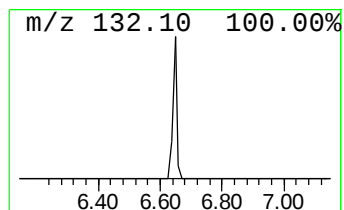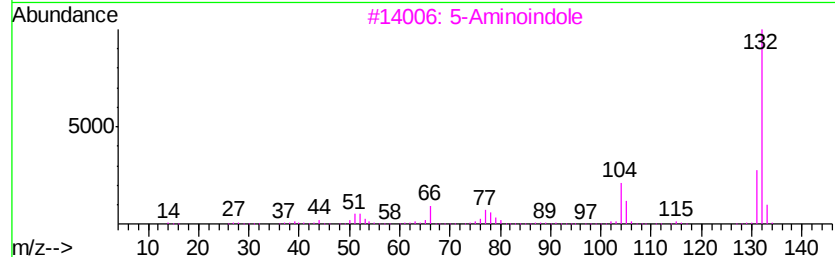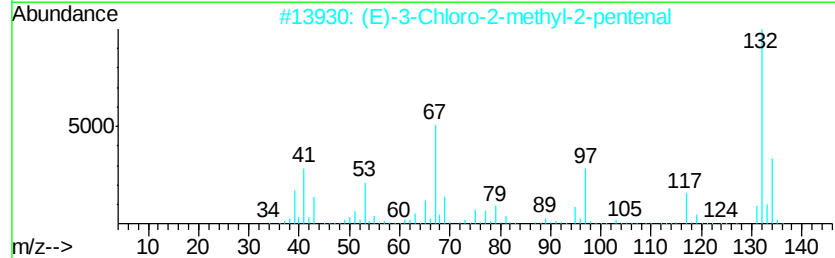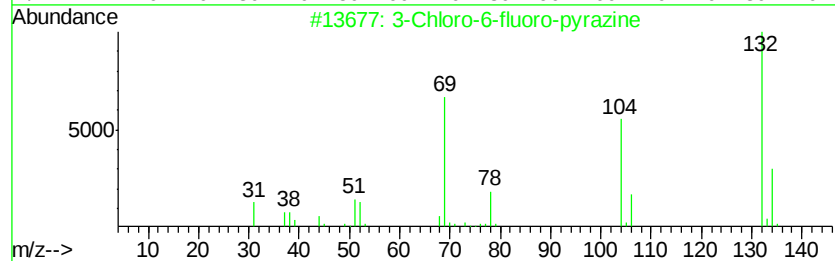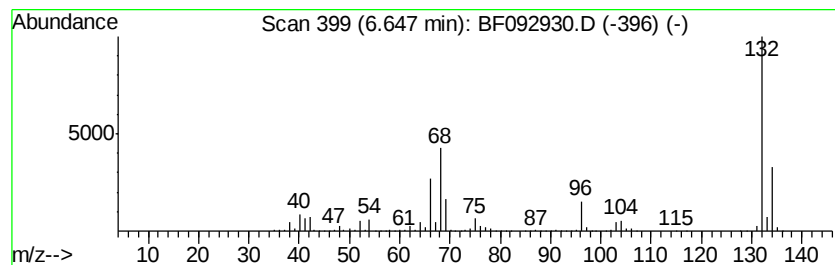

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021317\
Data File : BF092930.D
Acq On : 13 Feb 2017 20:45
Operator : SJ/MA
Sample : I1799-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.06	33.5	ng	1483350	1	6.88	884172	20.0
unknown6.65	6.65	76.1	ng	3365880	1	6.88	884172	20.0