


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021317\
 Data File : BF092914.D
 Acq On : 13 Feb 2017 9:54
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 13 18:04:38 2017

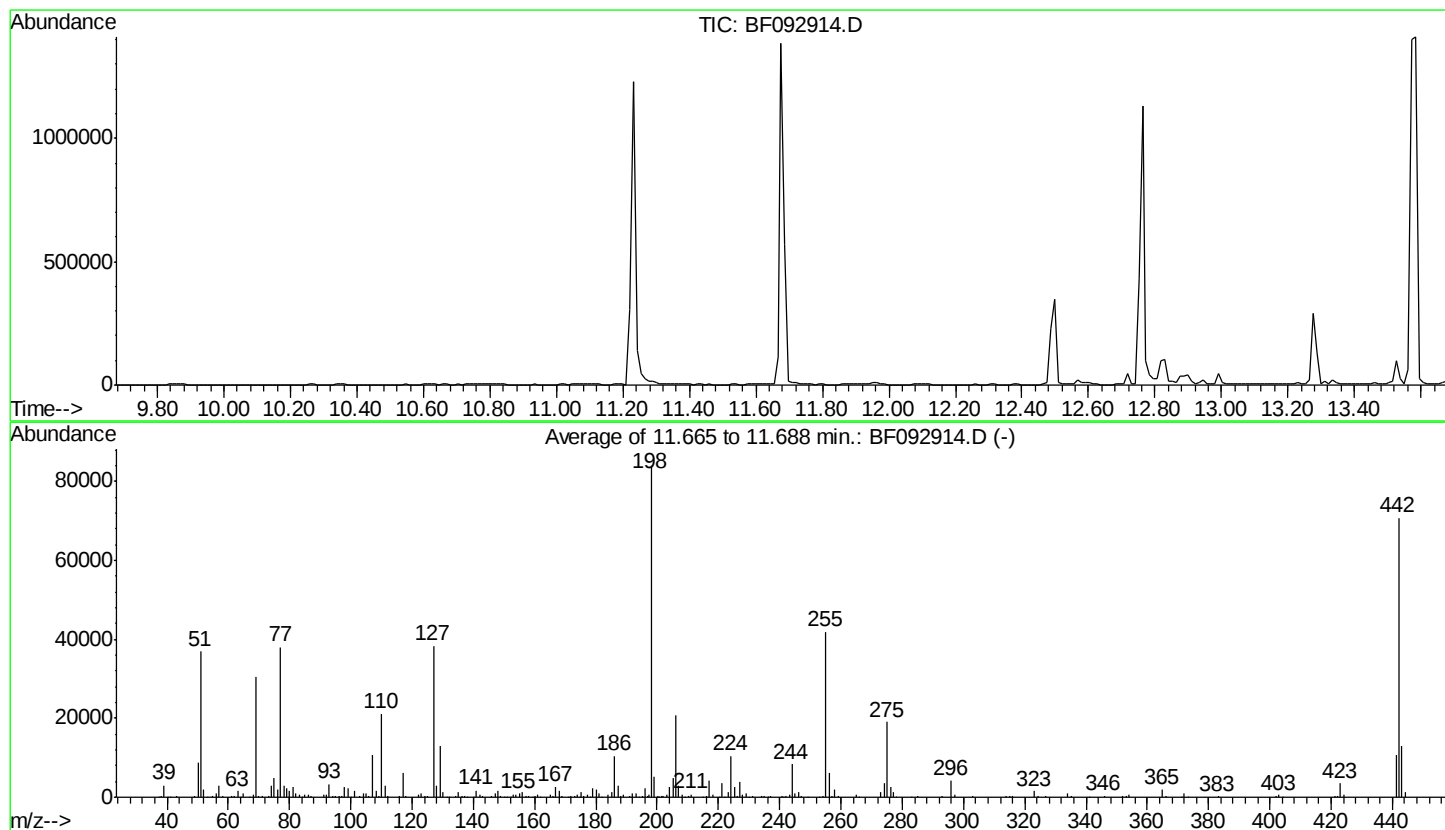

AutoFind: Scans 838, 839, 840; Background Corrected with Scan 835

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	36879	PASS
68	69	0.00	2	1.9	570	PASS
69	198	0.00	100	36.2	30390	PASS
70	69	0.00	2	0.6	177	PASS
127	198	10	80	45.6	38348	PASS
197	198	0.00	2	0.9	734	PASS
198	198	100	100	100.0	84005	PASS
199	198	5	9	6.4	5359	PASS
275	198	10	60	22.7	19033	PASS
365	198	1	100	2.2	1825	PASS
441	442	0.01	24	15.1	10683	PASS
442	198	50	100	84.3	70789	PASS
443	442	15	24	18.2	12874	PASS