


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021317\
 Data File : BF092917.D
 Acq On : 13 Feb 2017 14:17
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 13 18:04:38 2017

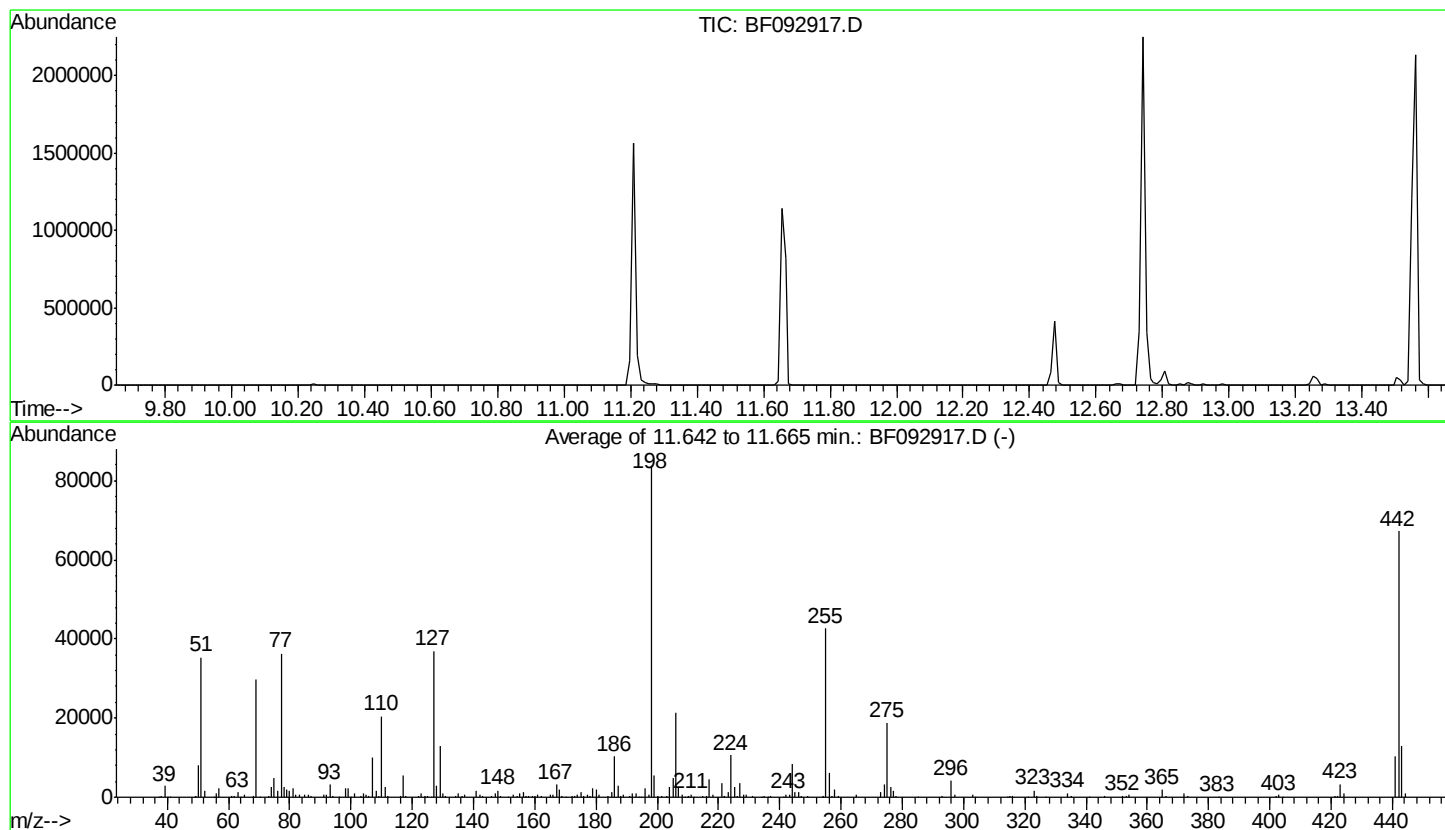

AutoFind: Scans 836, 837, 838; Background Corrected with Scan 833

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	35295	PASS
68	69	0.00	2	1.7	491	PASS
69	198	0.00	100	35.4	29619	PASS
70	69	0.00	2	0.6	164	PASS
127	198	10	80	44.1	36964	PASS
197	198	0.00	2	0.8	682	PASS
198	198	100	100	100.0	83781	PASS
199	198	5	9	6.7	5583	PASS
275	198	10	60	22.5	18834	PASS
365	198	1	100	2.2	1851	PASS
441	442	0.01	24	15.3	10275	PASS
442	198	50	100	80.1	67122	PASS
443	442	15	24	19.1	12808	PASS