


Data Path : Z:\HPCHEM1\BNA_F\Data\BF021318\
 Data File : BF102951.D
 Acq On : 13 Feb 2018 10:19
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 16 14:34:49 2018

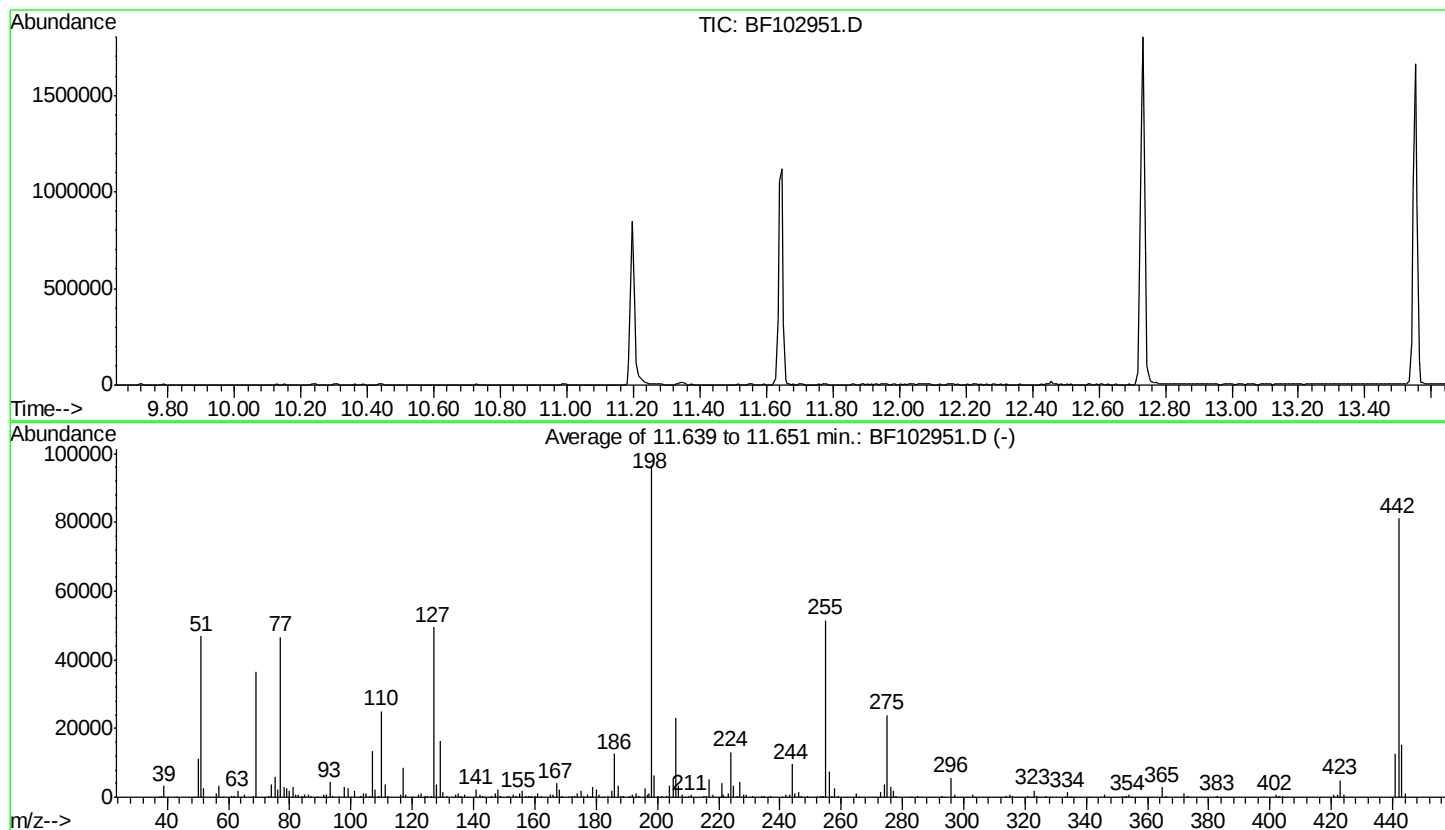

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.5	46785	PASS
68	69	0.00	2	1.4	526	PASS
69	198	0.00	100	37.9	36581	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.3	49493	PASS
197	198	0.00	2	1.1	1084	PASS
198	198	100	100	100.0	96472	PASS
199	198	5	9	6.7	6456	PASS
275	198	10	60	24.7	23857	PASS
365	198	1	100	3.1	2978	PASS
441	443	0.01	100	82.5	12521	PASS
442	198	50	100	84.0	81045	PASS
443	442	15	24	18.7	15184	PASS