
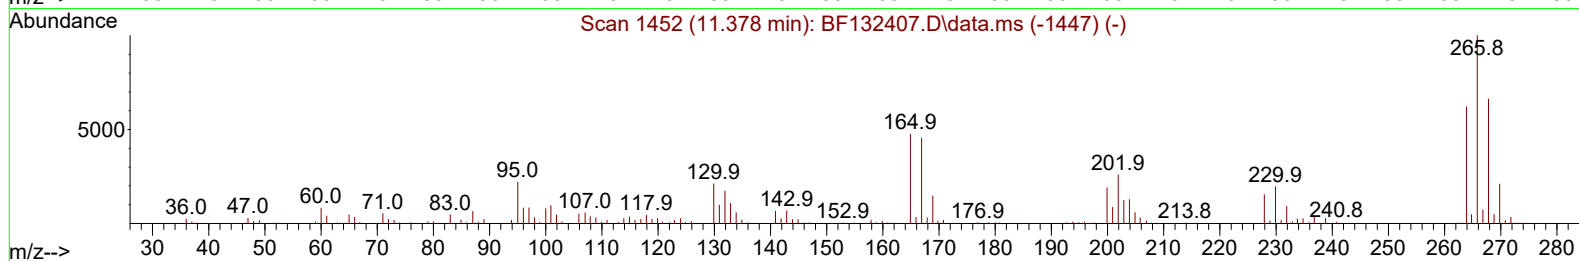
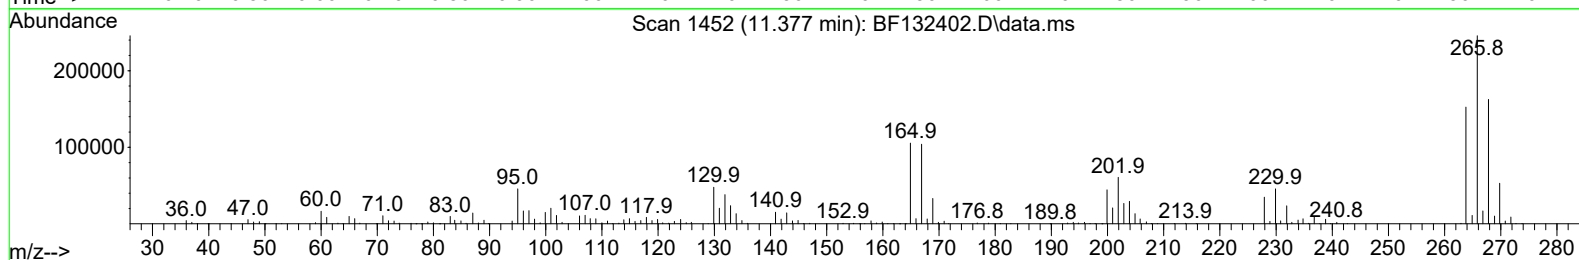


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021323\
Data File : BF132402.D
Acq On : 13 Feb 2023 10:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 04:14:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 14 00:51:00 2023
Response via : Initial Calibration

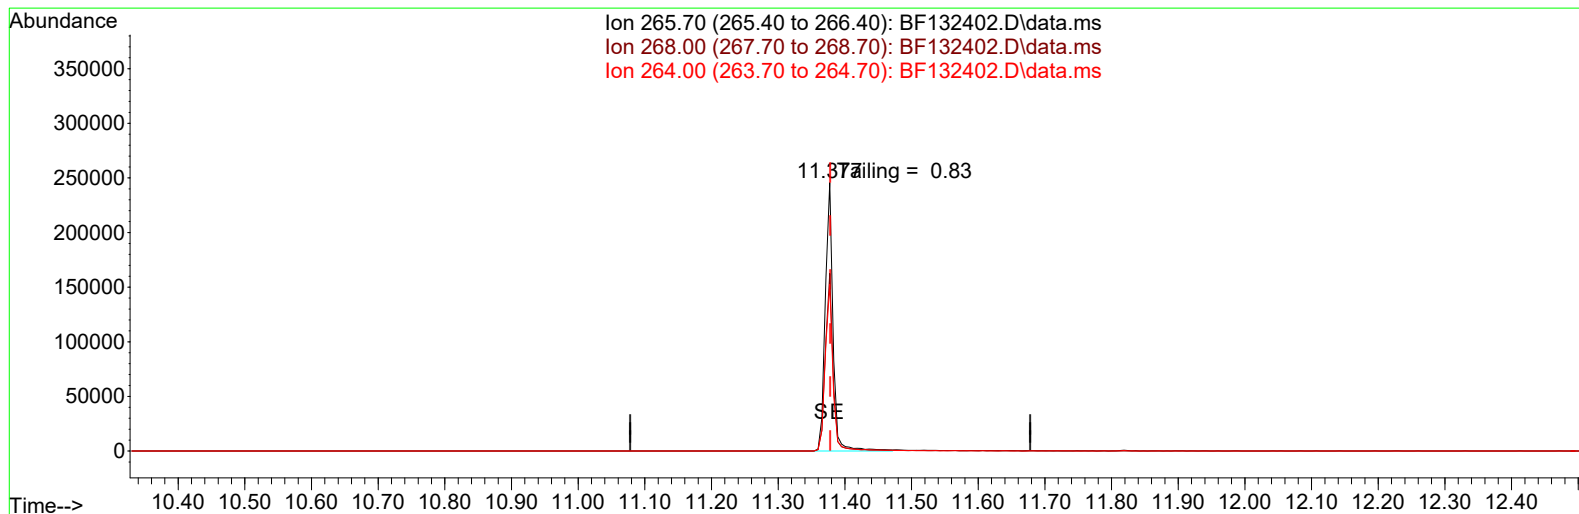

TIC: BF132402.D\data.ms

(70) Pentachlorophenol (C)




11.377min (-0.000) 30666.36 ng

response 200391

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	66.14
264.00	62.00	62.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021323\
Data File : BF132402.D
Acq On : 13 Feb 2023 10:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 04:14:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 14 00:51:00 2023
Response via : Initial Calibration

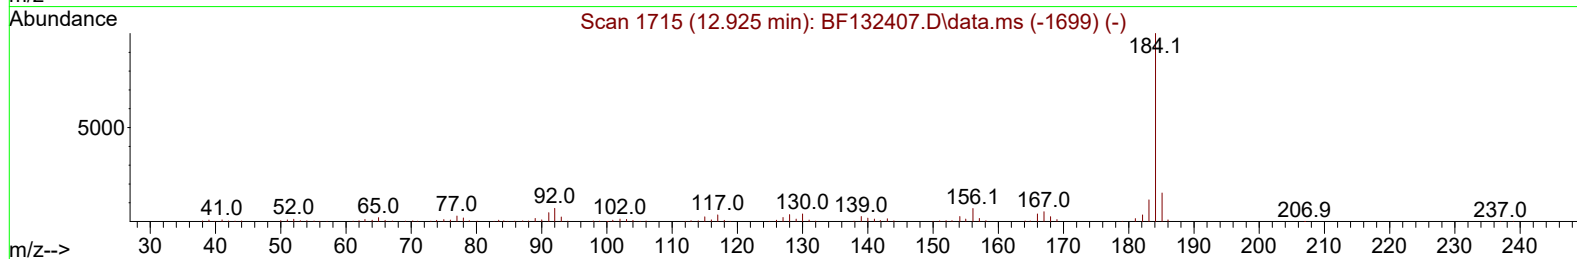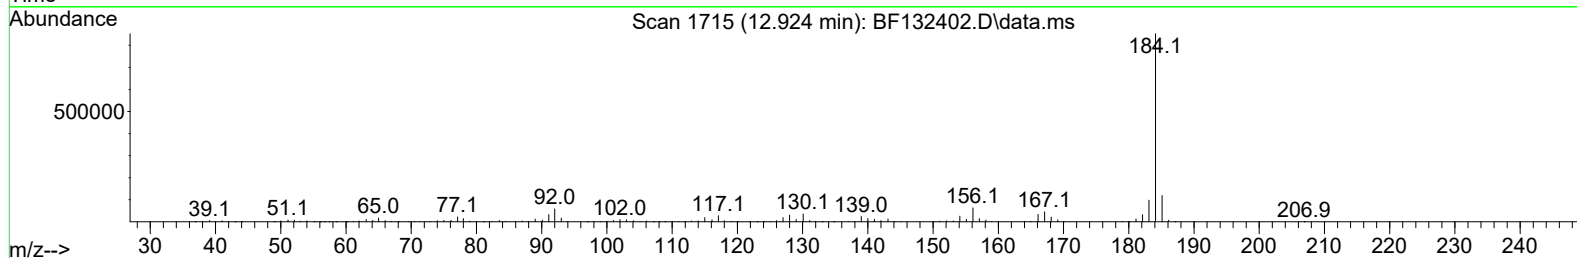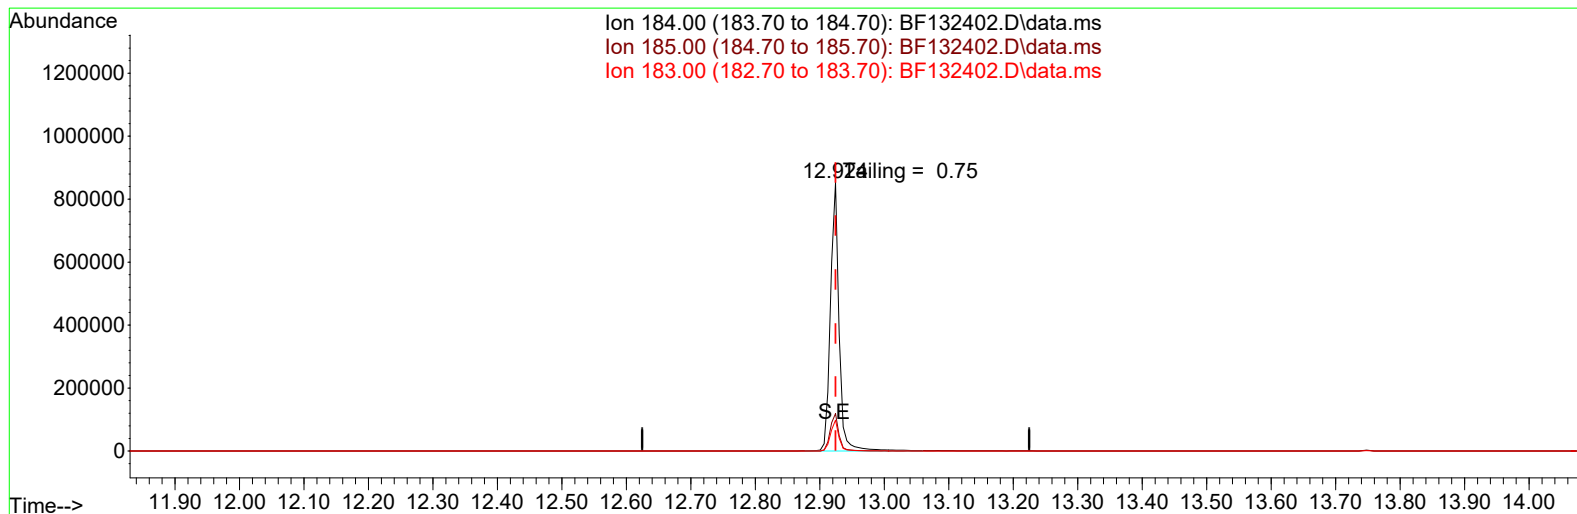

TIC: BF132402.D\data.ms

(77) Benzidine

12.924min (-0.000) 0.00 ng

response 798715

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	13.99
183.00	11.60	11.54
0.00	0.00	0.00