


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021323\
Data File : BF132402.D
Acq On : 13 Feb 2023 10:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021323.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 14 00:51:00 2023

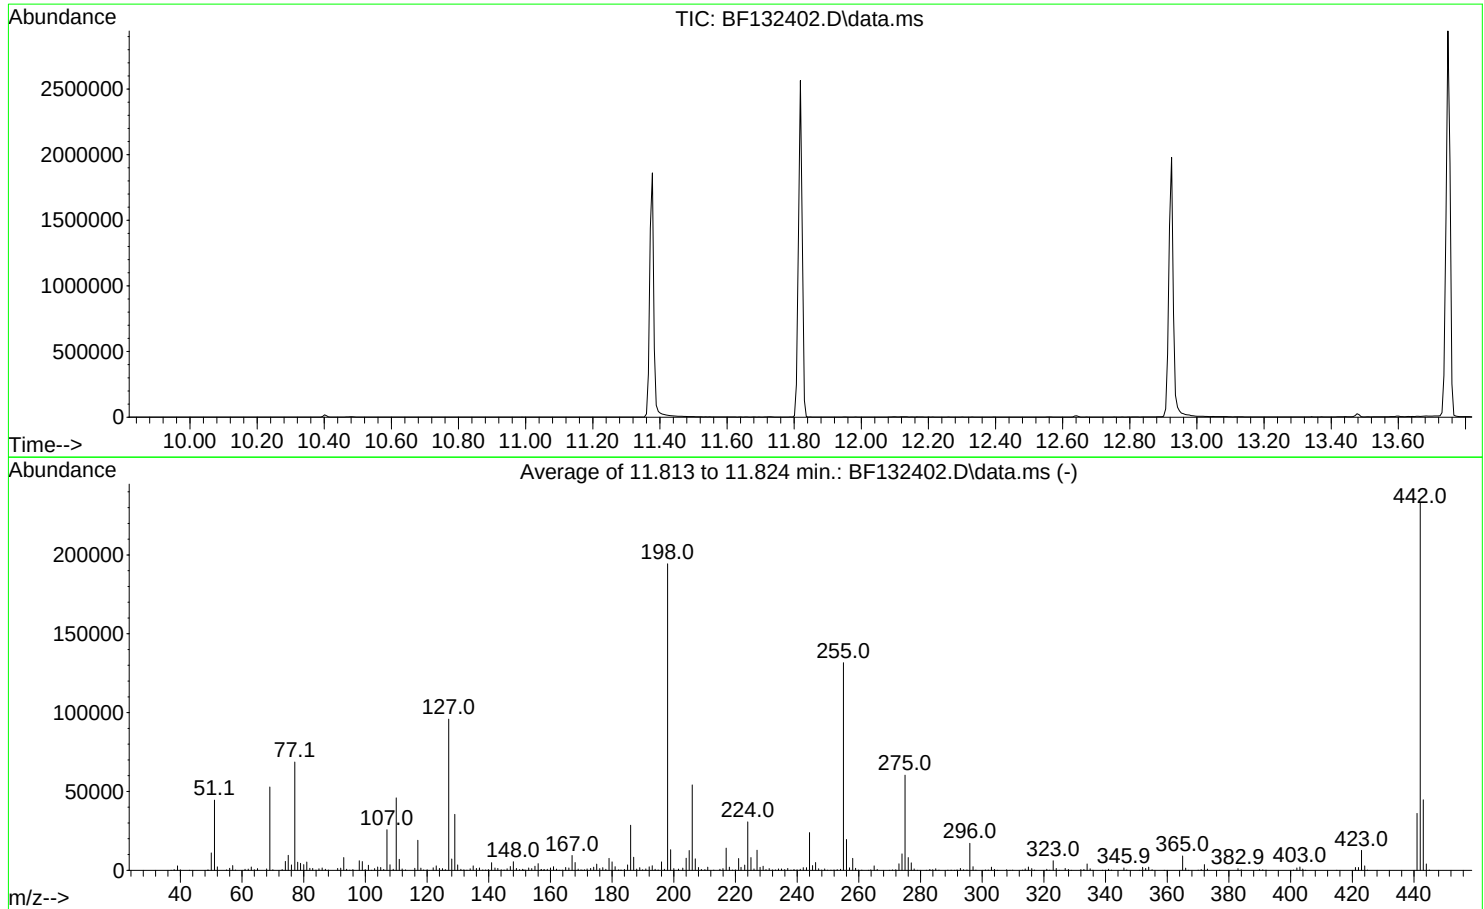




AutoFind: Scans 1526, 1527, 1528; Background Corrected with Scan 1521

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.9	44501	PASS
68	69	0.00	2	1.7	901	PASS
69	198	0.00	100	27.2	52861	PASS
70	69	0.00	2	0.6	341	PASS
127	198	10	80	49.3	95877	PASS
197	198	0.00	2	0.3	621	PASS
198	198	100	100	100.0	194368	PASS
199	198	5	9	6.7	13003	PASS
275	198	10	60	31.0	60299	PASS
365	198	1	100	4.7	9077	PASS
441	198	0.01	100	18.6	36106	PASS
442	442	50	100	100.0	233299	PASS
443	442	15	24	19.2	44741	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021323\
Data File : BF132402.D
Acq On : 13 Feb 2023 10:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 14 04:14:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 14 00:51:00 2023
Response via : Initial Calibration

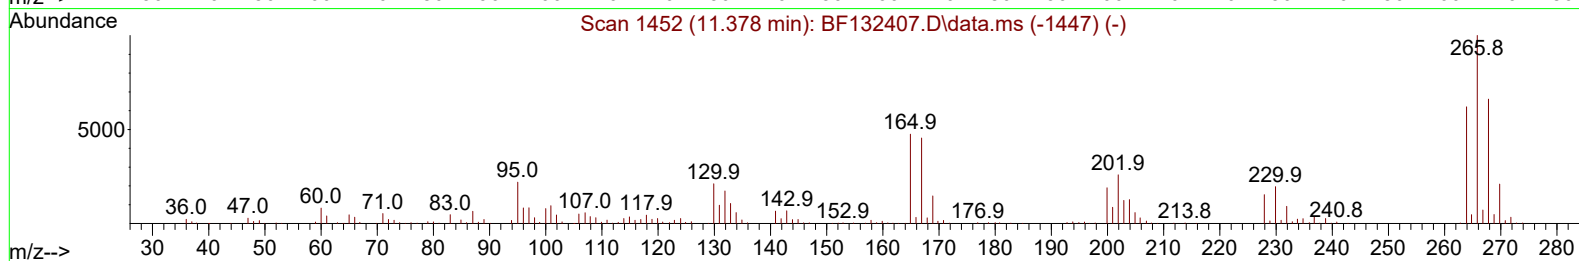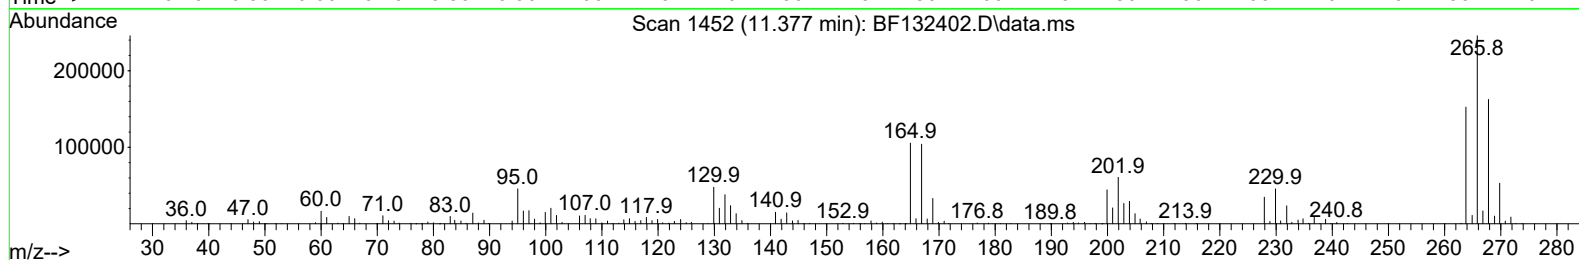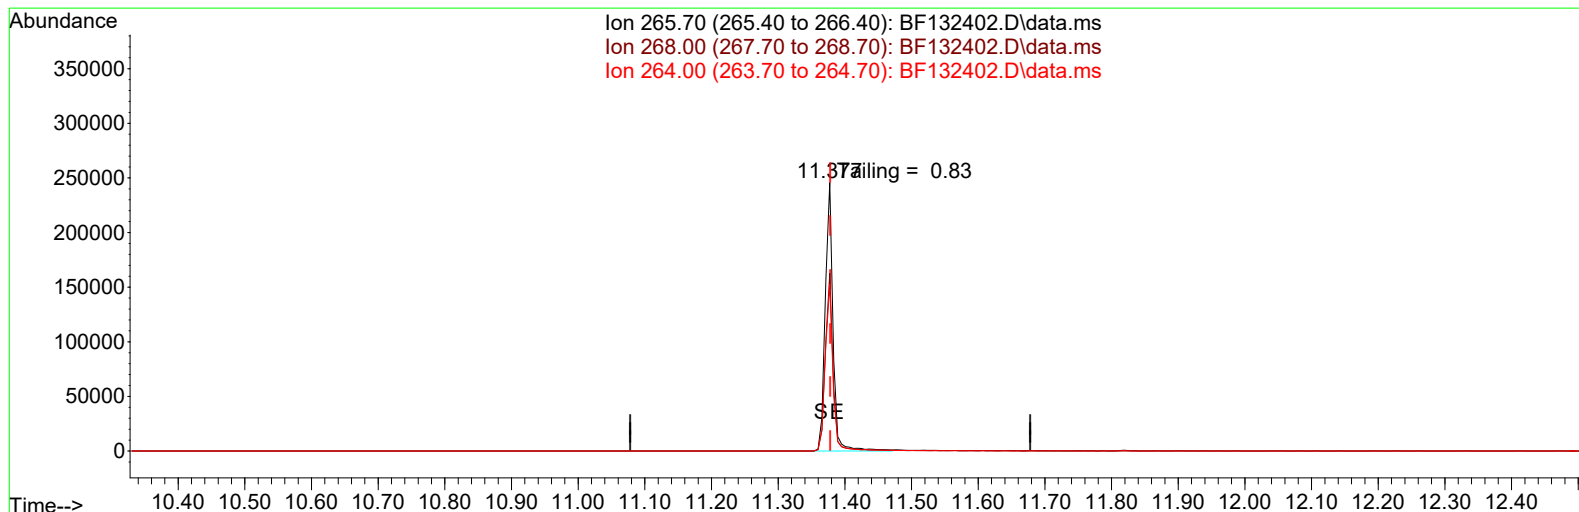

TIC: BF132402.D\data.ms

(70) Pentachlorophenol (C)

11.377min (-0.000) 30666.36 ng




response 200391

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	66.14
264.00	62.00	62.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021323\
Data File : BF132402.D
Acq On : 13 Feb 2023 10:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 14 04:14:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 14 00:51:00 2023
Response via : Initial Calibration

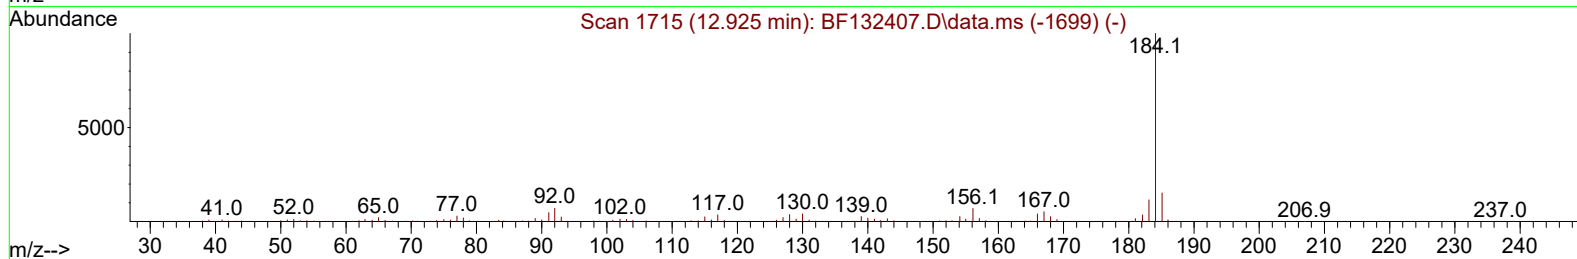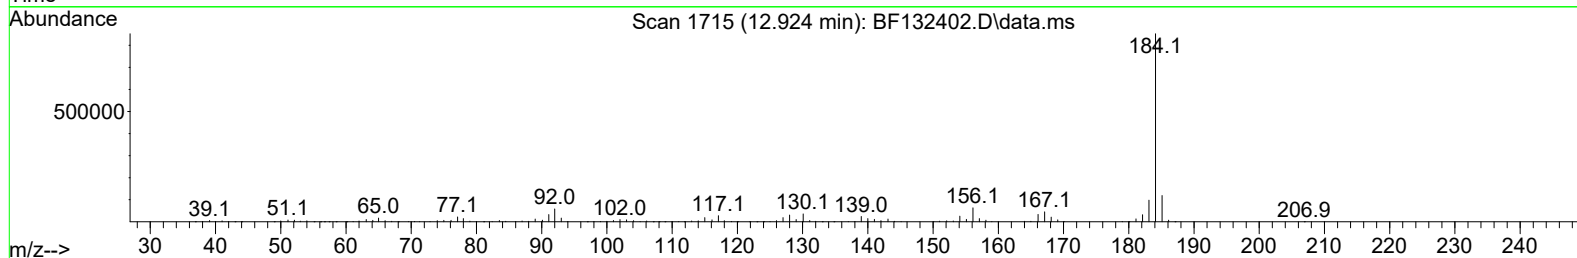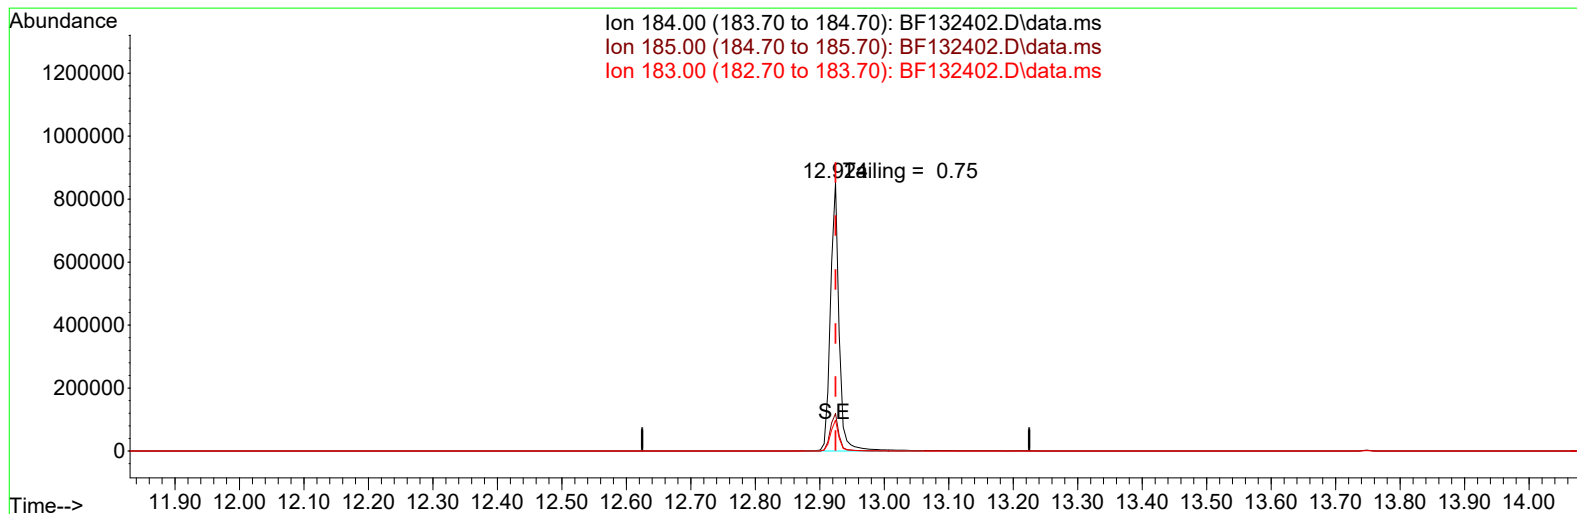

TIC: BF132402.D\data.ms

(77) Benzidine

12.924min (-0.000) 0.00 ng

response 798715

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	13.99
183.00	11.60	11.54
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/13/2023	BNA_F	<u>BF132402.D</u>
Compound Name	Response	Retention Time
DDT	493008	13.748
DDD	4527	13.477
DDE	0	13.113
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4527	497535	0.91

Instrument :
BNA_F
ClientSampleId :
DFTPP