
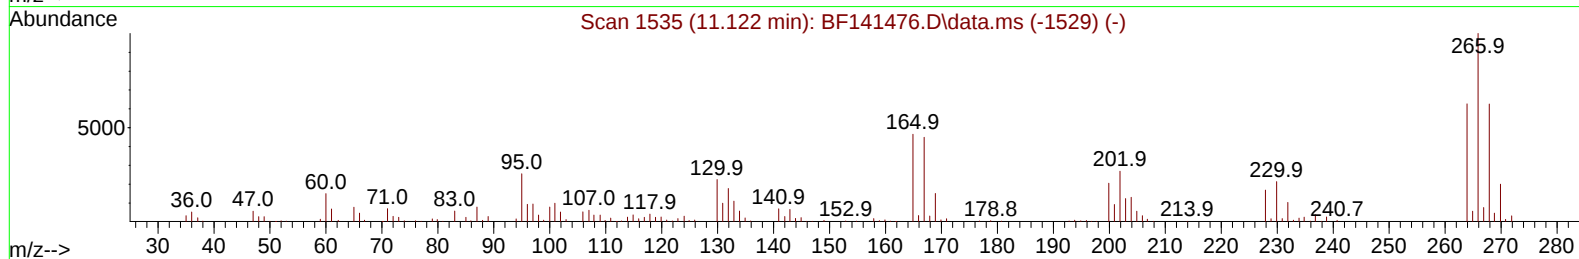
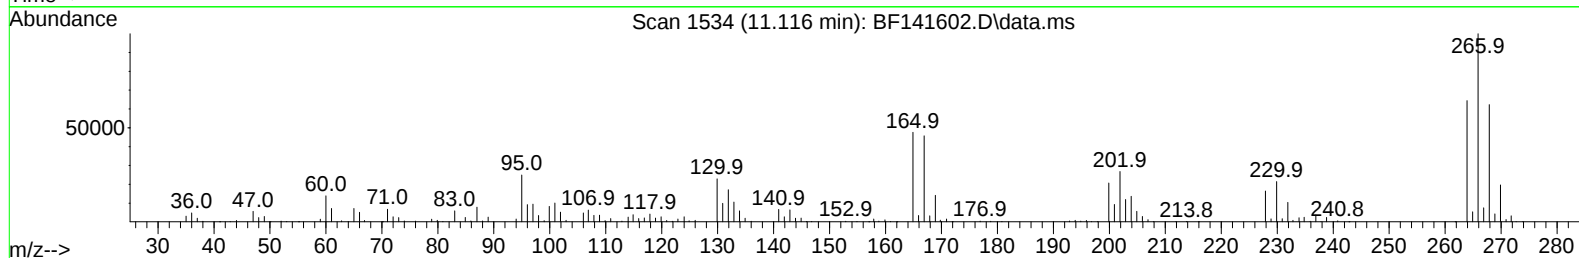


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021325\
Data File : BF141602.D
Acq On : 13 Feb 2025 09:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 10:48:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

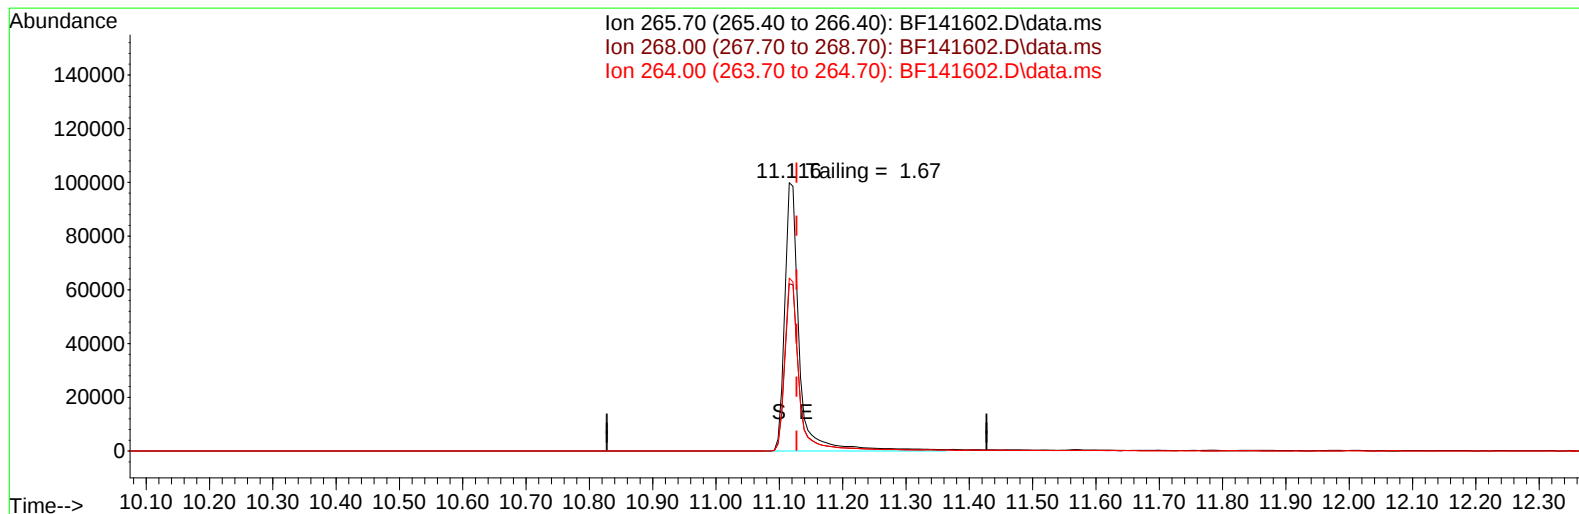

TIC: BF141602.D\data.ms

(70) Pentachlorophenol (C)




11.116min (-0.012) 14042.47 ng

response 160894

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.33
264.00	62.60	64.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021325\
Data File : BF141602.D
Acq On : 13 Feb 2025 09:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 10:48:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

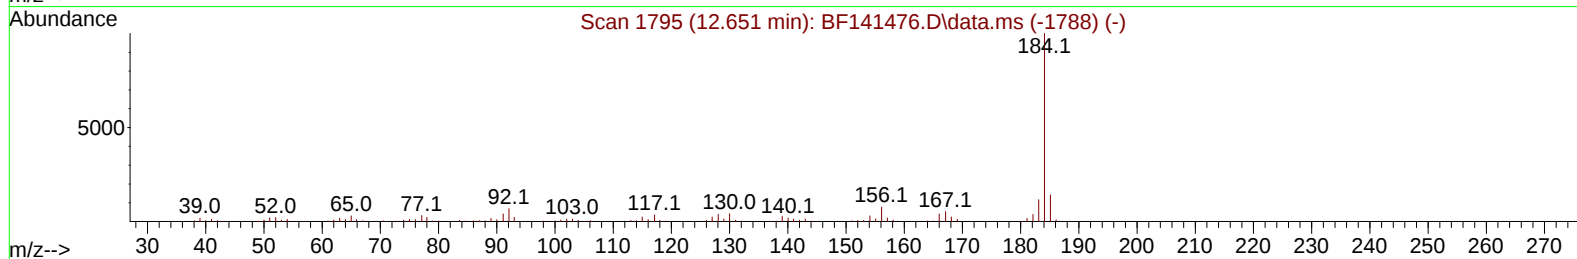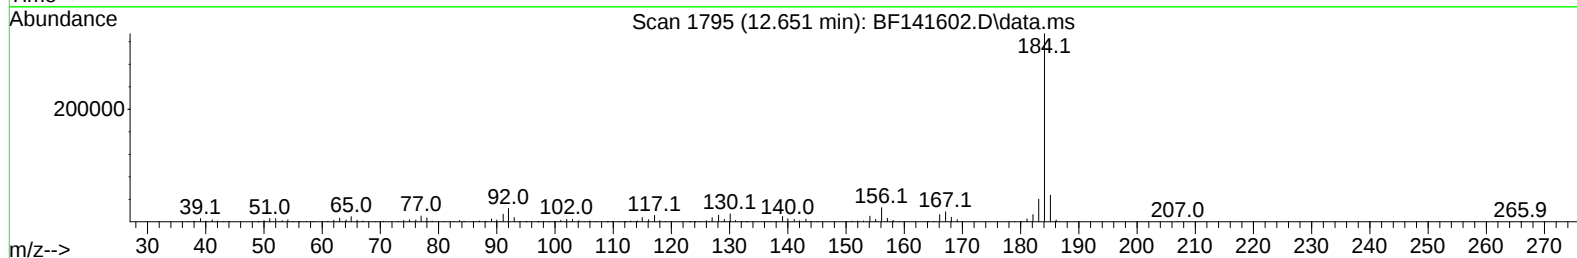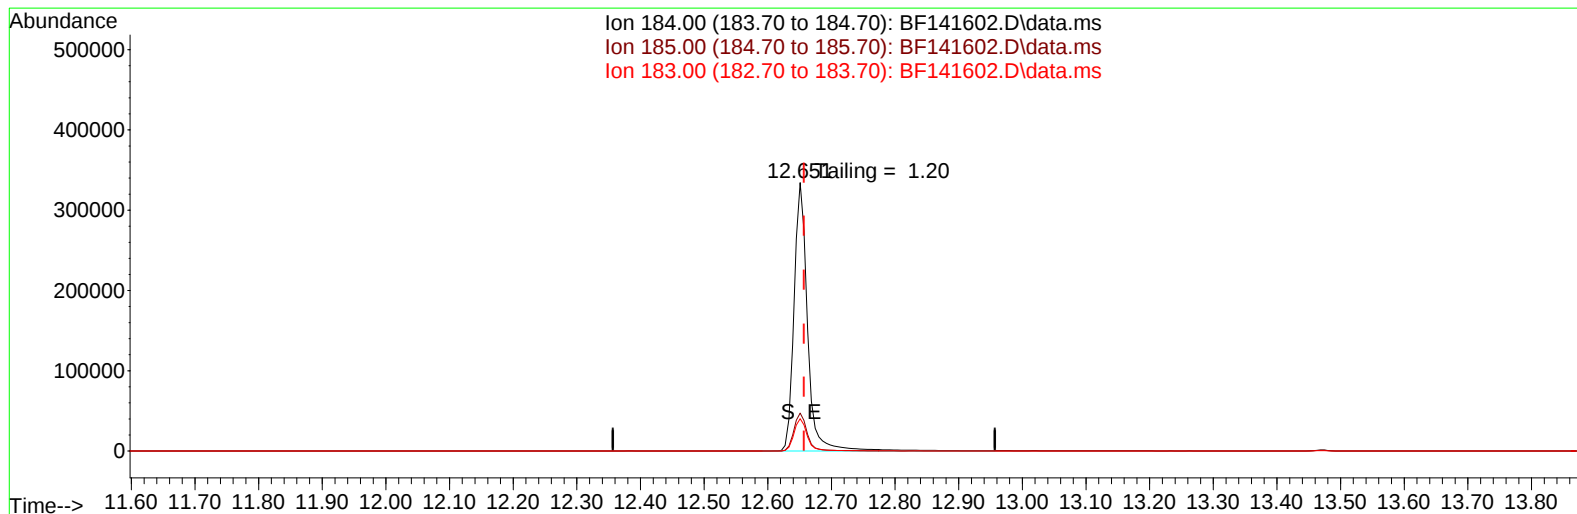

TIC: BF141602.D\data.ms

(77) Benzidine

12.651min (-0.006) 15729.00 ng

response 494669

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.14
183.00	11.60	12.06
0.00	0.00	0.00