

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021325\
 Data File : BF141624.D
 Acq On : 13 Feb 2025 19:27
 Operator : RC/JU
 Sample : Q1365-03 2X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 72-11995

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141624.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.804	282	291	297	rBV	4526	8549	1.06%	0.117%
2	5.404	558	563	588	rBV	428010	639159	79.49%	8.718%
3	6.422	731	736	758	rBV	425662	686153	85.34%	9.359%
4	6.787	792	798	806	rBV	426098	561851	69.88%	7.664%
5	7.345	885	893	905	rBV	321743	447476	55.65%	6.104%
6	7.616	934	939	952	rBV3	6494	16440	2.04%	0.224%
7	8.069	1010	1016	1035	rBV	536616	754108	93.79%	10.286%
8	9.016	1171	1177	1185	rBV5	4676	10412	1.29%	0.142%
9	9.139	1191	1198	1209	rBV	484078	646238	80.37%	8.815%
10	9.822	1308	1314	1323	rBV	599407	804032	100.00%	10.967%
11	10.239	1379	1385	1390	rBV2	6748	10301	1.28%	0.141%
12	10.533	1430	1435	1443	rBV	39089	55130	6.86%	0.752%
13	10.610	1443	1448	1459	rBV	238380	336412	41.84%	4.589%
14	10.845	1483	1488	1495	rBV4	5098	10813	1.34%	0.147%
15	11.304	1561	1566	1578	rBV	513261	693898	86.30%	9.465%
16	11.851	1654	1659	1666	rBV7	9249	28245	3.51%	0.385%
17	11.945	1672	1675	1680	rVB6	8597	11713	1.46%	0.160%
18	12.045	1689	1692	1695	rBV3	14859	18214	2.27%	0.248%
19	12.086	1695	1699	1704	rVB	21773	26947	3.35%	0.368%
20	12.251	1723	1727	1730	rBV2	9439	11857	1.47%	0.162%
21	12.522	1769	1773	1776	rBV	13822	16871	2.10%	0.230%
22	12.557	1776	1779	1783	rVB	9593	11348	1.41%	0.155%
23	12.745	1808	1811	1817	rBV	14037	21541	2.68%	0.294%
24	12.886	1830	1835	1843	rBV	292298	391535	48.70%	5.341%
25	13.945	2008	2015	2027	rBV	404060	610634	75.95%	8.329%
26	15.392	2256	2261	2280	rVB	288046	501412	62.36%	6.839%




Sum of corrected areas: 7331289

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021325\
Data File : BF141624.D
Acq On : 13 Feb 2025 19:27
Operator : RC/JU
Sample : Q1365-03 2X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
72-11995

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

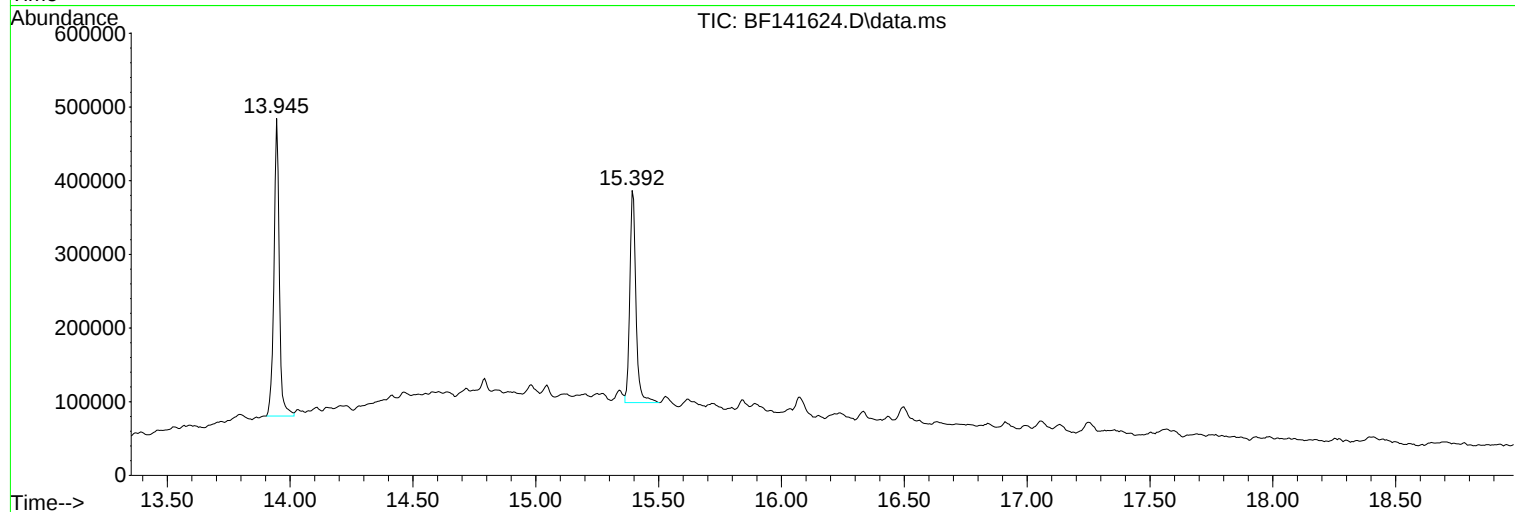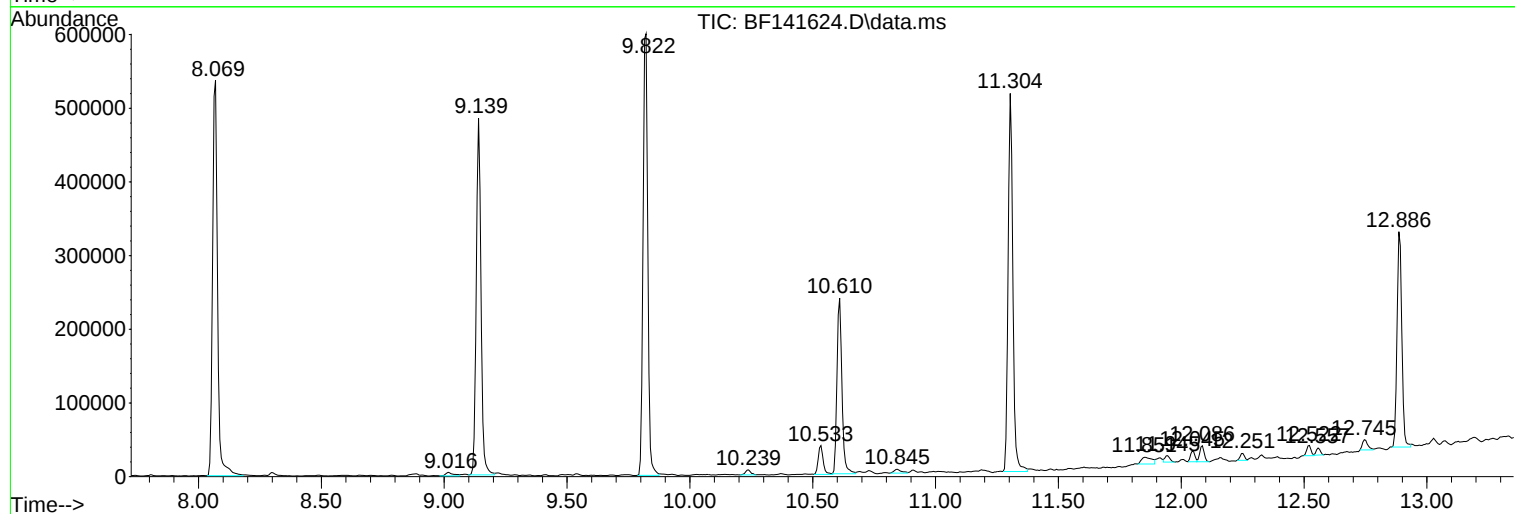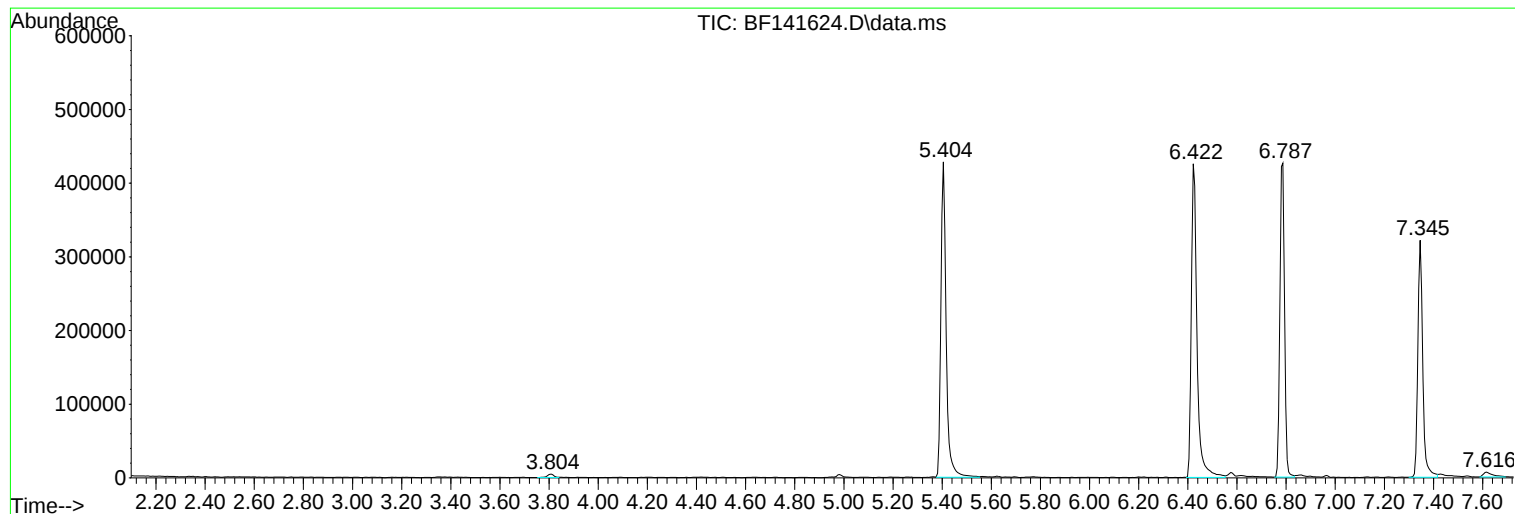

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021325\
Data File : BF141624.D
Acq On : 13 Feb 2025 19:27
Operator : RC/JU
Sample : Q1365-03 2X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
72-11995

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021325\
Data File : BF141624.D
Acq On : 13 Feb 2025 19:27
Operator : RC/JU
Sample : Q1365-03 2X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
72-11995

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------