
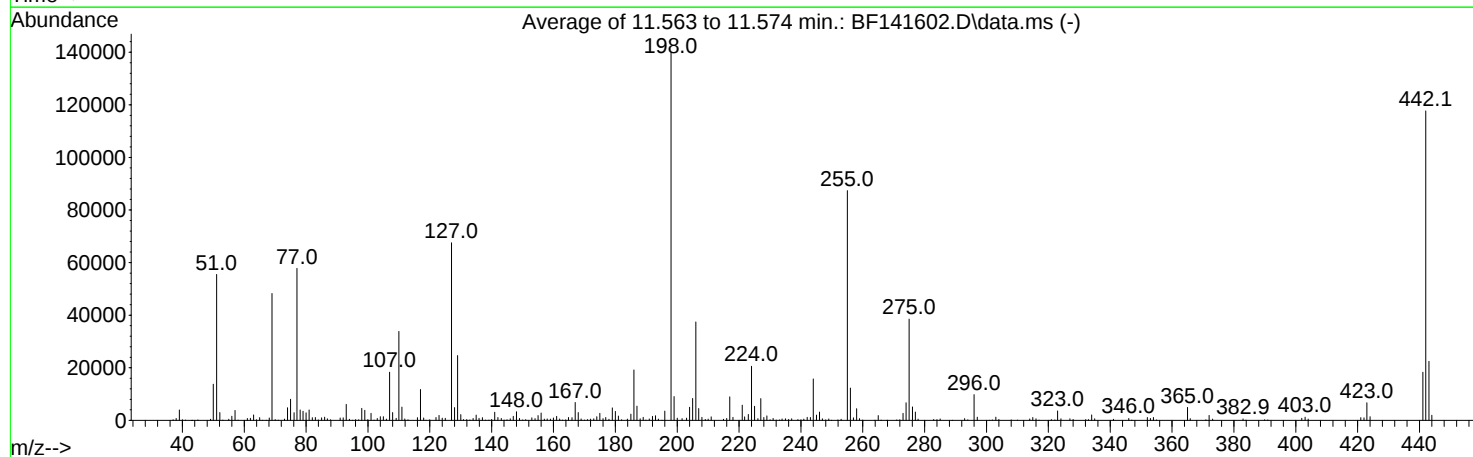


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021325\
Data File : BF141602.D
Acq On : 13 Feb 2025 09:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 06 16:58:59 2025

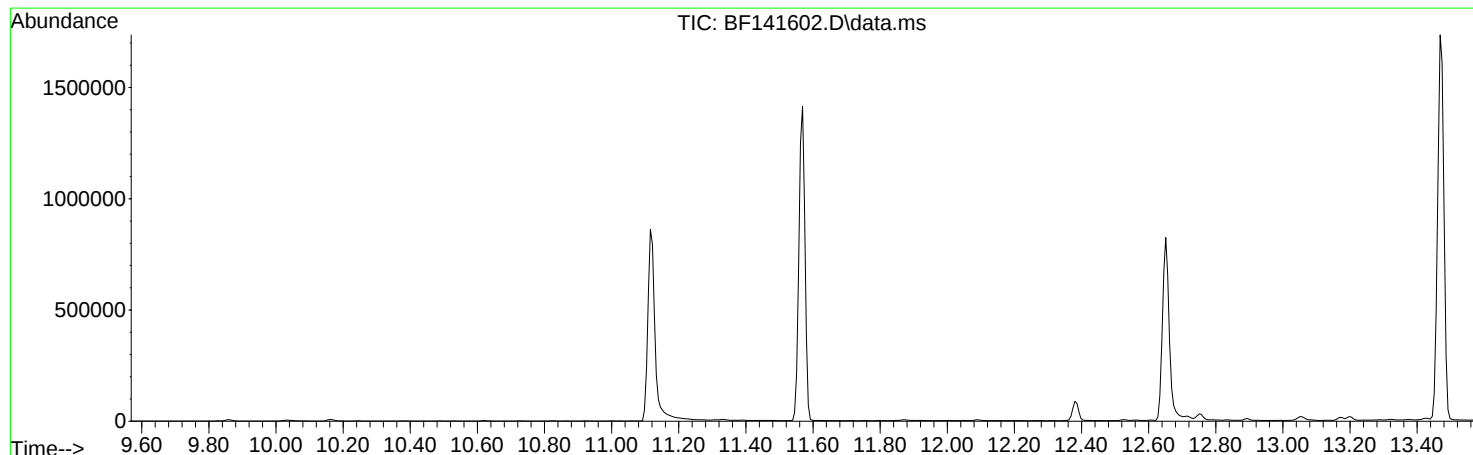

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	55464	PASS
68	69	0.00	2	1.9	906	PASS
69	198	0.00	100	34.5	48224	PASS
70	69	0.00	2	0.6	300	PASS
127	198	10	80	48.3	67533	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	139891	PASS
199	198	5	9	6.5	9041	PASS
275	198	10	60	27.5	38525	PASS
365	198	1	100	3.5	4928	PASS
441	198	0.01	100	13.1	18338	PASS
442	442	50	100	100.0	117696	PASS
443	442	15	24	19.1	22443	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/13/2025	BNA_F	<u>BF141602.D</u>
Compound Name	Response	Retention Time
DDT	449110	13.468
DDD	9352	13.198
DDE	582	12.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9934	459044	2.16

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021325\
Data File : BF141602.D
Acq On : 13 Feb 2025 09:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 13 10:48:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

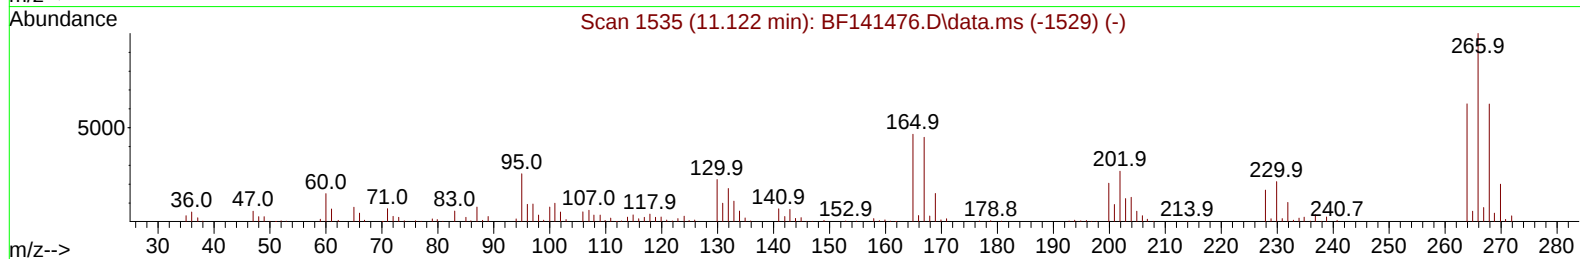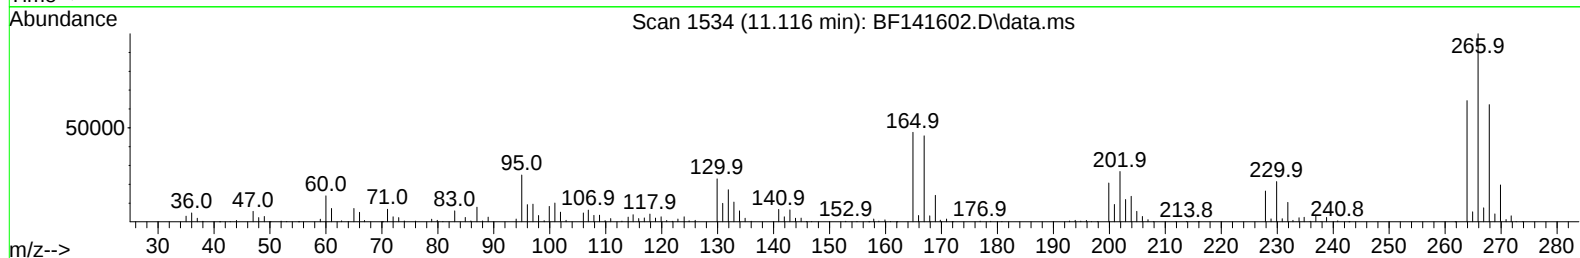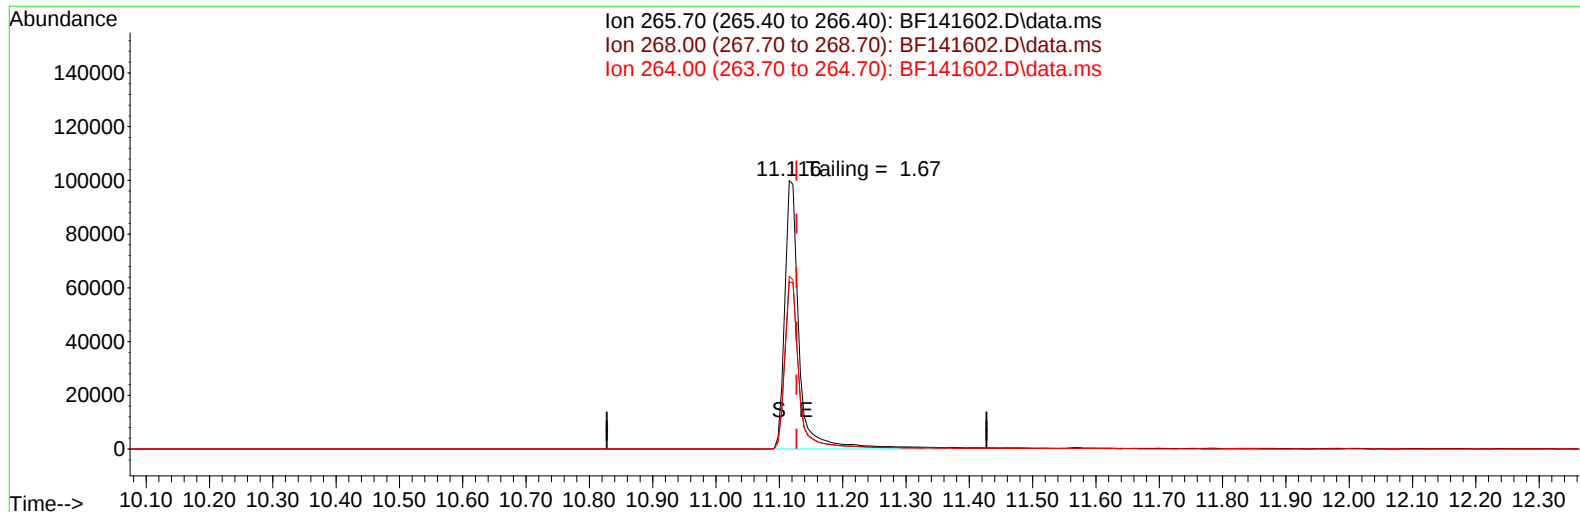

TIC: BF141602.D\data.ms

(70) Pentachlorophenol (C)

11.116min (-0.012) 14042.47 ng




response 160894

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.33
264.00	62.60	64.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021325\
Data File : BF141602.D
Acq On : 13 Feb 2025 09:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 13 10:48:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

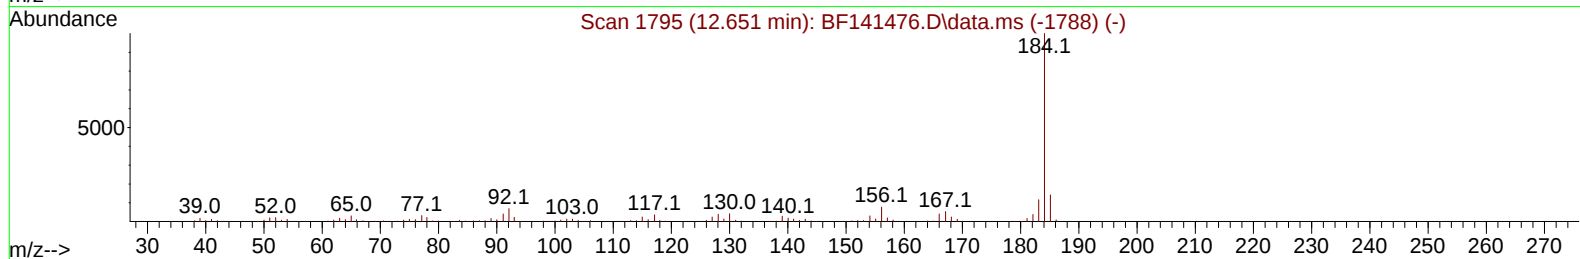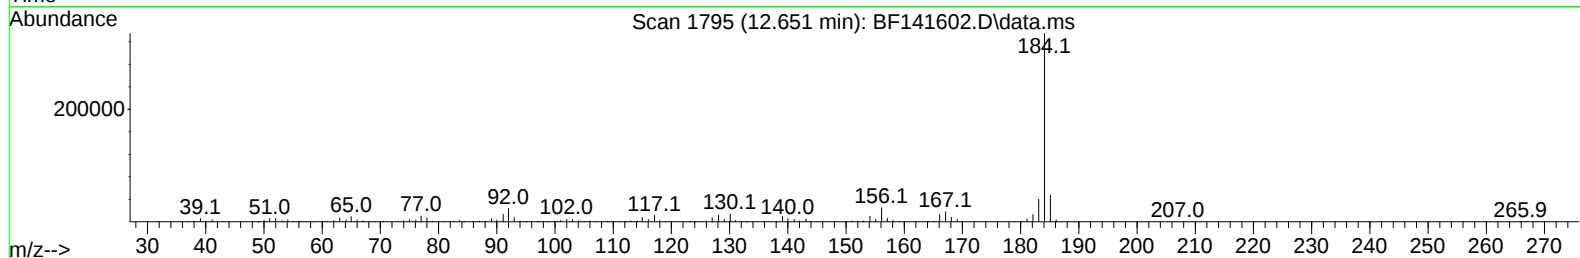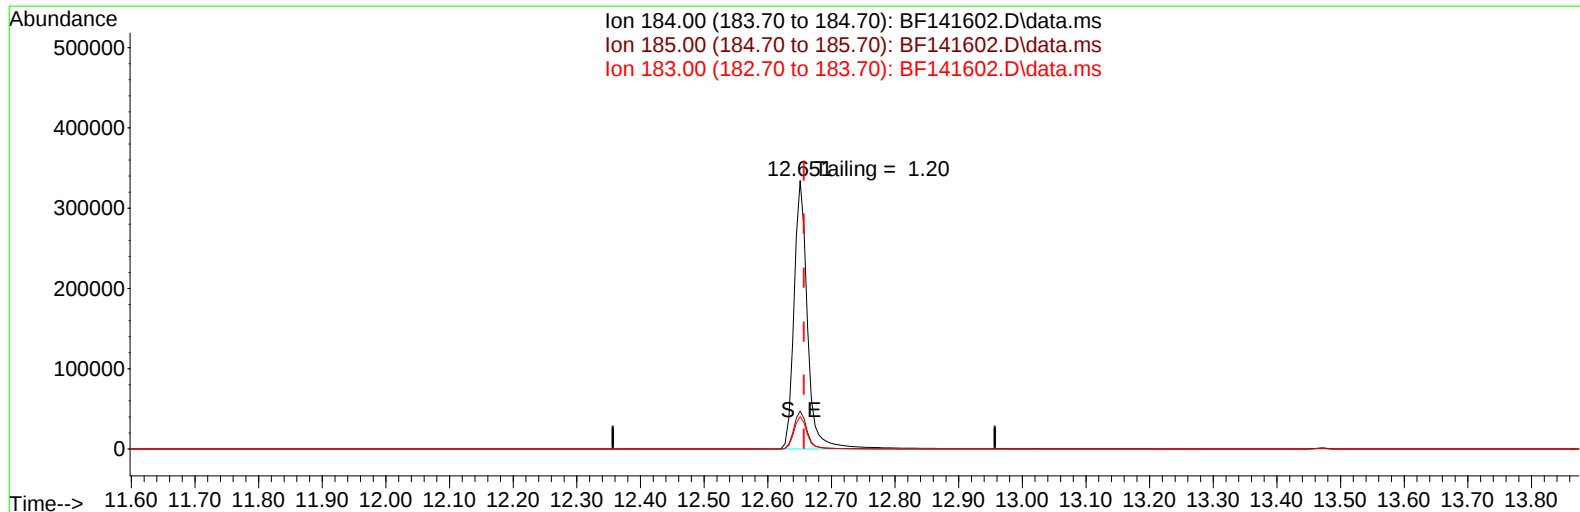

TIC: BF141602.D\data.ms

(77) Benzidine

12.651min (-0.006) 15729.00 ng

response 494669

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.14
183.00	11.60	12.06
0.00	0.00	0.00