
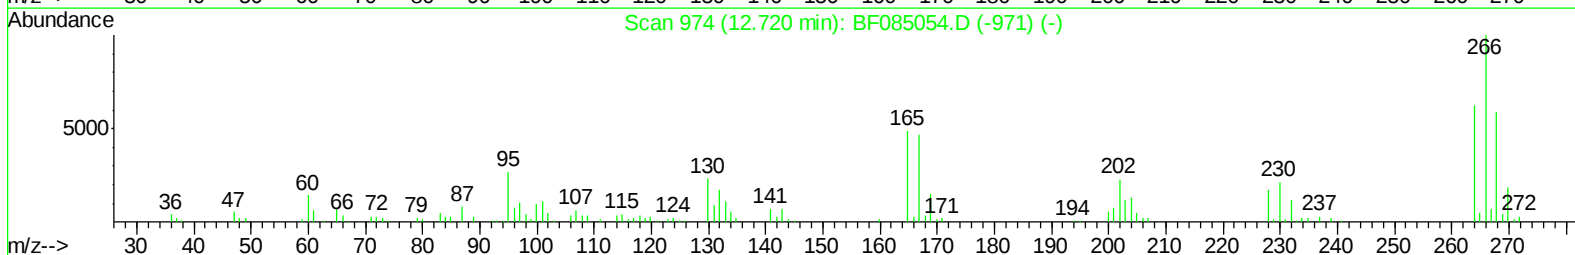
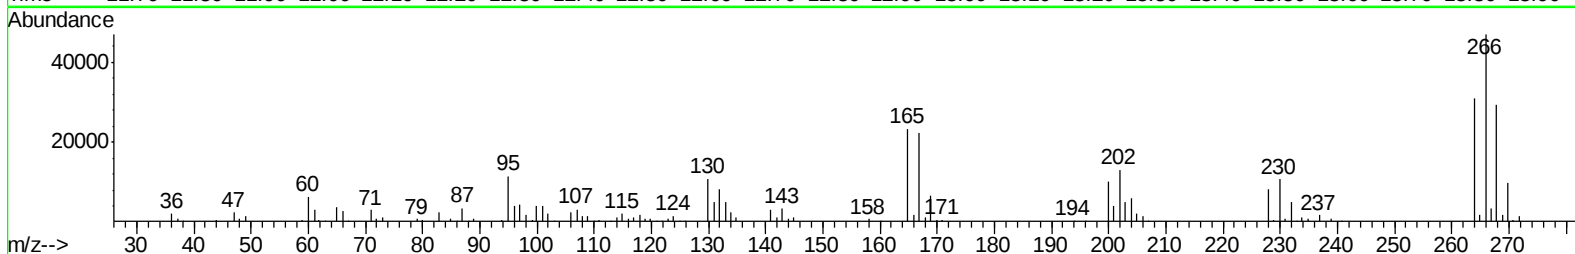


Data Path : Z:\HPCHEM1\BNA_F\Data\BF021416\
Data File : BF085059.D
Acq On : 13 Feb 2016 00:16
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 15 08:14:27 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 13 00:11:18 2016
Response via : Initial Calibration

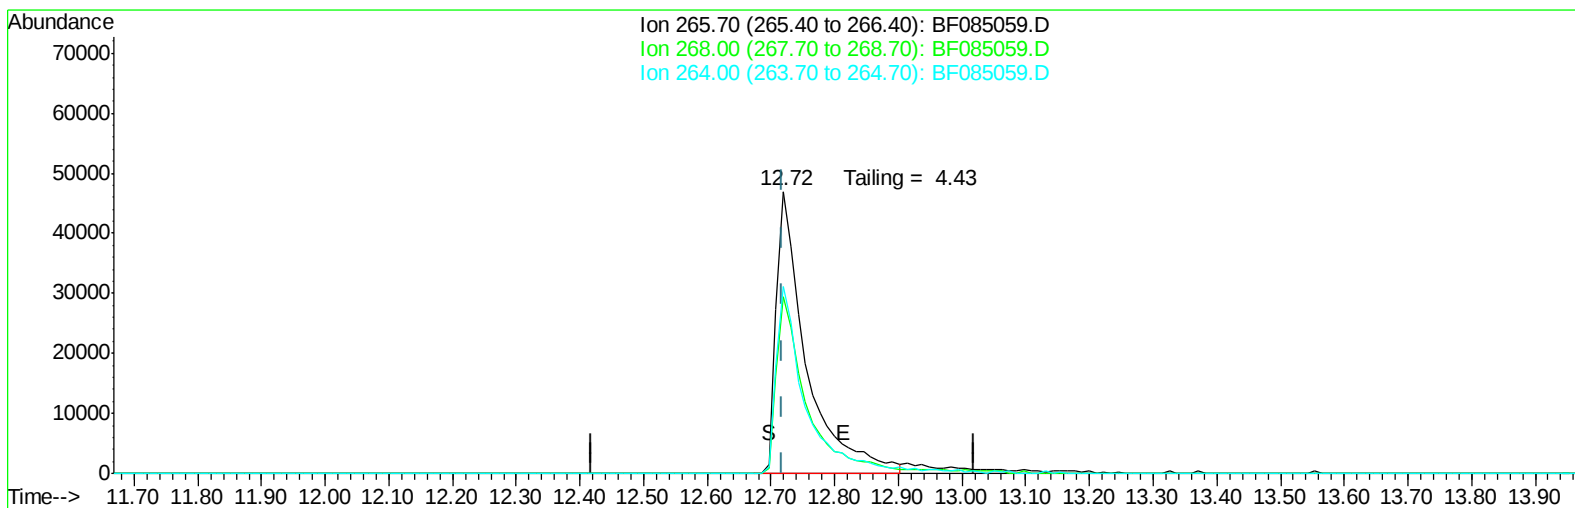

TIC: BF085059.D

(69) Pentachlorophenol (C)




12.719min (+0.000) 65021.65ng

response 156781

Ion	Exp%	Act%
265.70	100	100
268.00	59.10	62.59
264.00	62.20	66.30
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF021416\
Data File : BF085059.D
Acq On : 13 Feb 2016 00:16
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 15 08:14:27 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 13 00:11:18 2016
Response via : Initial Calibration

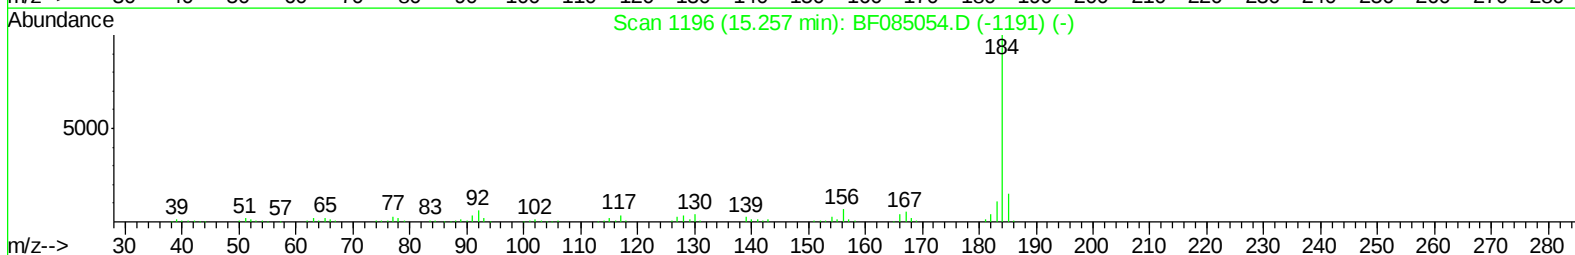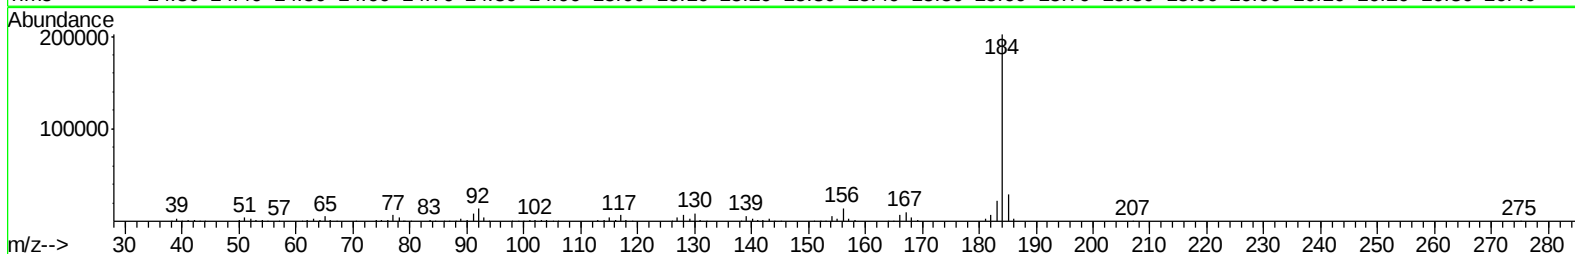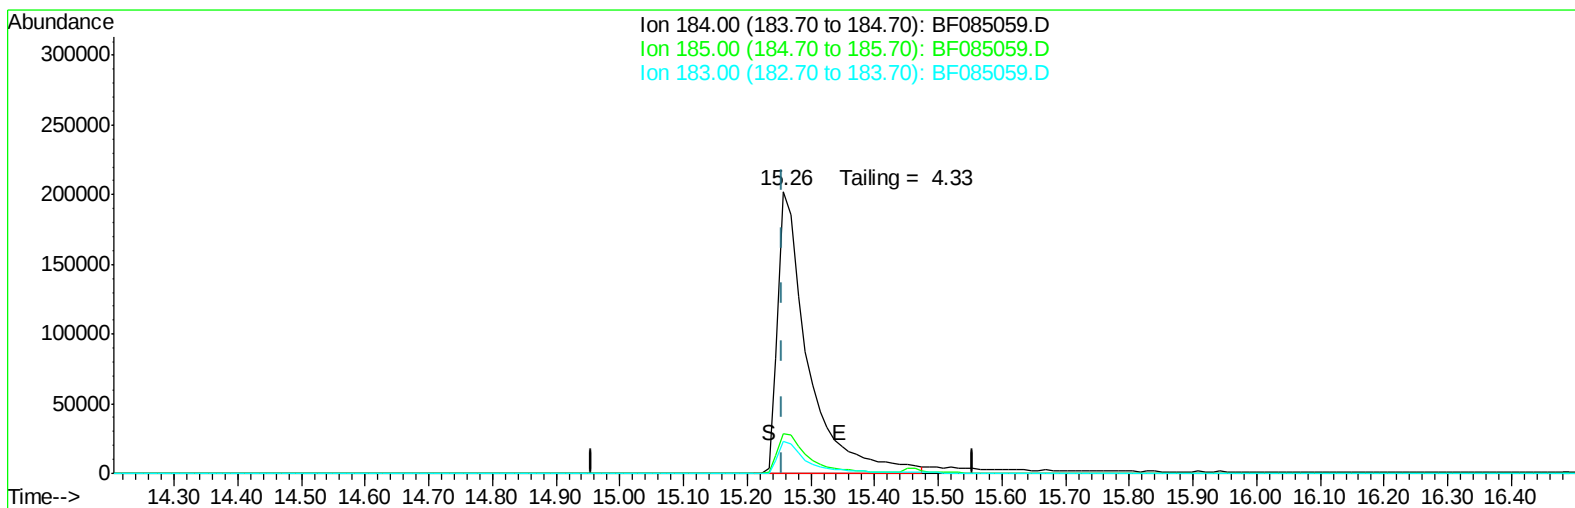

TIC: BF085059.D

(76) Benzidine

15.257min (+0.001) -20.00ng

response 673671

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.29
183.00	10.70	11.33
0.00	0.00	0.00