

Data Path : Z:\HPCHEM1\BNA F\DATA\BF021416\
 Data File : BF085061.D
 Acq On : 13 Feb 2016 1:27
 Operator : SJ/IZ
 Sample : H1396-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 S4-B002(2-4)

Quant Time: Feb 13 04:11:55 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 13 00:11:18 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	5.90	152	142750	20.00	ng	0.01
21) Naphthalene-d8	7.79	136	648029	20.00	ng	0.00
38) Acenaphthene-d10	10.58	164	314429	20.00	ng	0.00
63) Phenanthrene-d10	12.99	188	592870	20.00	ng	0.00
75) Chrysene-d12	17.17	240	441671	20.00	ng	-0.01
86) Perylene-d12	18.79	264	286434	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	4.15	112	1053959	129.10	ng	-0.01
7) Phenol-d6	5.43	99	1548953	142.36	ng	-0.01
23) Nitrobenzene-d5	6.71	82	1015151	92.51	ng	-0.01
41) 2,4,6-Tribromophenol	11.88	330	402569	123.96	ng	0.00
44) 2-Fluorobiphenyl	9.53	172	1812670	82.41	ng	0.00
78) Terphenyl-d14	15.62	244	1518708	70.77	ng	0.00
Target Compounds						Qvalue
49) Dimethylphthalate	10.22	163	264527	11.22	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF021416\
Data File : BF085061.D
Acq On : 13 Feb 2016 1:27
Operator : SJ/IZ
Sample : H1396-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S4-B002(2-4)

Quant Time: Feb 13 04:11:55 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 13 00:11:18 2016
Response via : Initial Calibration

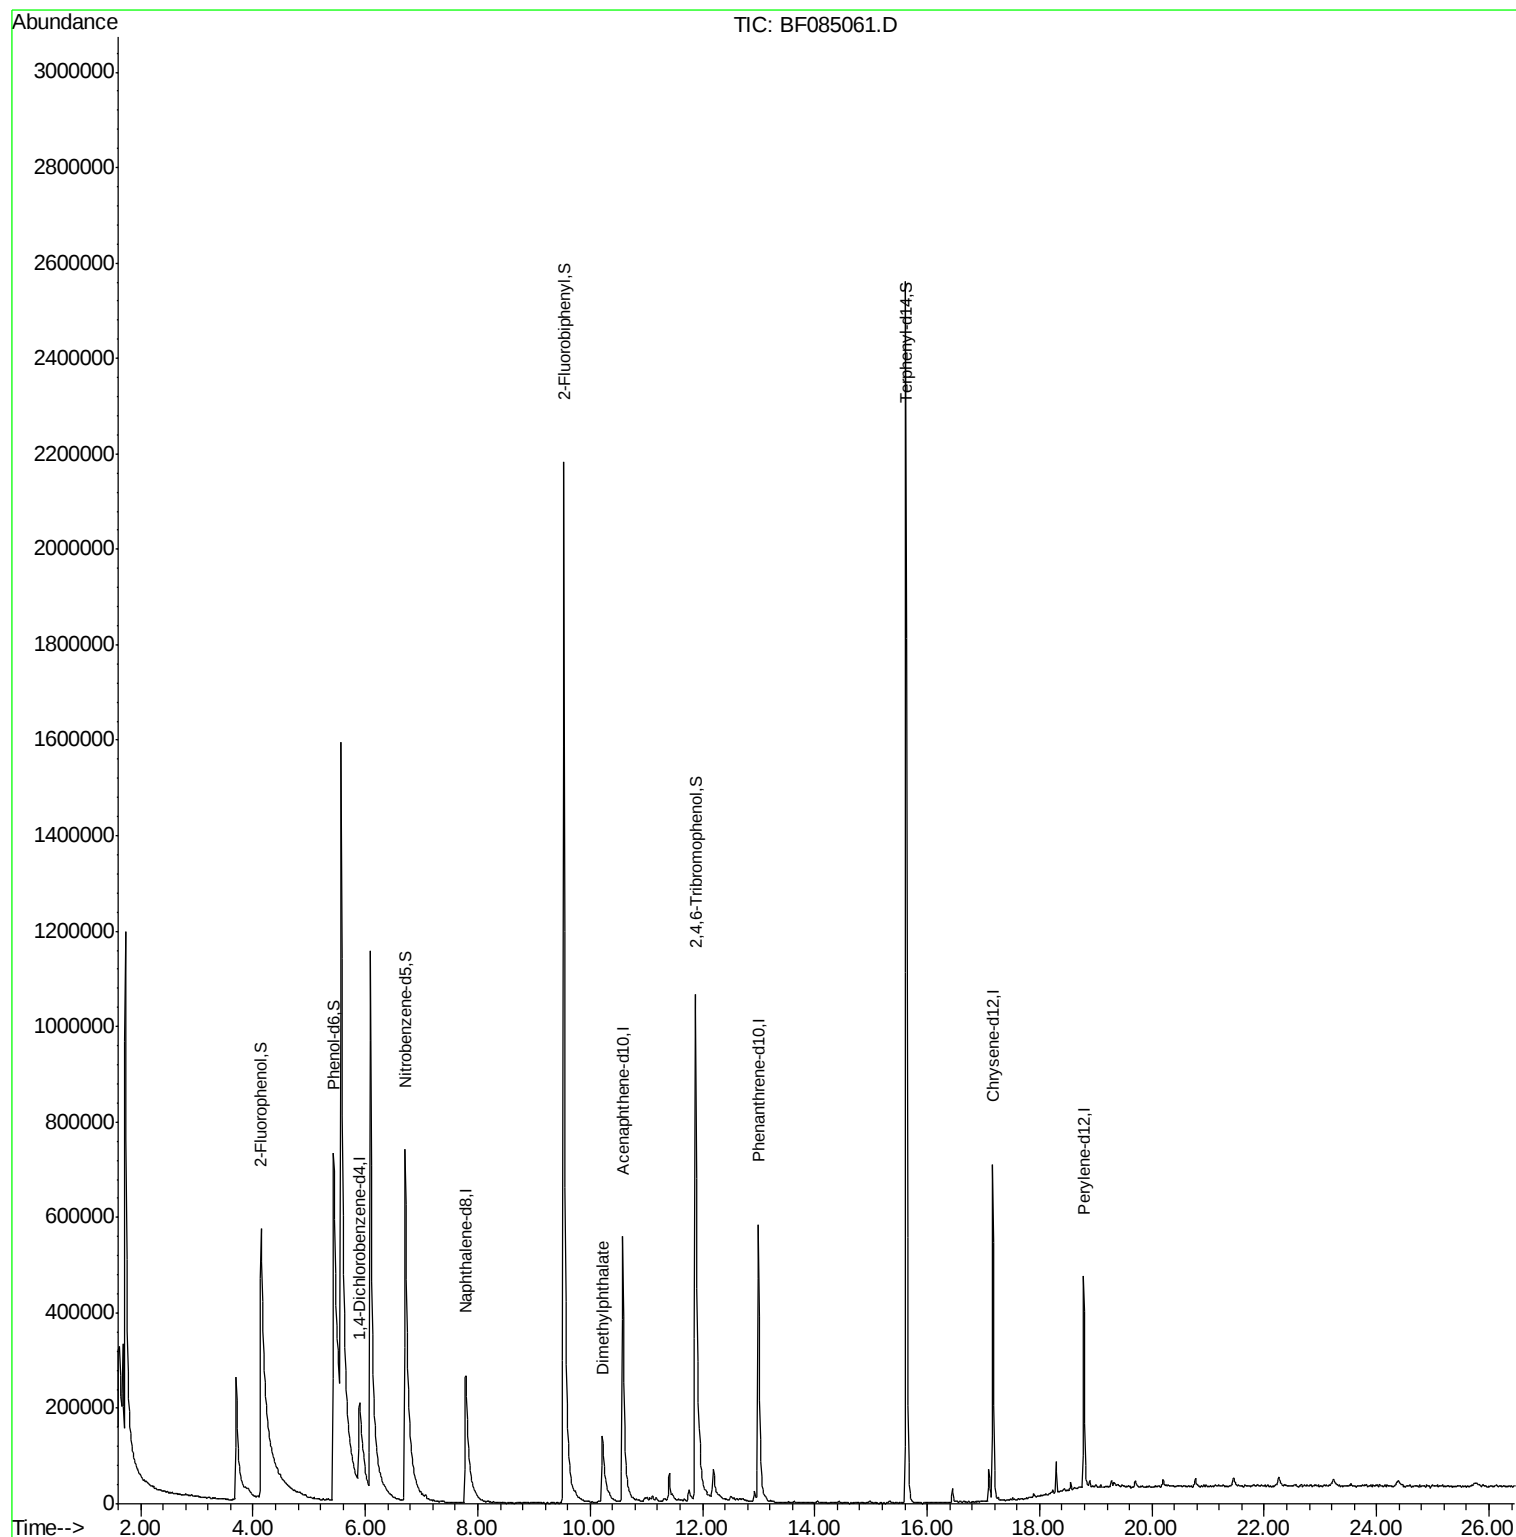




#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 5.90 min Scan# 377
 Delta R.T. 0.01 min
 Lab File: BF085061.D
 Acq: 13 Feb 2016 1:27

Instrument :
 BNA_F
 ClientSampleId :
 S4-B002(2-4)

Tot Ion	152	Resp	142750
Ion	Ratio	Lower	Upper
152	100		
150	163.0	127.4	191.2
115	70.7	50.5	75.7




Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

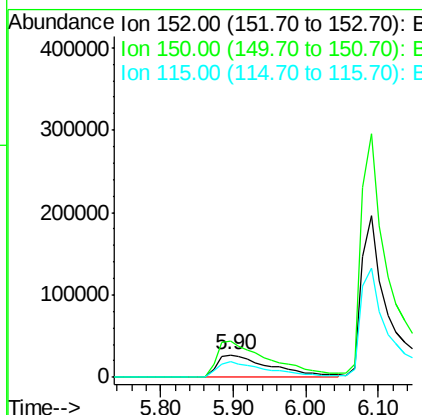



#5


2-Fluorophenol
 Concen: 129.10 ng
 RT: 4.15 min Scan# 224
 Delta R.T. -0.01 min
 Lab File: BF085061.D
 Acq: 13 Feb 2016 1:27

Tgt Ion	112	Resp	1053959
Ion	Ratio	Lower	Upper
112	100		
64	59.0	45.4	68.2
63	30.2	23.2	34.8



Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

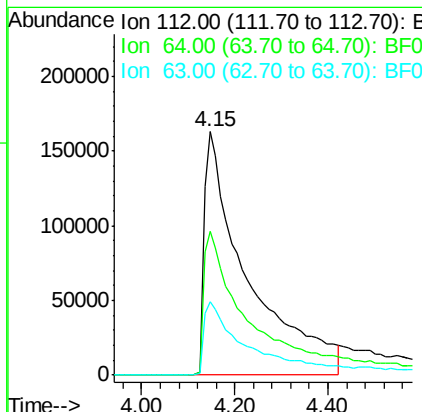

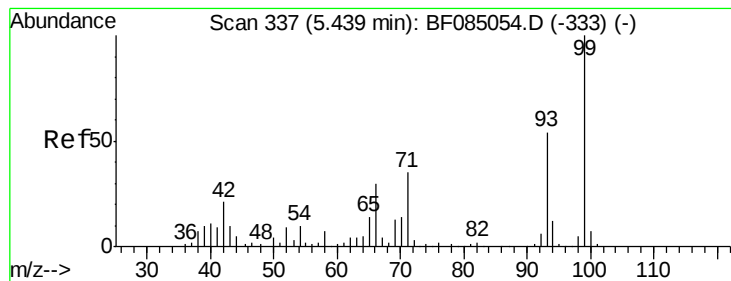

#7

Phenol-d6

Concen: 142.36 ng

RT: 5.43 min Scan# 336

Delta R.T. -0.01 min

Lab File: BF085061.D

Acq: 13 Feb 2016 1:27

Instrument :

BNA_F

ClientSampleId :

S4-B002(2-4)


Tot Ion: 99 Resp: 1548953

Ion Ratio Lower Upper

99 100

42 20.9 17.0 25.4




71 34.9 28.3 42.5



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

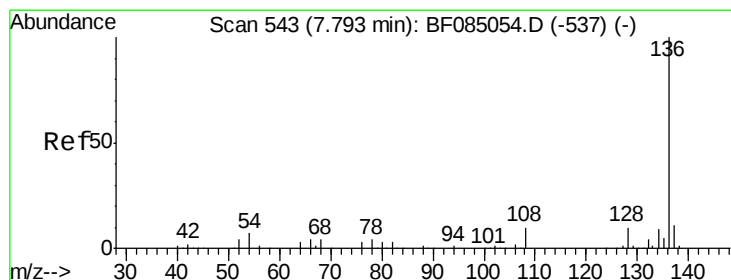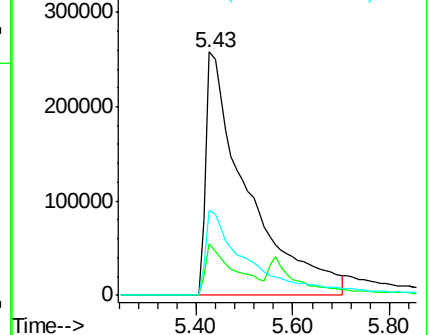

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.79 min Scan# 543

Delta R.T. -0.00 min

Lab File: BF085061.D

Acq: 13 Feb 2016 1:27

Tgt Ion: 136 Resp: 648029


Ion Ratio Lower Upper

136 100

137 10.7 8.9 13.3

54 8.6 6.1 9.1

68 4.8 3.5 5.3






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

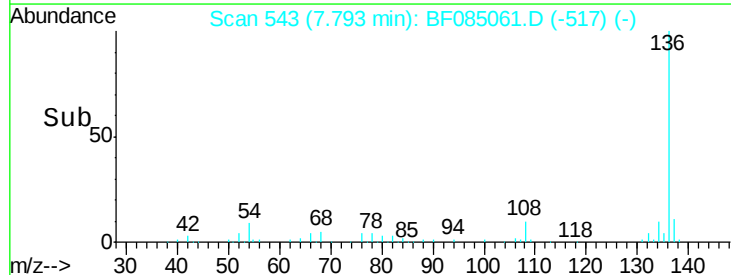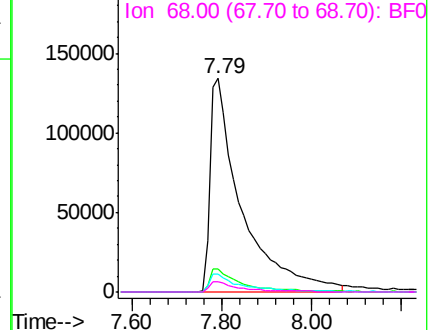



#23

Nitrobenzene-d5

Concen: 92.51 ng

RT: 6.71 min Scan# 448

Delta R.T. -0.01 min

Lab File: BF085061.D

Acq: 13 Feb 2016 1:27

Instrument :

BNA_F

ClientSampleId :

S4-B002(2-4)


Tot Ion: 82 Resp: 1015151

Ion Ratio Lower Upper




82 100

128 43.5 36.8 55.2

54 56.9 44.4 66.6



Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): B
Ion 54.00 (53.70 to 54.70): BF0

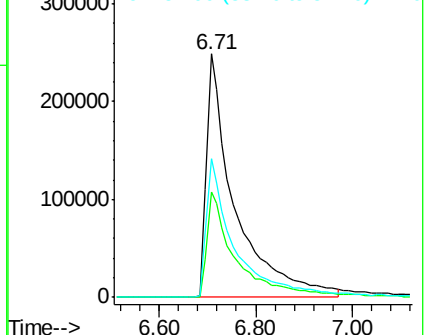

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 10.58 min Scan# 787

Delta R.T. -0.00 min

Lab File: BF085061.D

Acq: 13 Feb 2016 1:27


Tgt Ion:164 Resp: 314429

Ion Ratio Lower Upper



164 100


162 105.2 81.1 121.7

160 46.7 37.4 56.0



Abundance Ion 164.00 (163.70 to 164.70): B
Ion 162.00 (161.70 to 162.70): B
Ion 160.00 (159.70 to 160.70): B

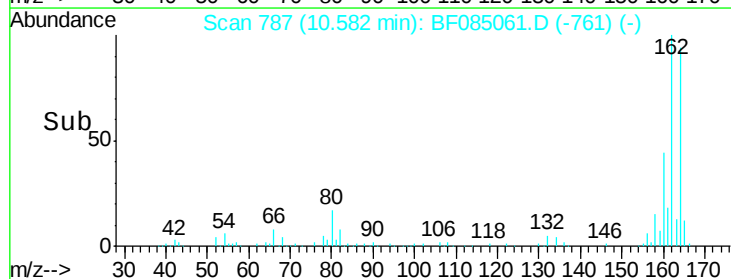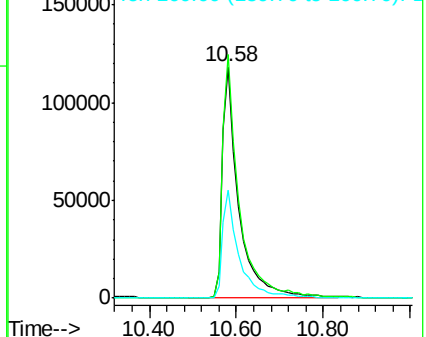


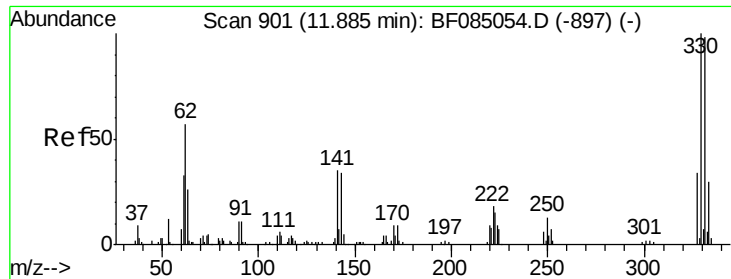




#41
 2,4,6-Tribromophenol
 Concen: 123.96 ng
 RT: 11.88 min Scan# 901
 Delta R.T. -0.00 min
 Lab File: BF085061.D
 Acq: 13 Feb 2016 1:27

Instrument :
 BNA_F
 ClientSampleId :
 S4-B002(2-4)

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.4	78.5	117.7
141	37.3	28.6	42.8




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

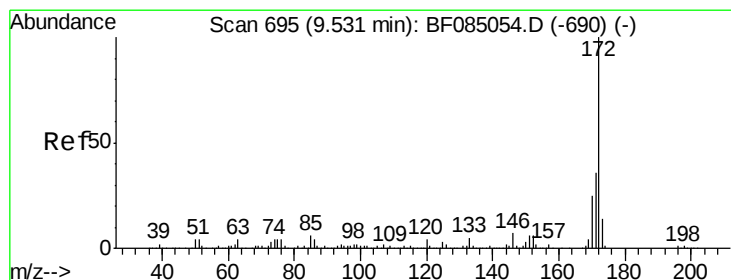
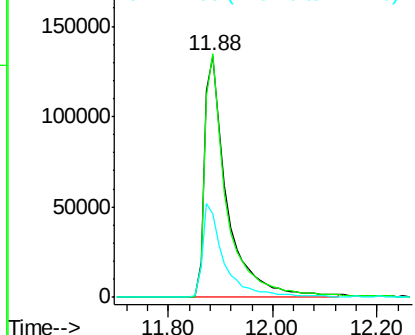



#44
 2-Fluorobiphenyl
 Concen: 82.41 ng
 RT: 9.53 min Scan# 695
 Delta R.T. -0.00 min
 Lab File: BF085061.D
 Acq: 13 Feb 2016 1:27

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.4	29.1	43.7
170	23.6	19.6	29.4

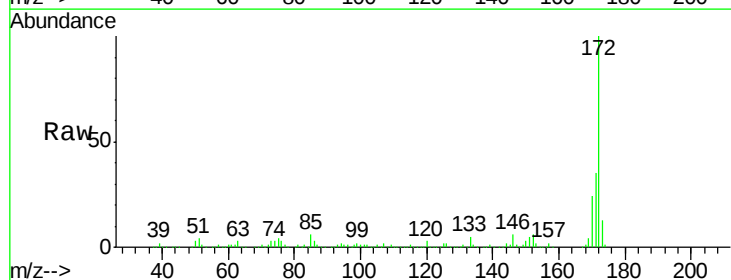

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

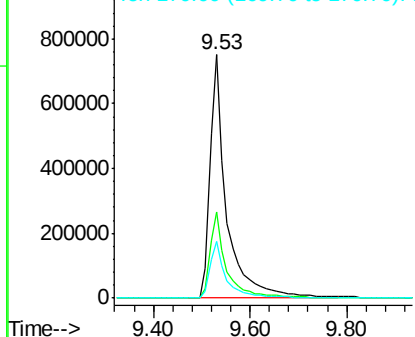

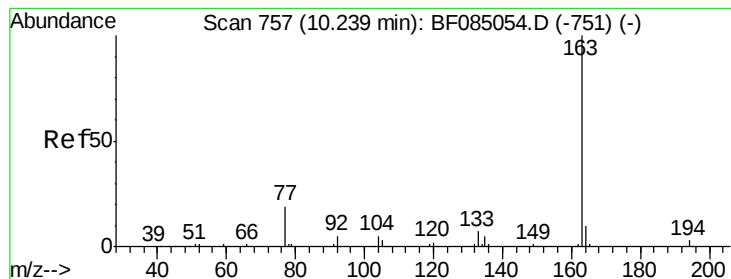

#49

Dimethylphthalate

Concen: 11.22 ng

RT: 10.22 min Scan# 755

Delta R.T. -0.02 min

Lab File: BF085061.D

Acq: 13 Feb 2016 1:27

Instrument :

BNA_F

ClientSampleId :

S4-B002(2-4)


Tot Ion:163 Resp: 264527

Ion Ratio Lower Upper

163 100

194 3.4 2.5 3.7




164 9.9 7.8 11.8



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

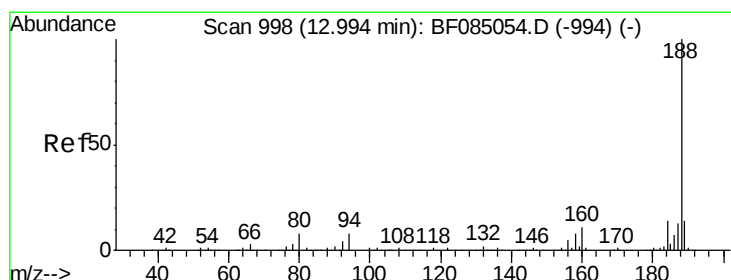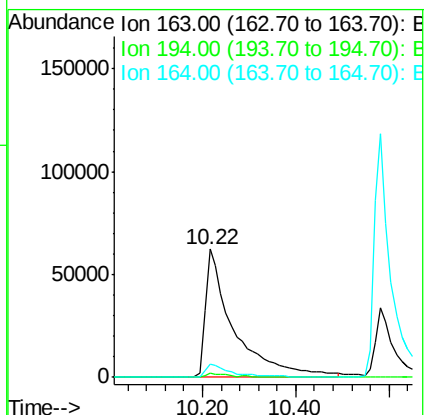

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 12.99 min Scan# 998

Delta R.T. -0.00 min

Lab File: BF085061.D

Acq: 13 Feb 2016 1:27


Tgt Ion:188 Resp: 592870

Ion Ratio Lower Upper

188 100

94 8.5 6.2 9.2



80 9.5 6.6 9.8




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

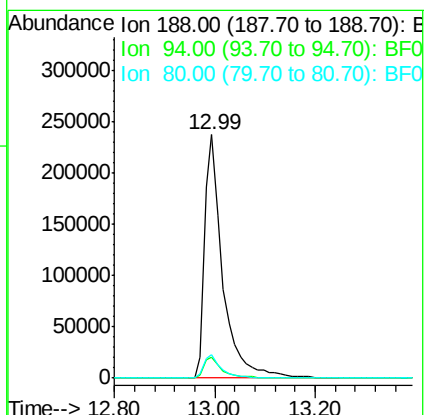

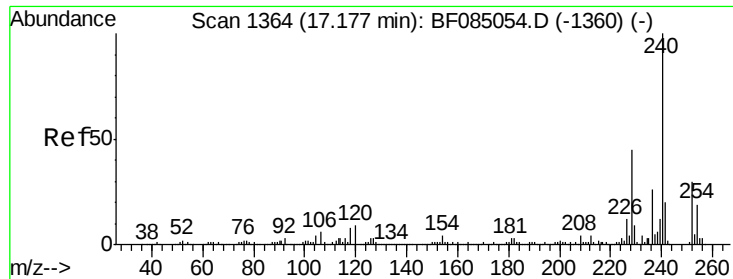

#75

Chrysene-d12

Concen: 20.00 ng

RT: 17.17 min Scan# 1363

Delta R.T. -0.01 min

Lab File: BF085061.D

Acq: 13 Feb 2016 1:27

Instrument :

BNA_F

ClientSampleId :

S4-B002(2-4)


Tot Ion:240 Resp: 441671

Ion Ratio Lower Upper

240 100

120 11.7 7.0 10.6#




236 25.0 20.5 30.7

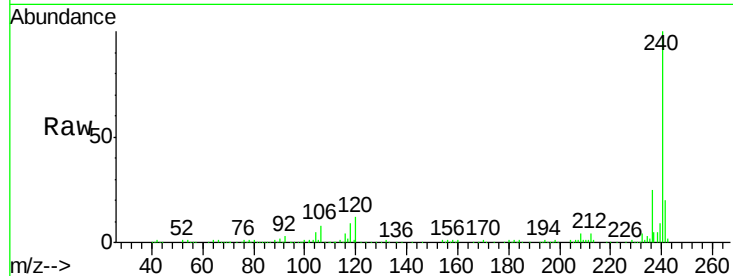

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

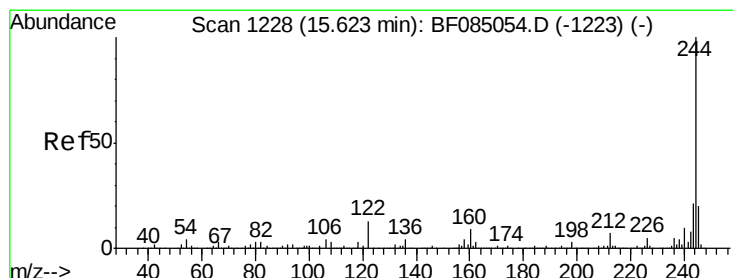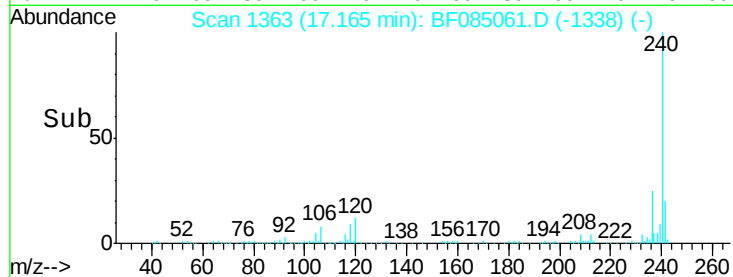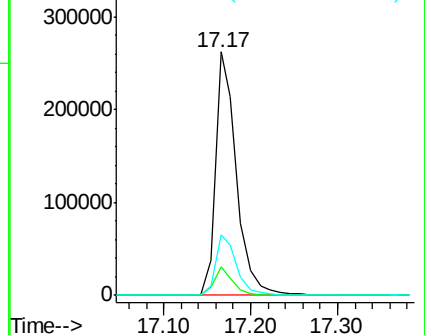

#78

Terphenyl-d14

Concen: 70.77 ng

RT: 15.62 min Scan# 1228

Delta R.T. -0.00 min

Lab File: BF085061.D

Acq: 13 Feb 2016 1:27


Tgt Ion:244 Resp: 1518708

Ion Ratio Lower Upper

244 100

212 7.4 6.0 9.0



122 12.6 10.1 15.1



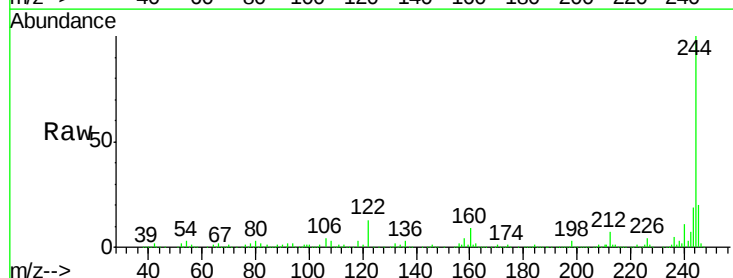


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

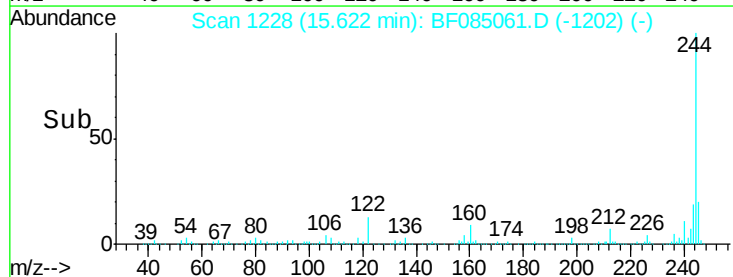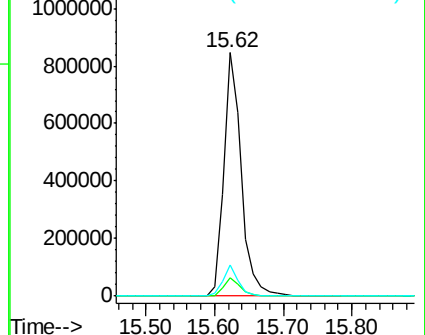

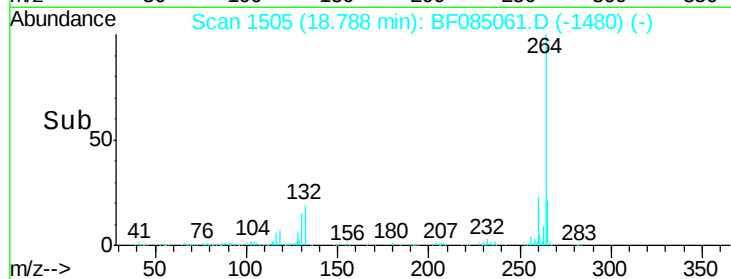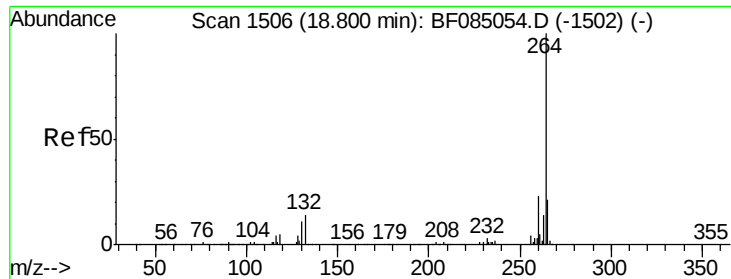

#86

Pervlene-d12

Concen: 20.00 ng

RT: 18.79 min Scan# 1505

Delta R.T. -0.01 min

Lab File: BF085061.D

Acq: 13 Feb 2016 1:27

Instrument :

BNA_F

ClientSampleId :

S4-B002(2-4)

Tot Ion: 264 Resp: 286434

Ion Ratio Lower Upper

264 100

260 23.2 18.5 27.7

265 21.3 16.7 25.1

