


Data Path : Z:\HPCHEM1\BNA F\DATA\BF021416\
 Data File : BF085059.D
 Acq On : 13 Feb 2016 00:16
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Feb 13 00:11:18 2016

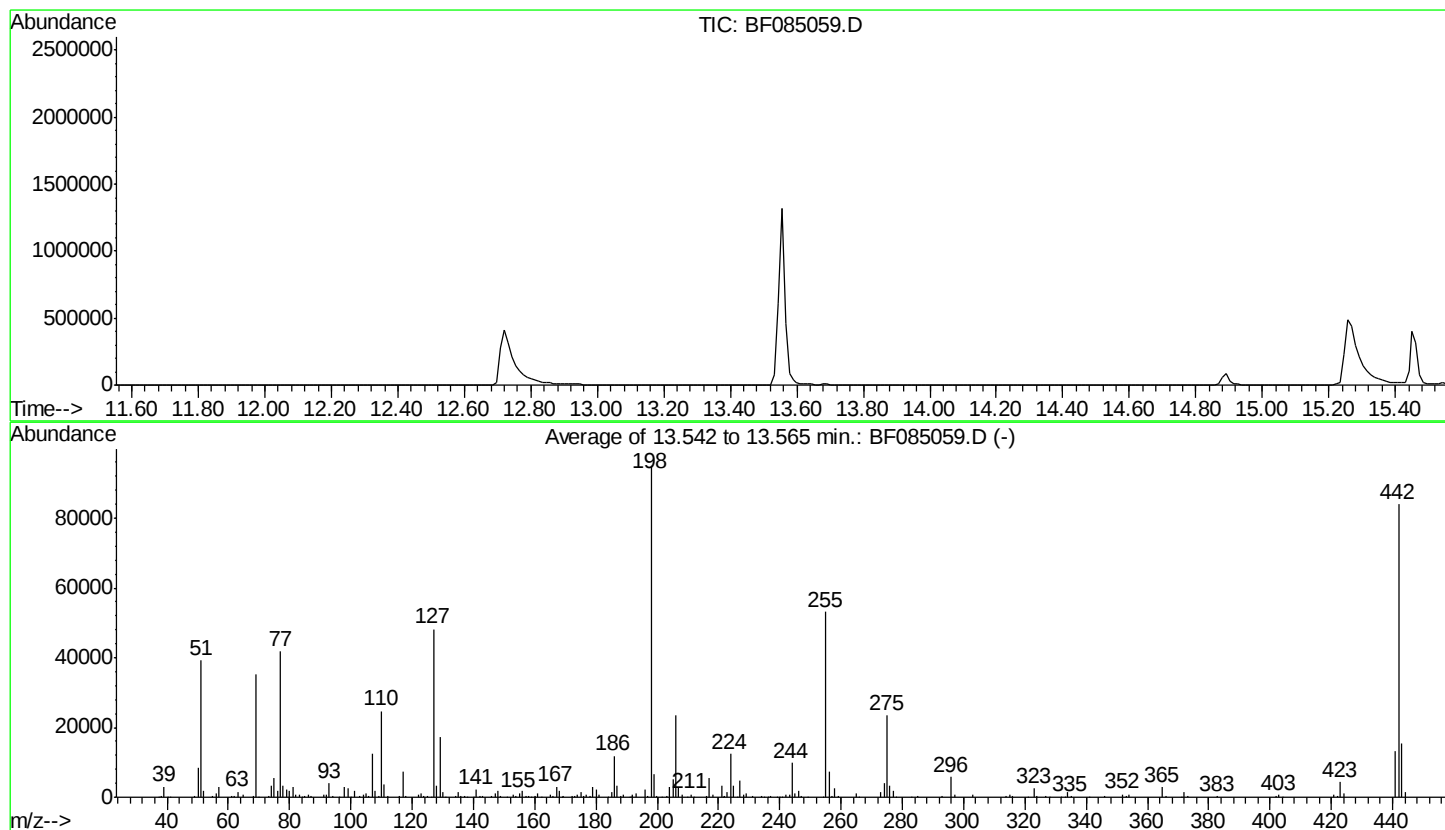

AutoFind: Scans 1046, 1047, 1048; Background Corrected with Scan 1041

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	39100	PASS
68	69	0.00	2	1.4	504	PASS
69	198	0.00	100	37.0	35179	PASS
70	69	0.00	2	0.3	110	PASS
127	198	10	80	50.7	48210	PASS
197	198	0.00	2	0.5	476	PASS
198	198	100	100	100.0	95053	PASS
199	198	5	9	6.8	6436	PASS
275	198	10	60	24.6	23366	PASS
365	198	1	100	3.1	2912	PASS
441	442	0.01	24	15.8	13304	PASS
442	198	50	100	88.3	83976	PASS
443	442	15	24	18.5	15565	PASS