


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021417\
 Data File : BF092933.D
 Acq On : 14 Feb 2017 10:12
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 13 18:04:38 2017

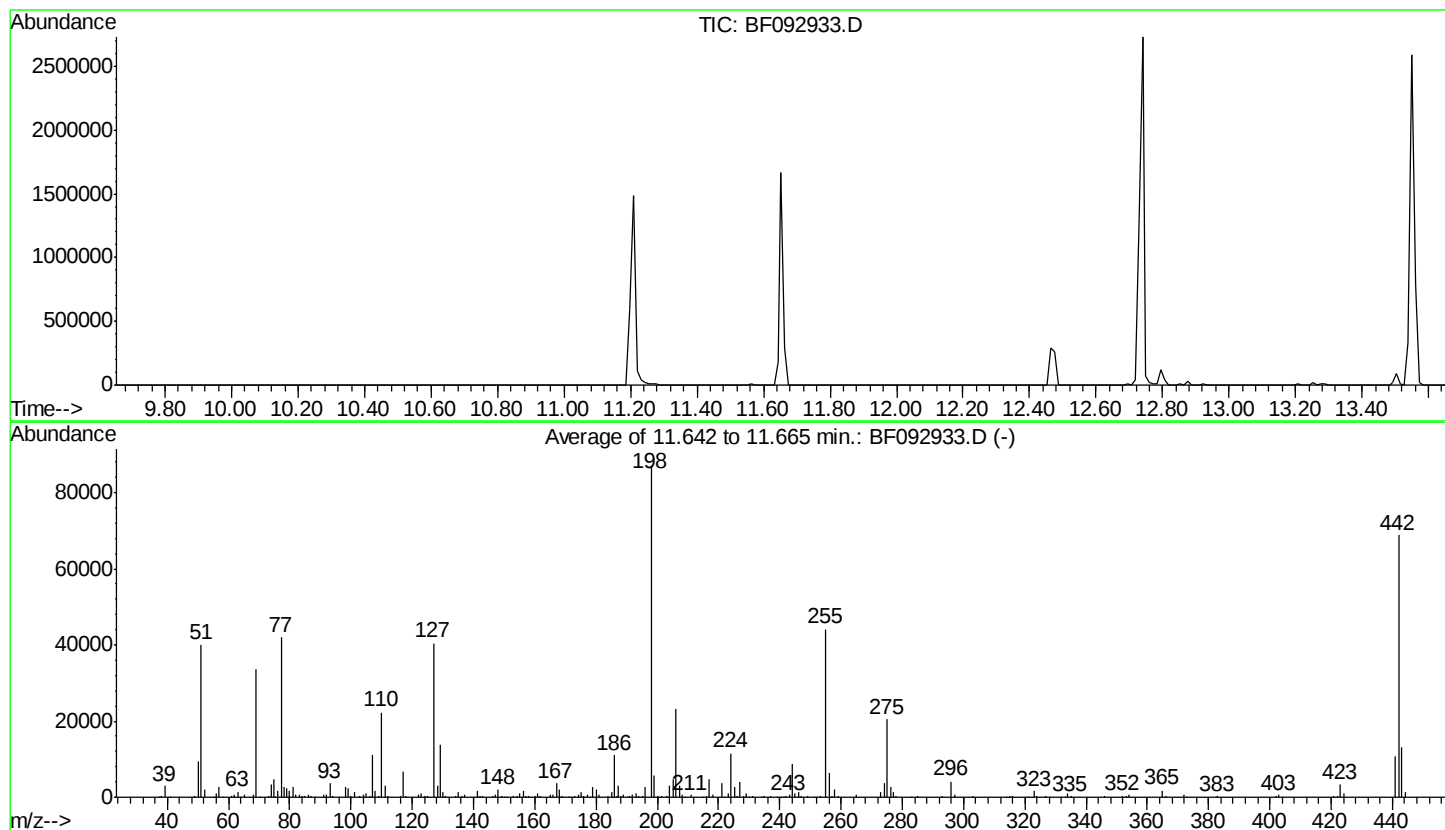

AutoFind: Scans 836, 837, 838; Background Corrected with Scan 833

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	40154	PASS
68	69	0.00	2	1.6	534	PASS
69	198	0.00	100	38.6	33579	PASS
70	69	0.00	2	0.3	111	PASS
127	198	10	80	46.5	40490	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	87103	PASS
199	198	5	9	6.5	5649	PASS
275	198	10	60	23.4	20379	PASS
365	198	1	100	2.1	1849	PASS
441	442	0.01	24	15.5	10682	PASS
442	198	50	100	79.0	68794	PASS
443	442	15	24	18.9	12984	PASS