
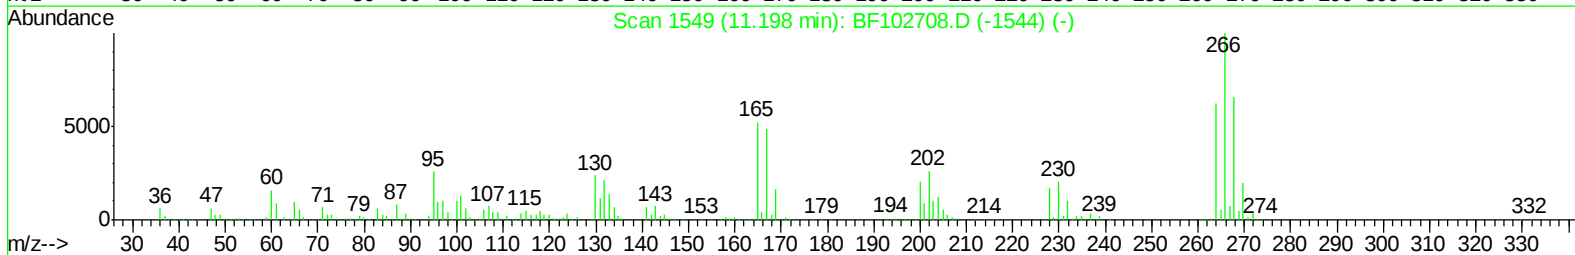
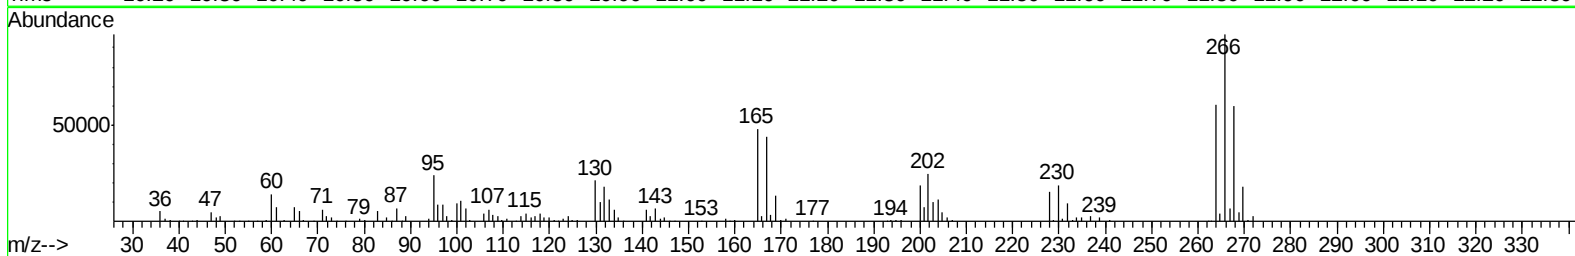


Data Path : Z:\HPCHEM1\BNA F\DATA\BF021418\
Data File : BF102976.D
Acq On : 14 Feb 2018 9:12
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 15 02:37:54 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 00:38:27 2018
Response via : Initial Calibration

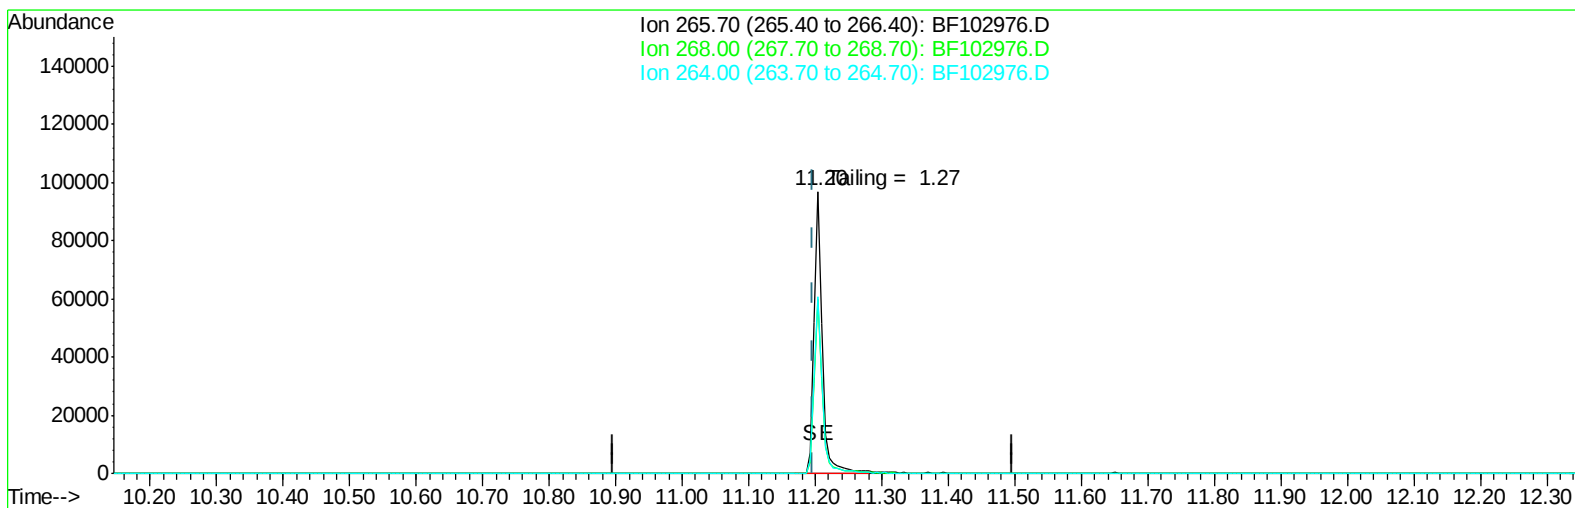

TIC: BF102976.D

(69) Pentachlorophenol (C)




11.204min (+0.006) 29027.65ng

response 86698

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.62
264.00	61.90	62.76
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF021418\
Data File : BF102976.D
Acq On : 14 Feb 2018 9:12
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 15 02:37:54 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 00:38:27 2018
Response via : Initial Calibration

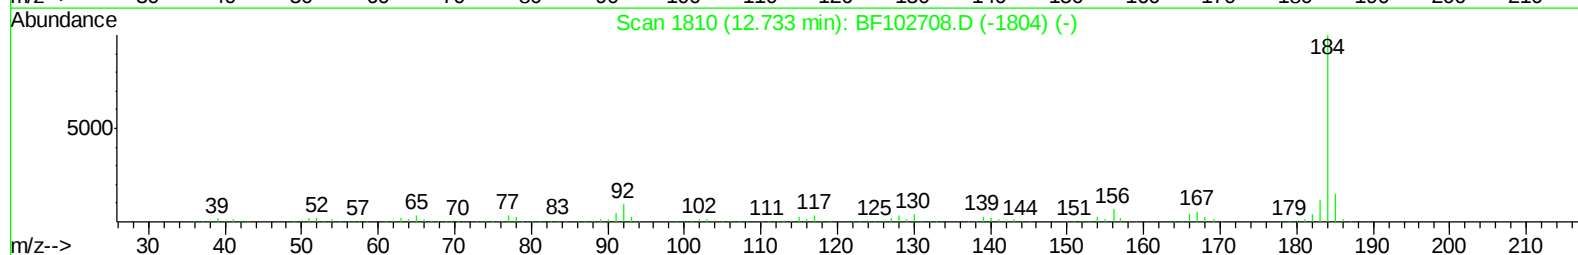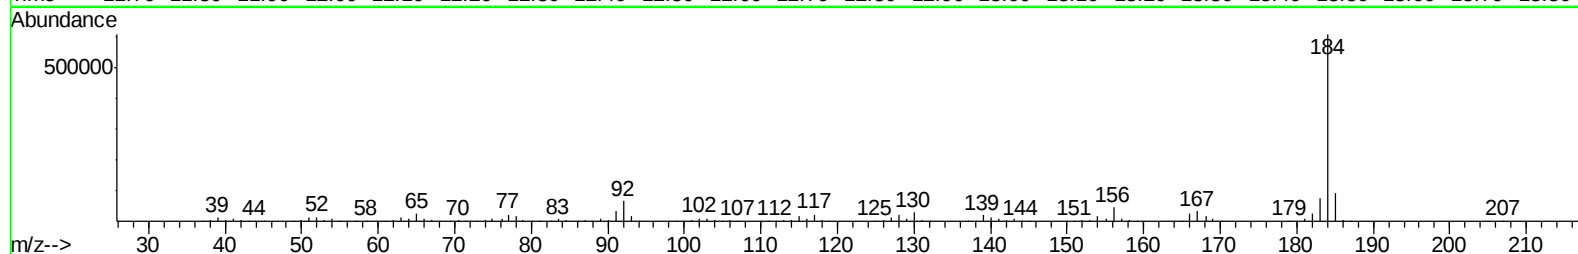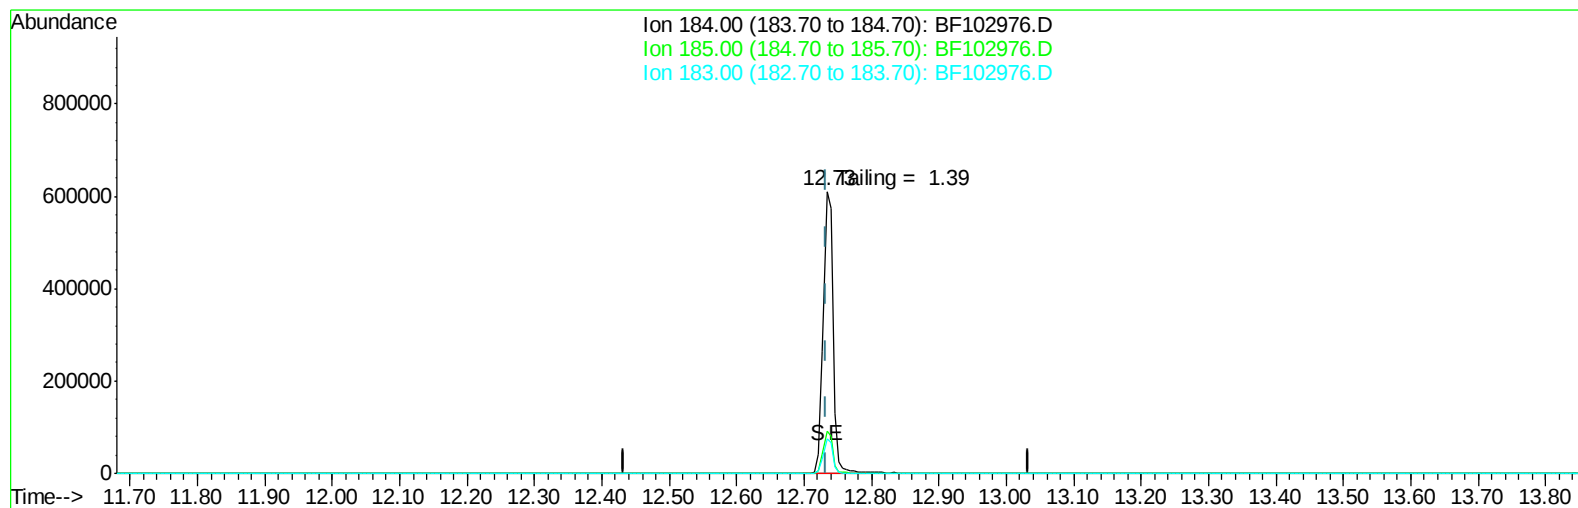

TIC: BF102976.D

(76) Benzidine

12.733min (+0.000) 0.00ng

response 601595

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.04
183.00	11.60	12.18
0.00	0.00	0.00