
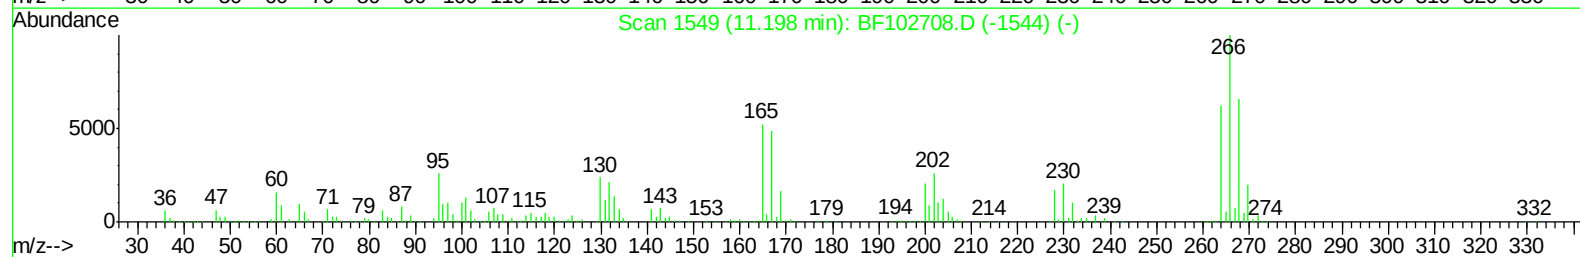
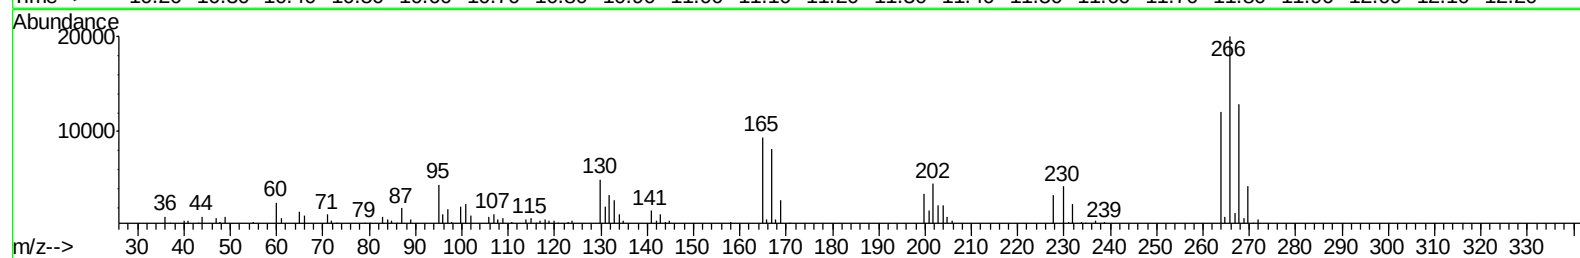


Data Path : Z:\HPCHEM1\BNA F\DATA\BF021418\
 Data File : BF103003.D
 Acq On : 14 Feb 2018 22:24
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 15 02:38:53 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 00:38:27 2018
 Response via : Initial Calibration

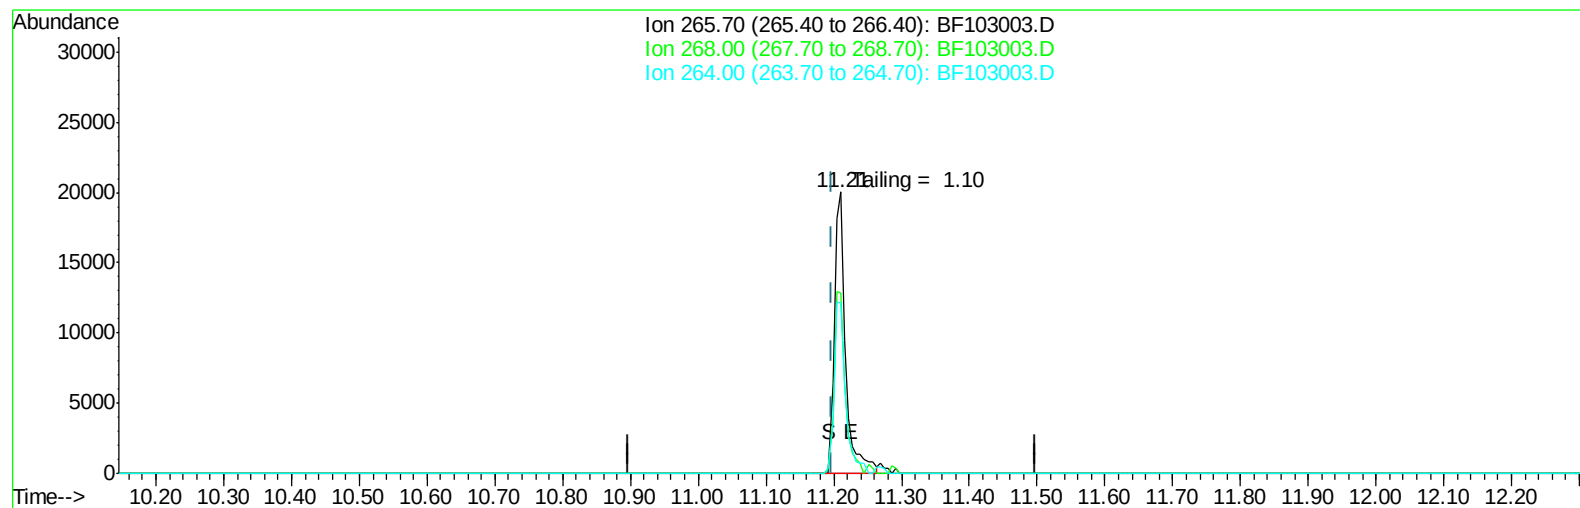

TIC: BF103003.D

(69) Pentachlorophenol (C)




11.210min (+0.012) 12762.70ng

response 23868

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.21
264.00	61.90	60.37
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF021418\
 Data File : BF103003.D
 Acq On : 14 Feb 2018 22:24
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 15 02:38:53 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 00:38:27 2018
 Response via : Initial Calibration

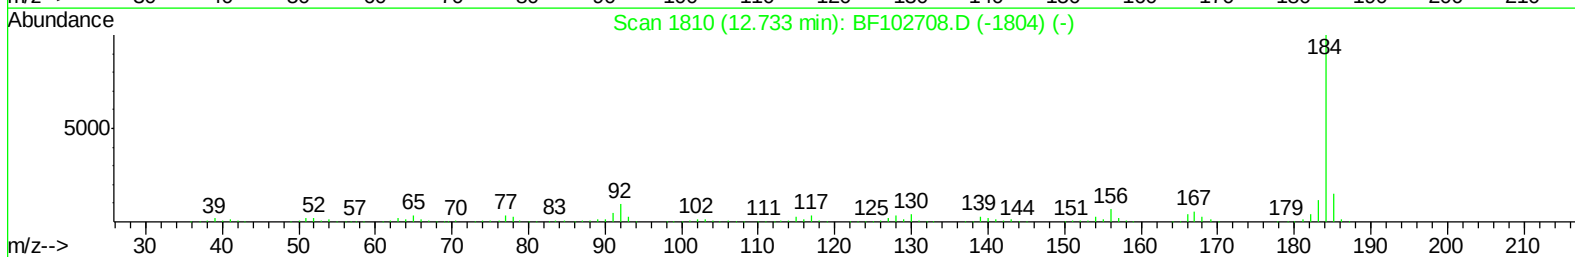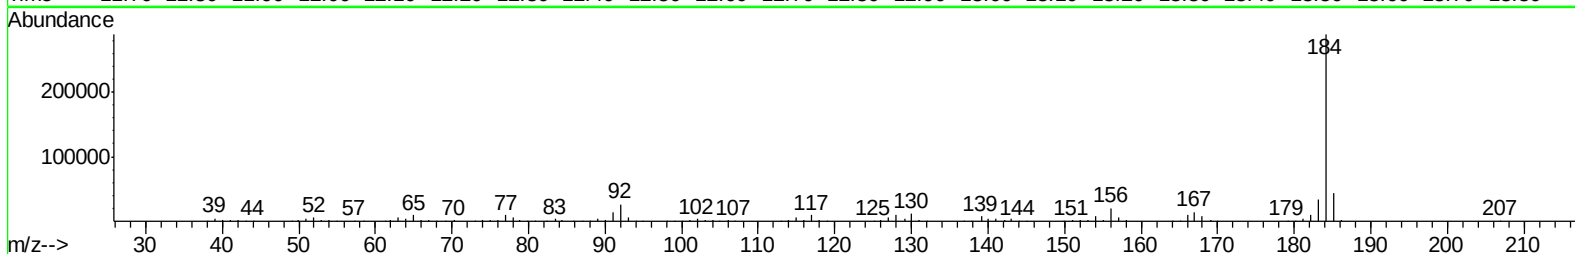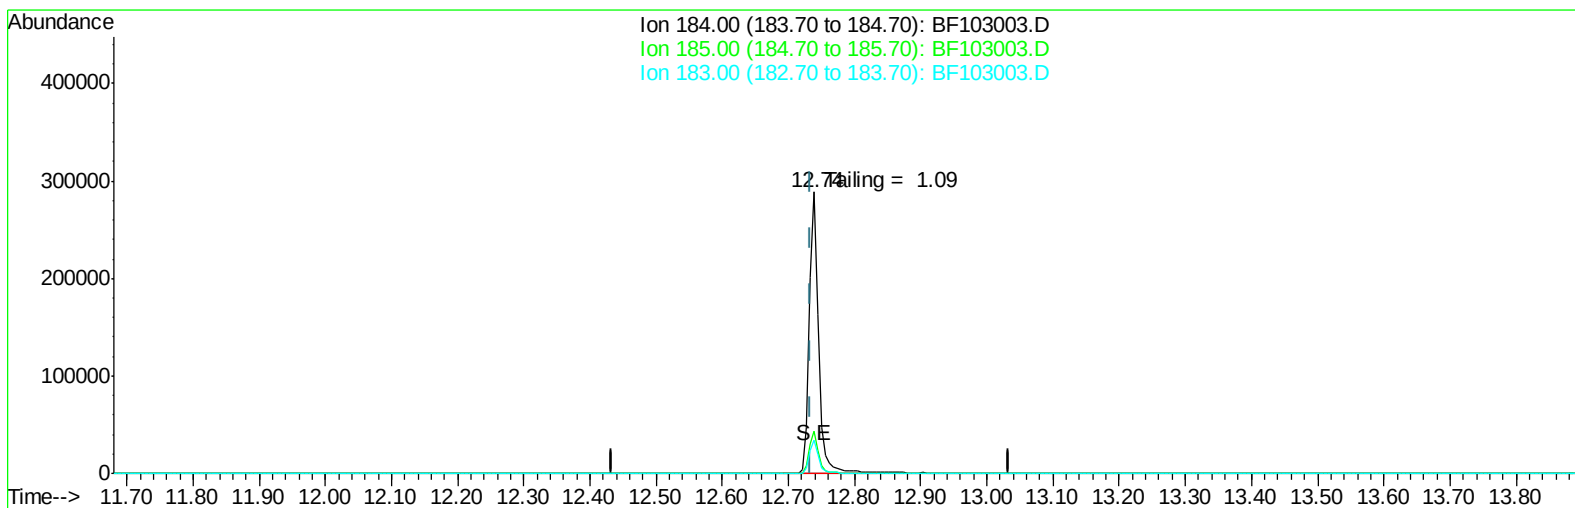

TIC: BF103003.D

(76) Benzidine

12.739min (+0.006) 0.00ng

response 289553

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.98
183.00	11.60	11.81
0.00	0.00	0.00