


Data Path : Z:\HPCHEM1\BNA F\Data\BF021418\
 Data File : BF102976.D
 Acq On : 14 Feb 2018 9:12
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 05 00:38:27 2018

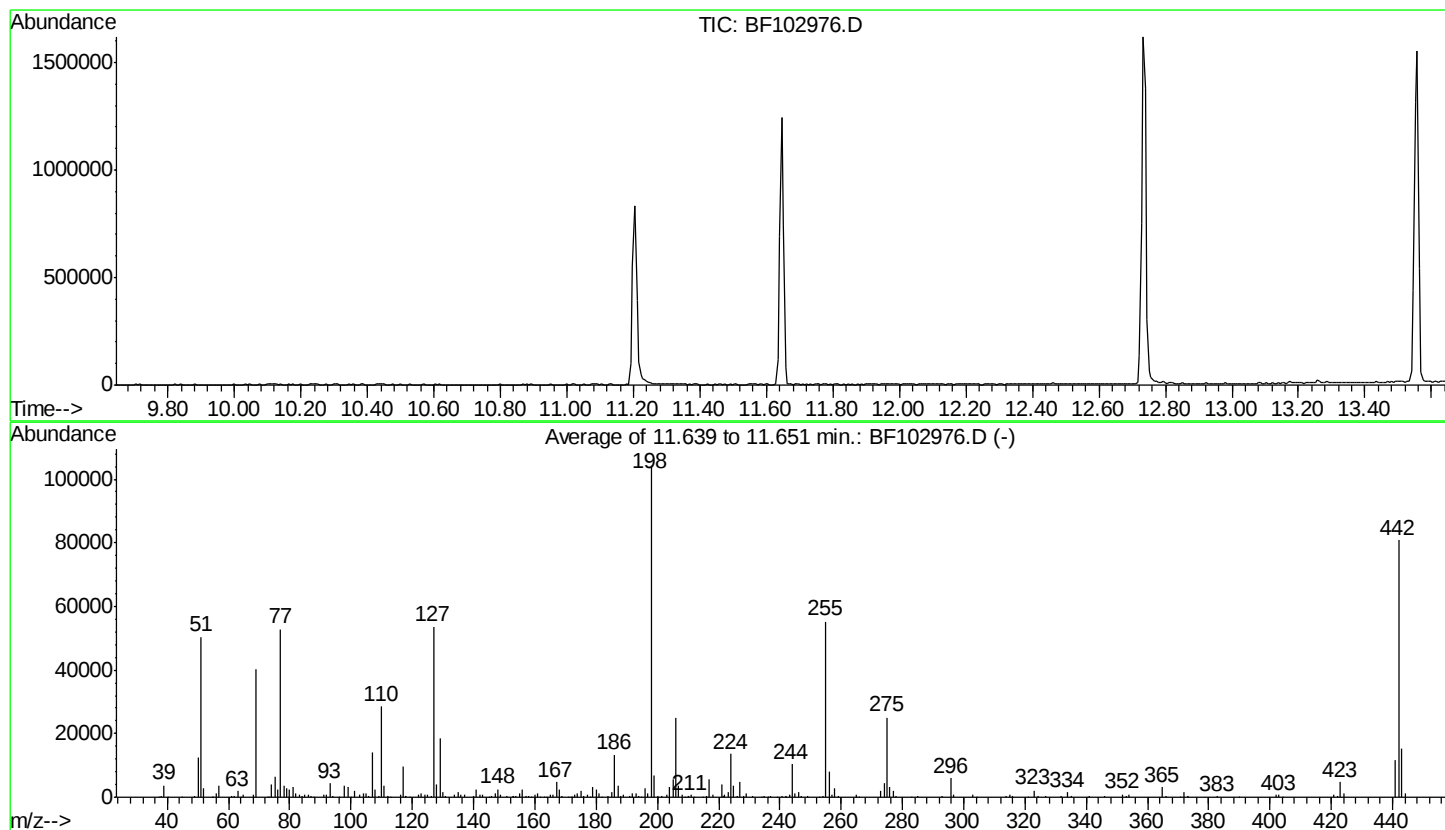

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.4	50450	PASS
68	69	0.00	2	1.7	667	PASS
69	198	0.00	100	38.6	40192	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.5	53640	PASS
197	198	0.00	2	1.0	1046	PASS
198	198	100	100	100.0	104256	PASS
199	198	5	9	6.7	6980	PASS
275	198	10	60	24.1	25120	PASS
365	198	1	100	3.0	3111	PASS
441	443	0.01	100	78.5	11882	PASS
442	198	50	100	77.5	80816	PASS
443	442	15	24	18.7	15139	PASS