


Data Path : Z:\HPCHEM1\BNA F\Data\BF021418\
 Data File : BF103003.D
 Acq On : 14 Feb 2018 22:24
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 05 00:38:27 2018

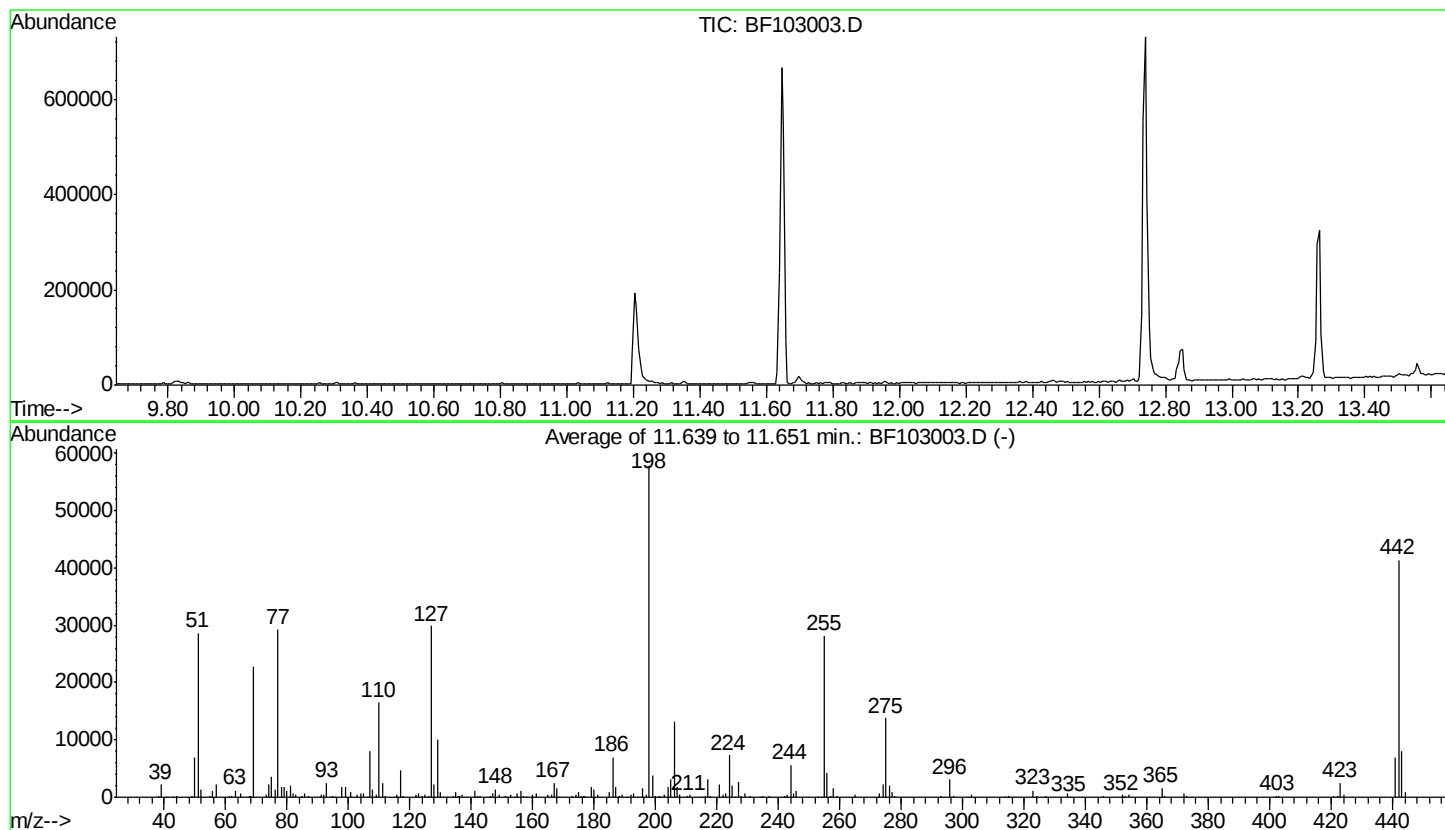

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.5	28613	PASS
68	69	0.00	2	1.4	325	PASS
69	198	0.00	100	39.5	22824	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.7	29893	PASS
197	198	0.00	2	0.9	501	PASS
198	198	100	100	100.0	57818	PASS
199	198	5	9	6.7	3889	PASS
275	198	10	60	23.8	13734	PASS
365	198	1	100	2.8	1644	PASS
441	443	0.01	100	84.0	6821	PASS
442	198	50	100	71.6	41407	PASS
443	442	15	24	19.6	8125	PASS