
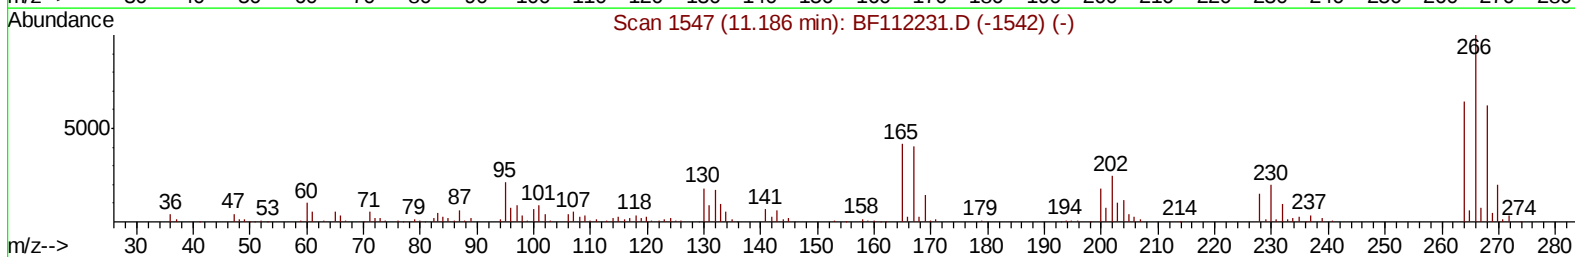
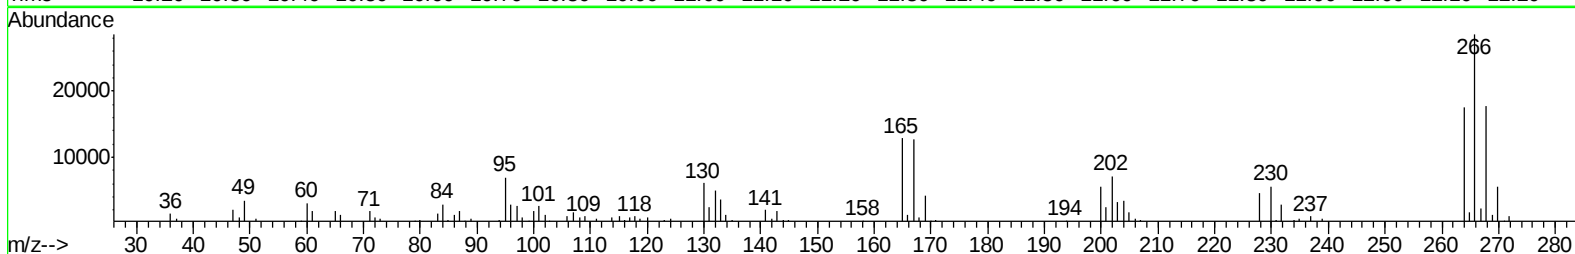


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021419\
Data File : BF112559.D
Acq On : 14 Feb 2019 10:51
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 15 07:41:36 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

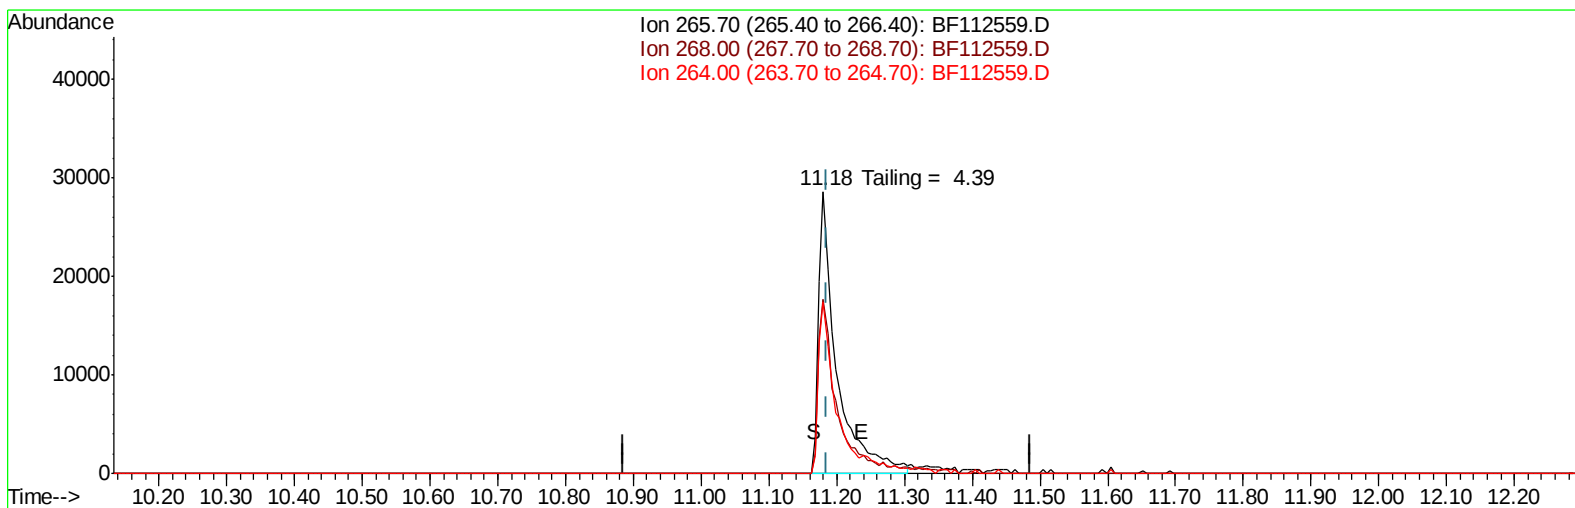

TIC: BF112559.D

(70) Pentachlorophenol (C)




11.181min (-0.006) 31875.45ng

response 51178

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	61.98
264.00	63.60	61.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021419\
Data File : BF112559.D
Acq On : 14 Feb 2019 10:51
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 15 07:41:36 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

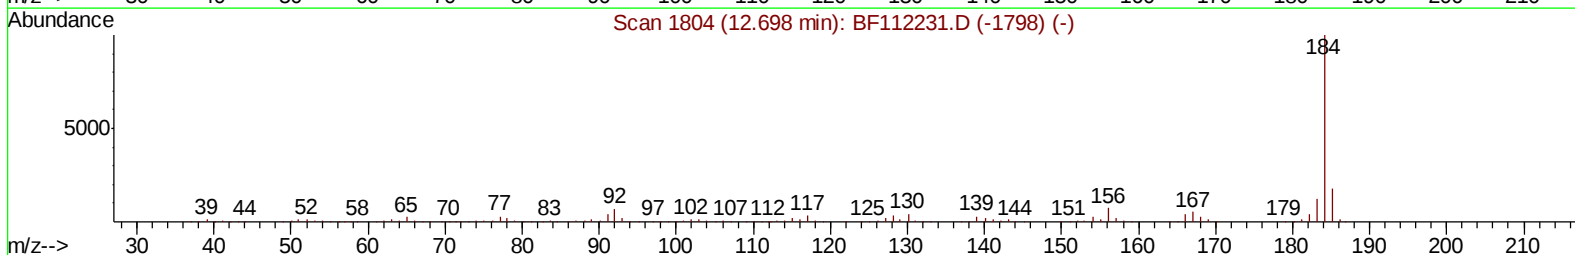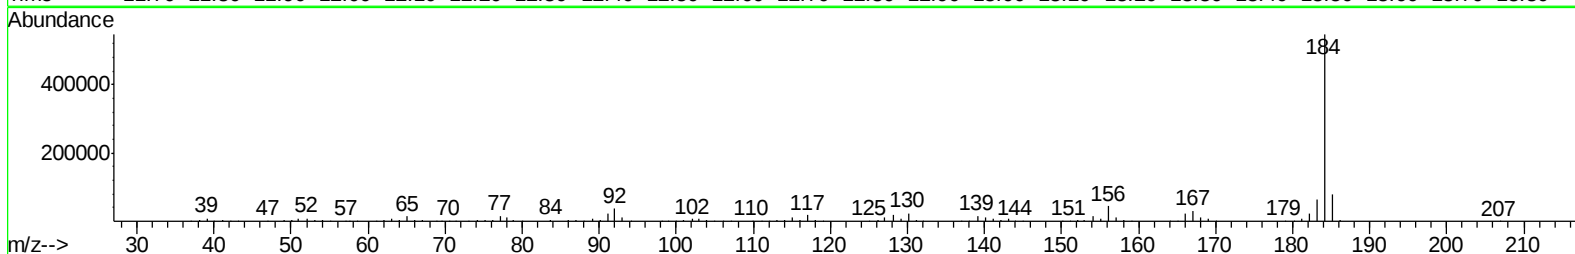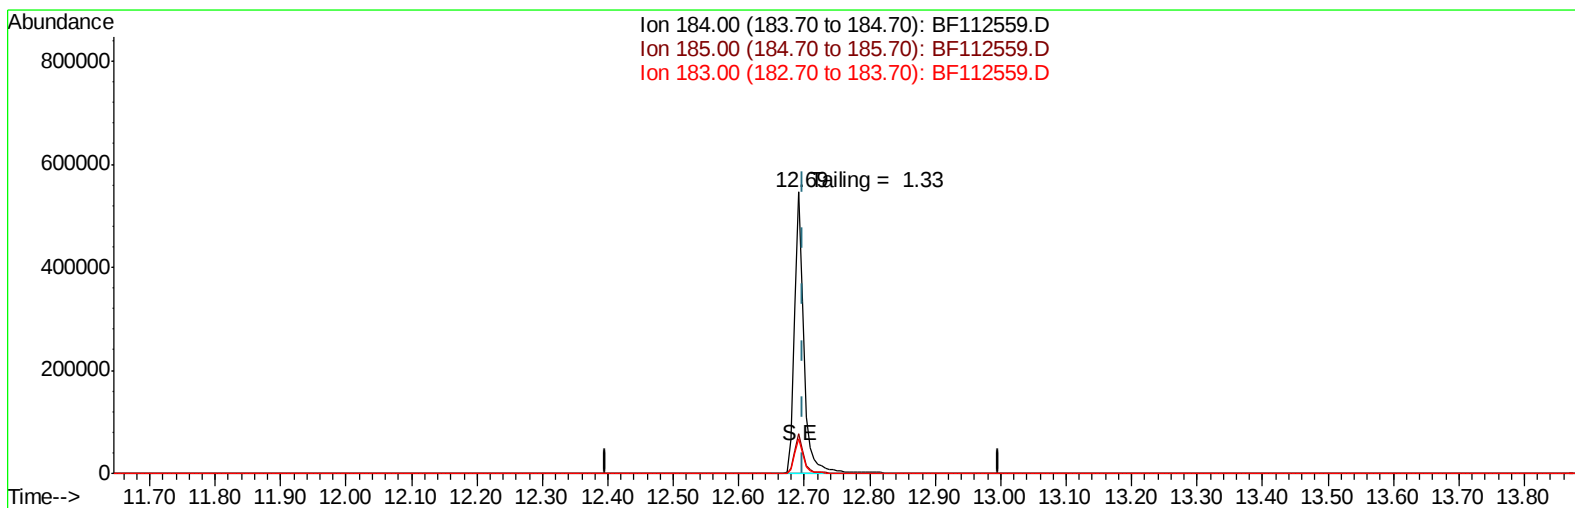

TIC: BF112559.D

(77) Benzidine

12.692min (-0.006) 0.00ng

response 550380

Ion	Exp%	Act%
184.00	100	100
185.00	17.40	14.31
183.00	12.50	12.06
0.00	0.00	0.00