


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021419\
 Data File : BF112559.D
 Acq On : 14 Feb 2019 10:51
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 28 10:38:18 2019

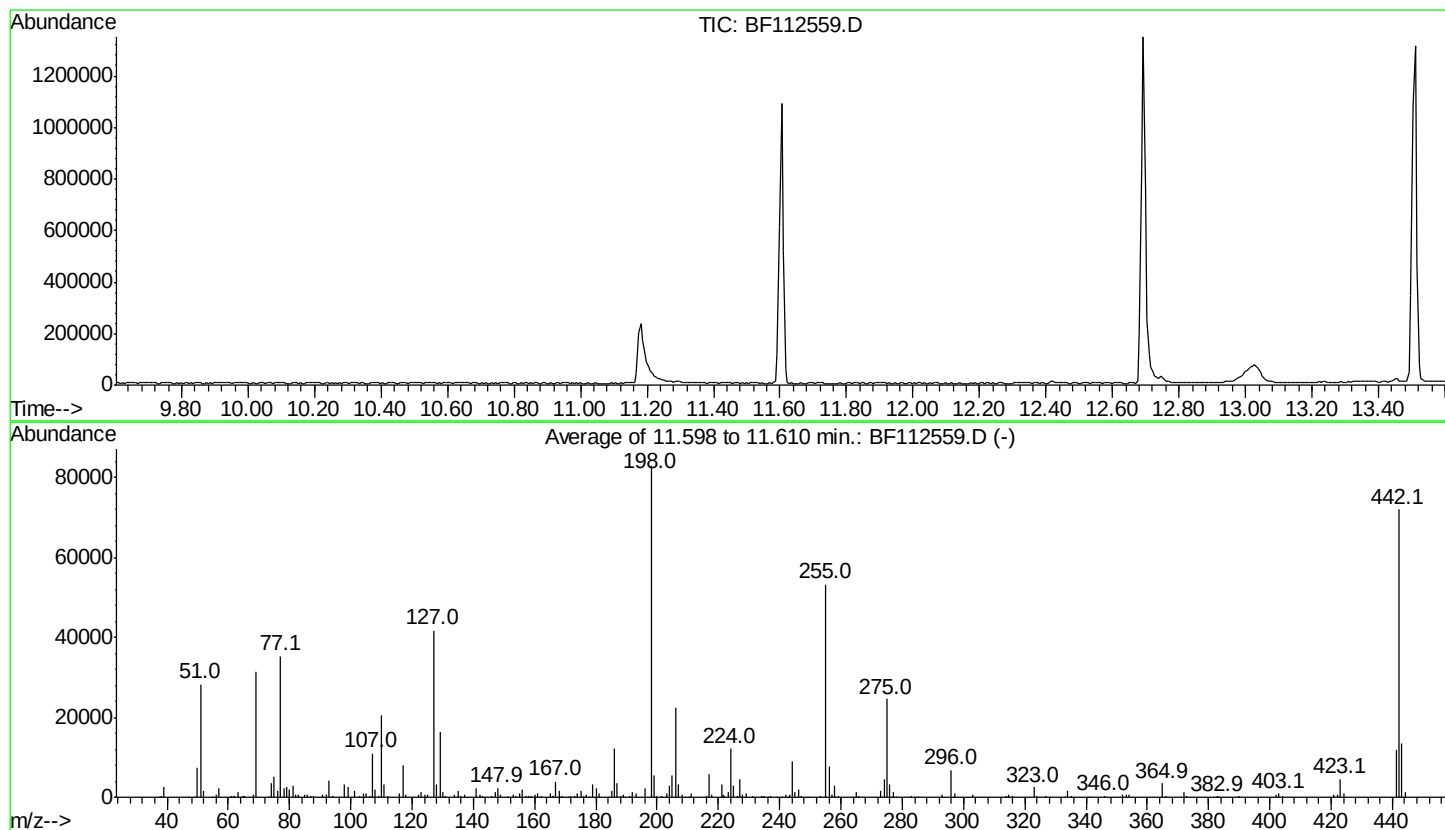

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	28247	PASS
68	69	0.00	2	1.9	611	PASS
69	198	0.00	100	37.9	31495	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.3	41765	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	83008	PASS
199	198	5	9	6.7	5575	PASS
275	198	10	60	29.7	24630	PASS
365	198	1	100	4.1	3431	PASS
441	198	0.01	100	14.2	11796	PASS
442	198	50	100	86.8	72029	PASS
443	442	15	24	18.8	13541	PASS