
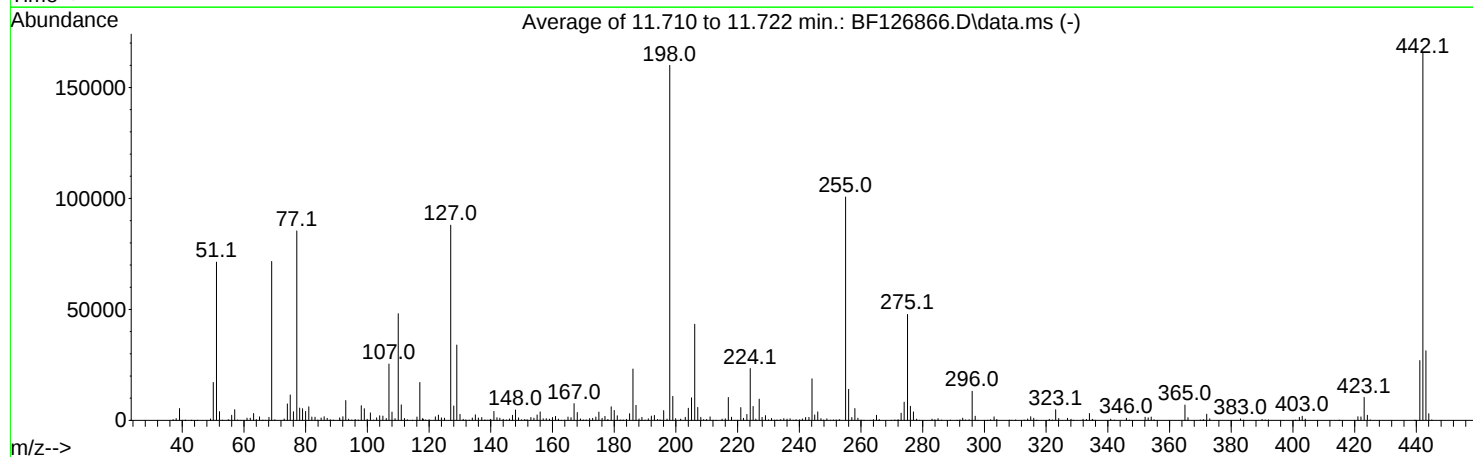


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021422\
 Data File : BF126866.D
 Acq On : 14 Feb 2022 12:53
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 10 00:44:00 2022

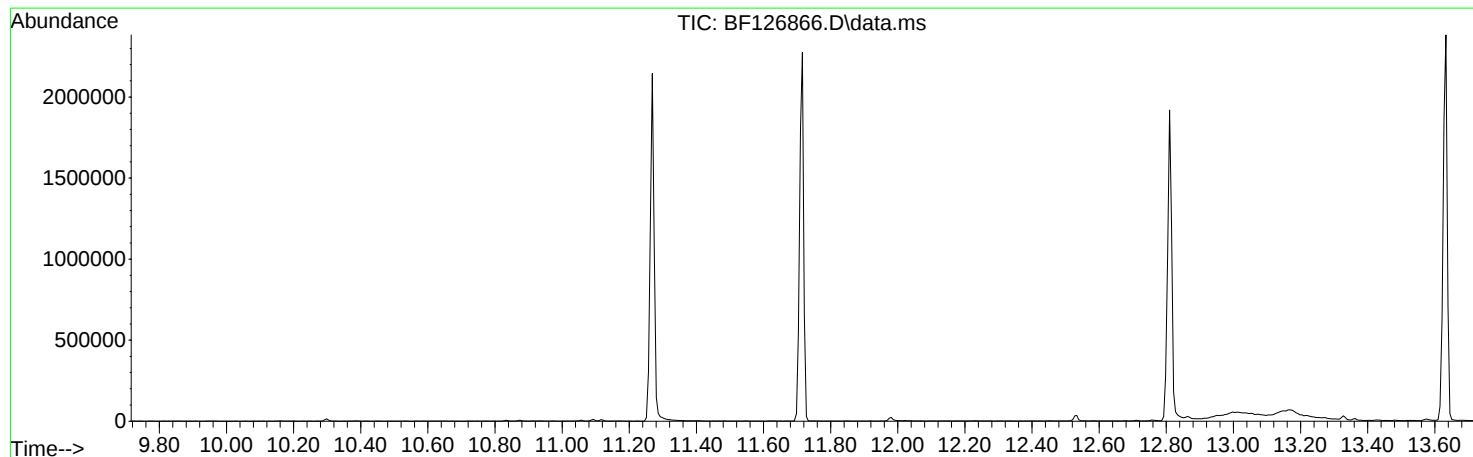

AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.6	71308	PASS
68	69	0.00	2	2.0	1410	PASS
69	198	0.00	100	44.8	71602	PASS
70	69	0.00	2	0.5	326	PASS
127	198	10	80	55.0	87976	PASS
197	198	0.00	2	0.3	544	PASS
198	198	100	100	100.0	159979	PASS
199	198	5	9	6.7	10798	PASS
275	198	10	60	29.8	47741	PASS
365	198	1	100	4.3	6945	PASS
441	198	0.01	100	16.9	27003	PASS
442	442	50	100	100.0	165768	PASS
443	442	15	24	18.9	31360	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/14/2022	BNA_F	<u>BF126866.D</u>
Compound Name	Response	Retention Time
DDT	354583	13.633
DDD	4977	13.327
DDE	693	12.992
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5670	360253	1.57

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021422\
 Data File : BF126866.D
 Acq On : 14 Feb 2022 12:53
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 15 01:32:59 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 10 00:44:00 2022
 Response via : Initial Calibration

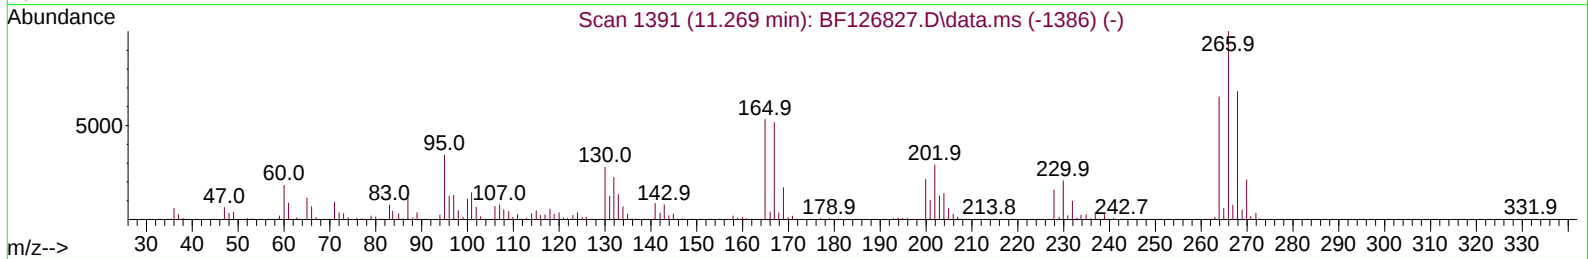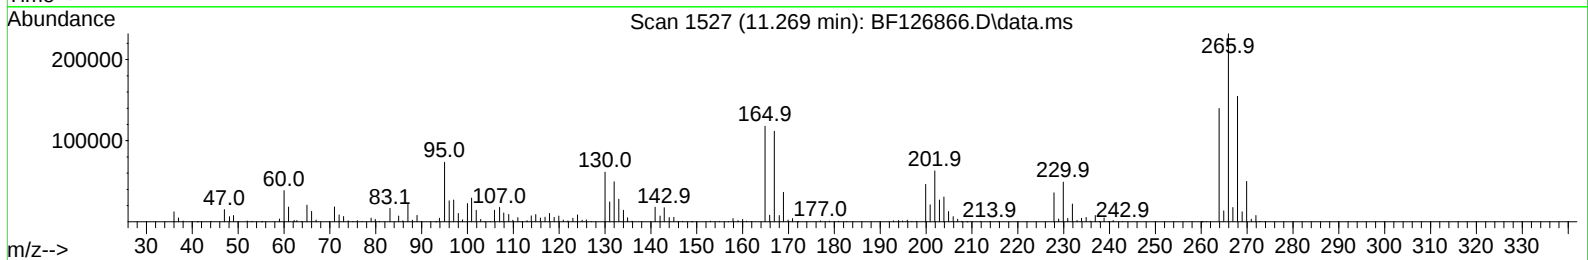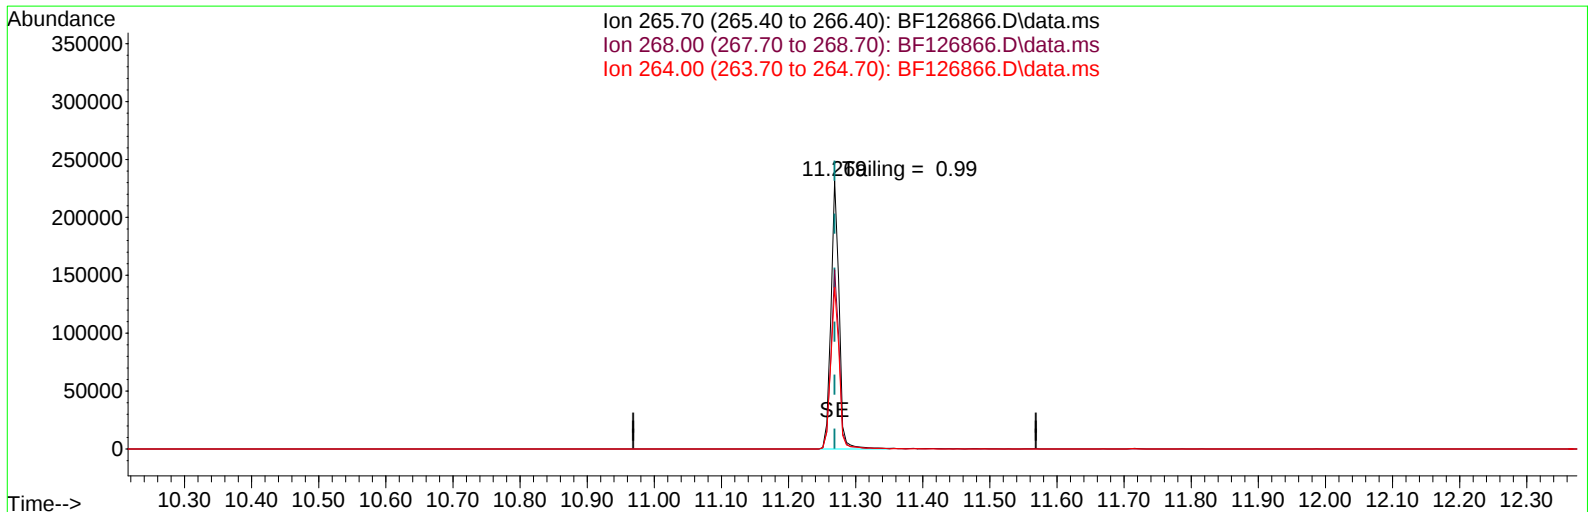

TIC: BF126866.D\data.ms

(70) Pentachlorophenol (C)

11.269min (+ 0.000) 35706.17 ng




response 194789

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.10	66.78
264.00	65.20	60.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021422\
Data File : BF126866.D
Acq On : 14 Feb 2022 12:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 15 01:32:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 10 00:44:00 2022
Response via : Initial Calibration

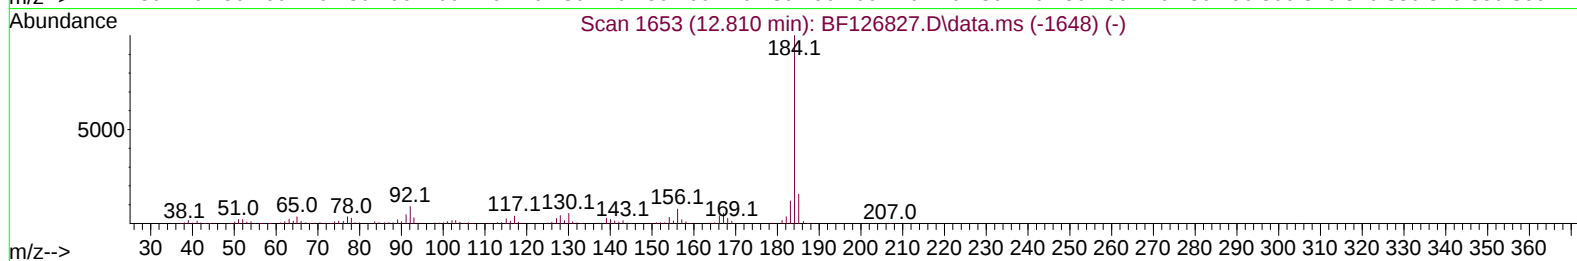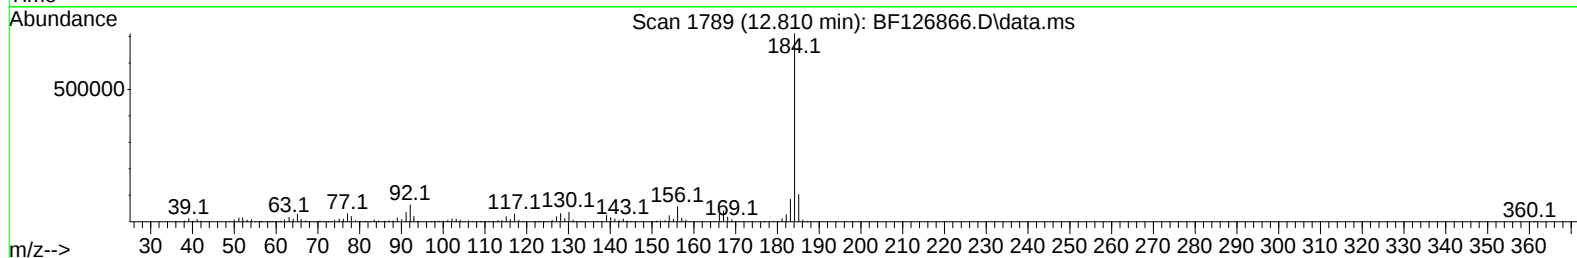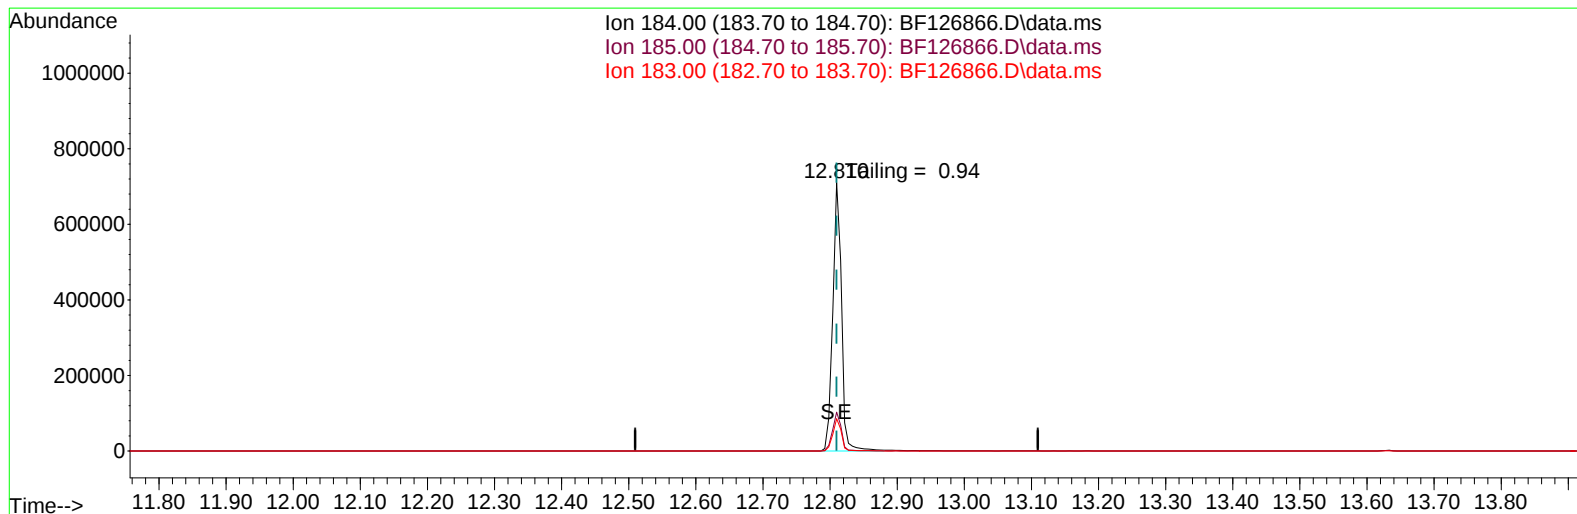

TIC: BF126866.D\data.ms

(77) Benzidine

12.810min (+ 0.000) 456071.46 ng

response 648047

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.60	14.53
183.00	12.00	12.06
0.00	0.00	0.00