
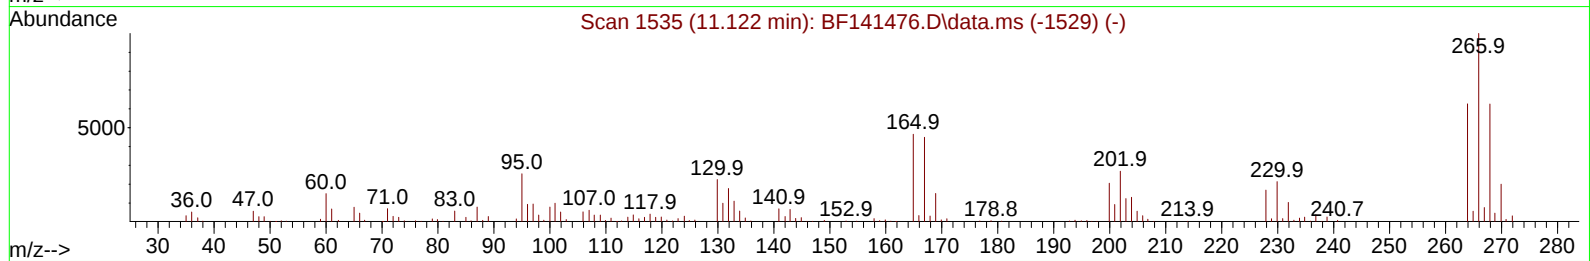
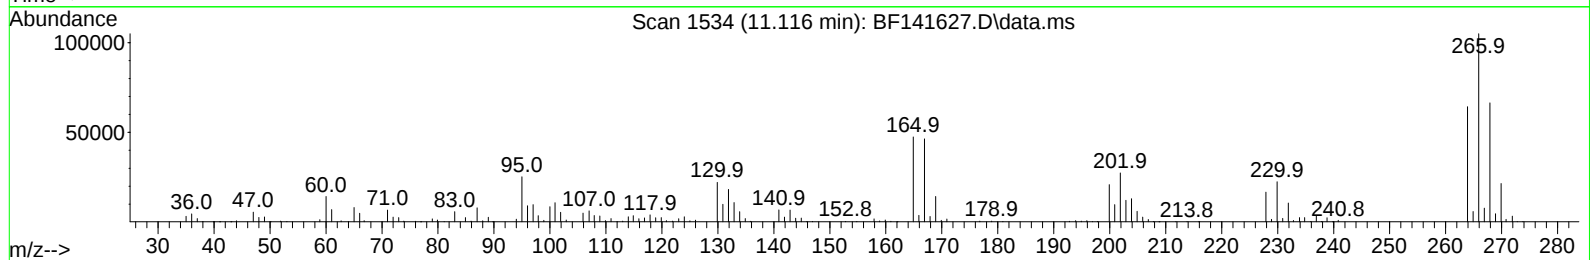


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021425\  
Data File : BF141627.D  
Acq On : 14 Feb 2025 09:19  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 10:34:35 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Feb 06 16:58:59 2025  
Response via : Initial Calibration

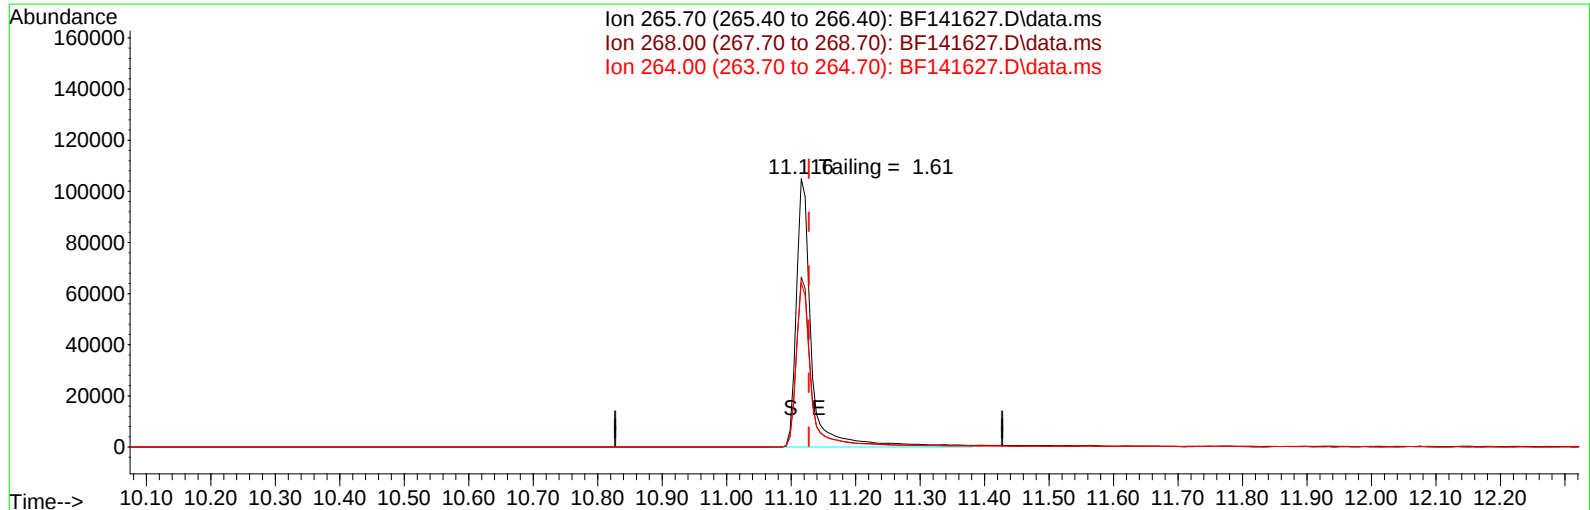

TIC: BF141627.D\data.ms

**(70) Pentachlorophenol (C)**




**11.116min (-0.012) 23053.12 ng**

**response 171340**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.60  | 63.29  |
| 264.00 | 62.60  | 61.26  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021425\  
Data File : BF141627.D  
Acq On : 14 Feb 2025 09:19  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 10:34:35 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020625.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Feb 06 16:58:59 2025  
Response via : Initial Calibration

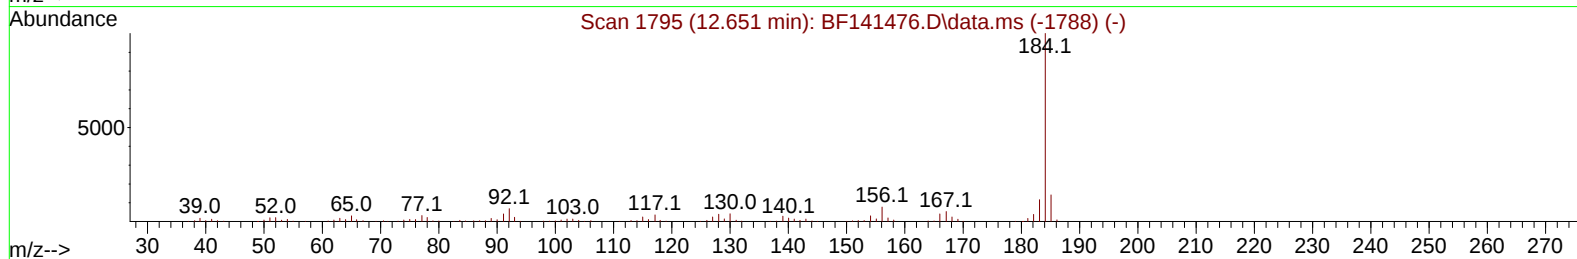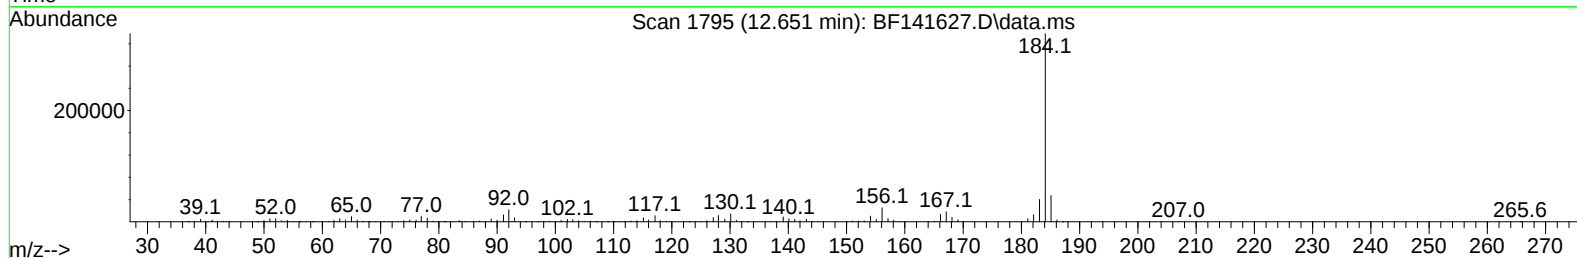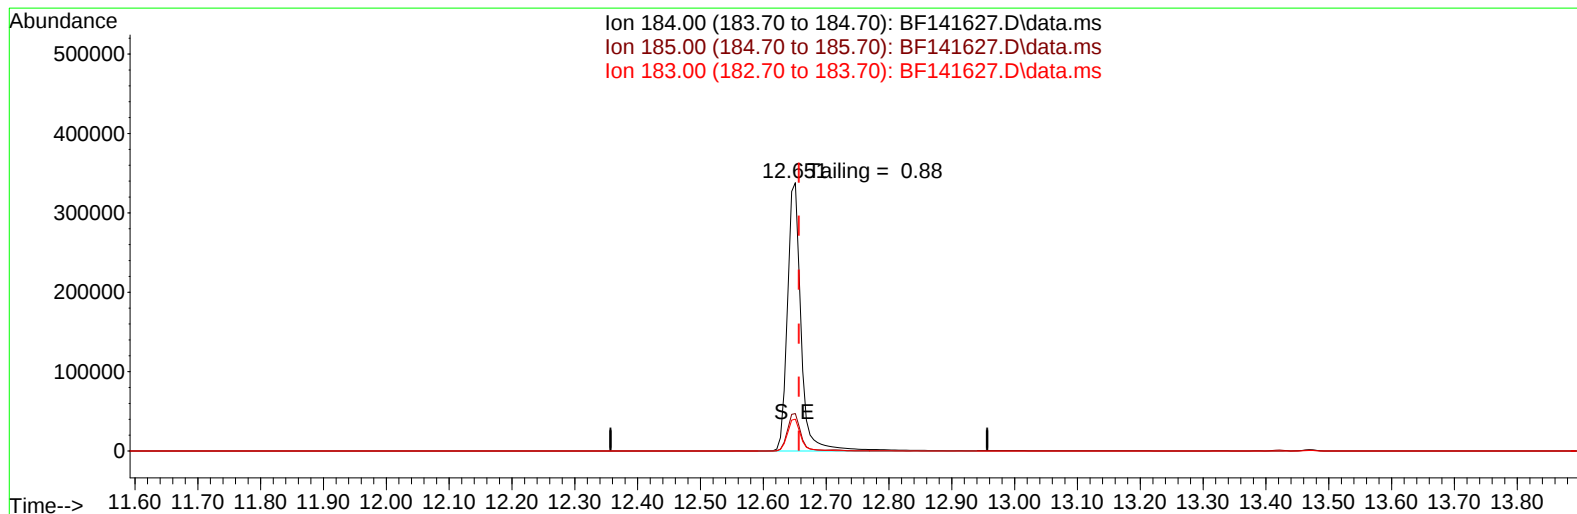

TIC: BF141627.D\data.ms

**(77) Benzidine**

12.651min (-0.006) 0.00 ng

response 512547

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.10  | 13.99  |
| 183.00 | 11.60  | 11.86  |
| 0.00   | 0.00   | 0.00   |