
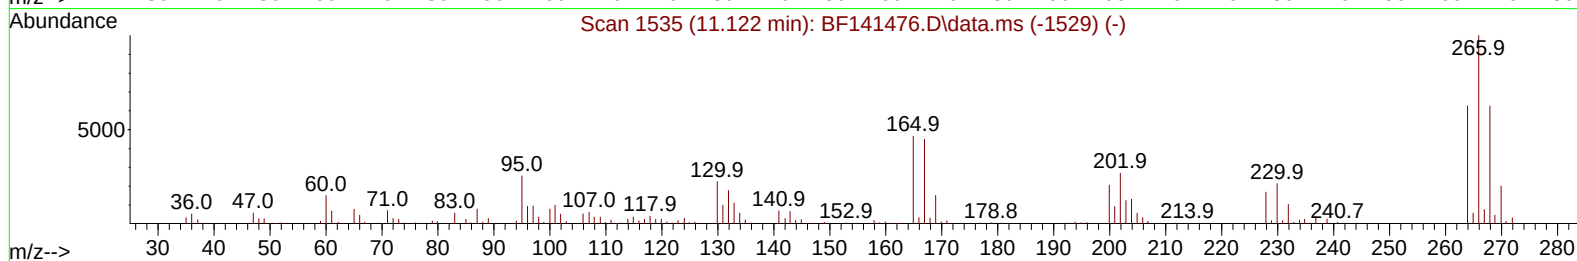
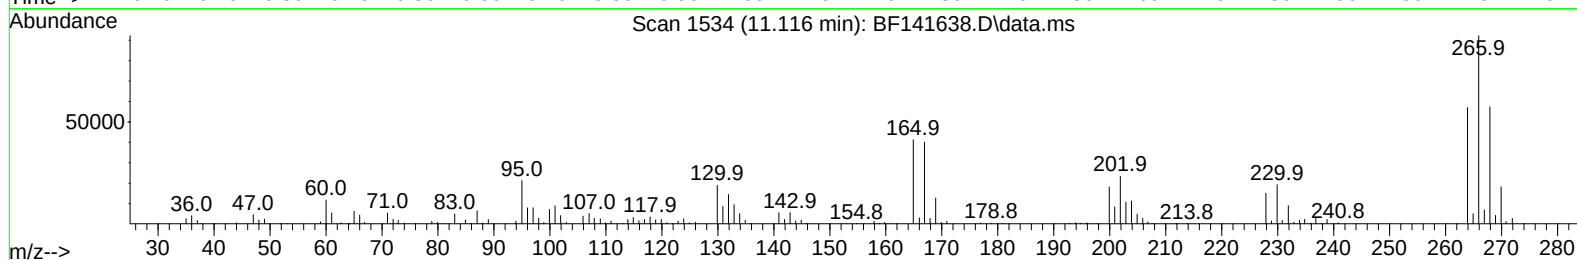


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021425\
Data File : BF141638.D
Acq On : 14 Feb 2025 14:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 15:24:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

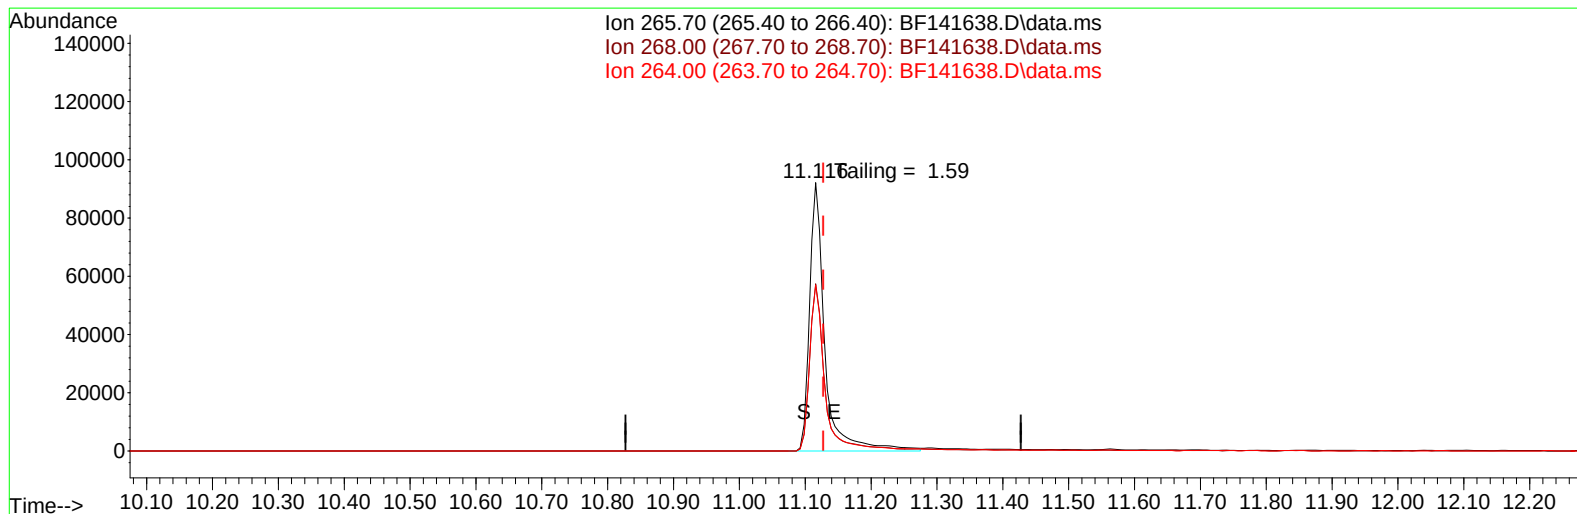

TIC: BF141638.D\data.ms

(70) Pentachlorophenol (C)




11.116min (-0.011) 158475.01 ng

response 149272

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.28
264.00	62.60	61.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021425\
Data File : BF141638.D
Acq On : 14 Feb 2025 14:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 15:24:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

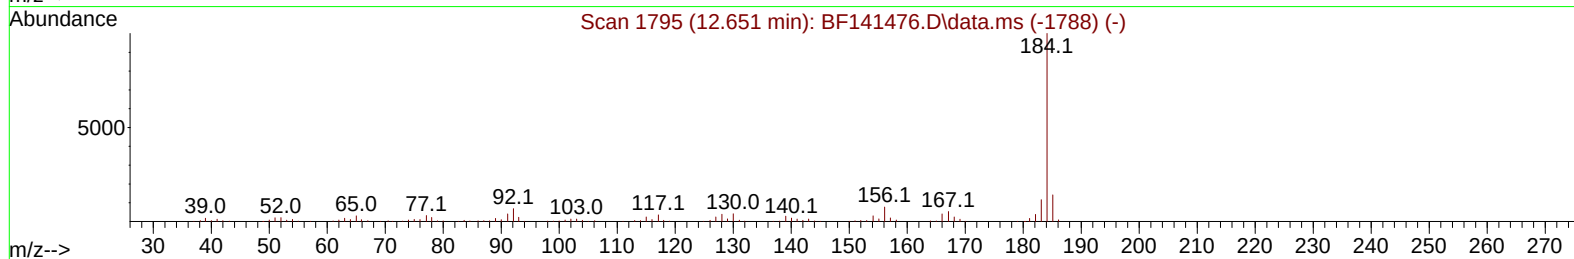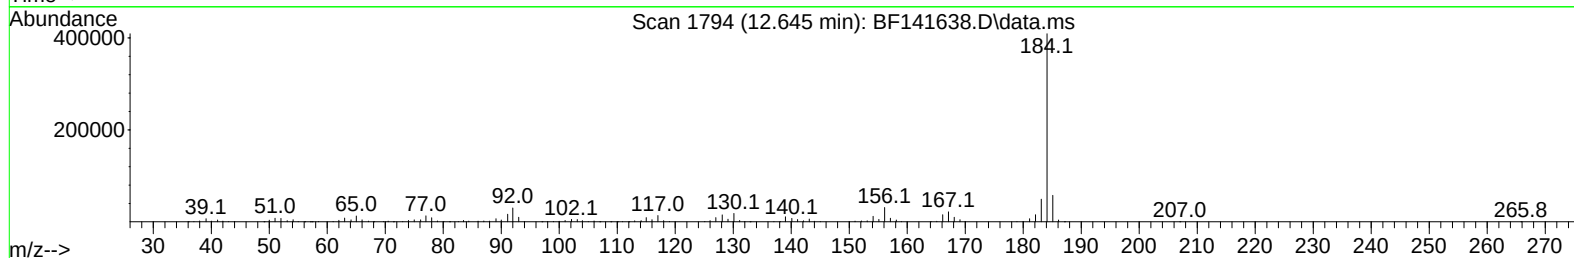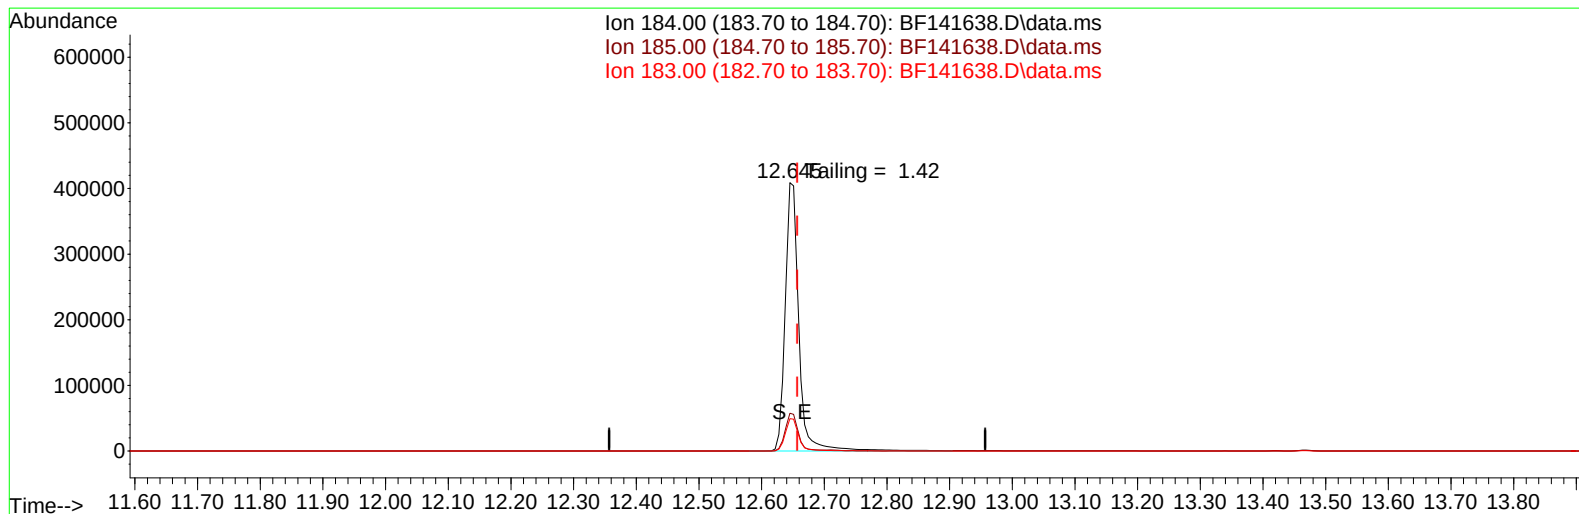

TIC: BF141638.D\data.ms

(77) Benzidine

12.645min (-0.011) 0.00 ng

response 621132

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.06
183.00	11.60	12.06
0.00	0.00	0.00