

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021425\
 Data File : BF141640.D
 Acq On : 14 Feb 2025 15:30
 Operator : RC/JU
 Sample : PB166719BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB166719BL

Quant Time: Feb 14 15:52:53 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 06 16:58:59 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.787	152	87966	20.000	ng	0.00
21) Naphthalene-d8	8.069	136	348866	20.000	ng	0.00
39) Acenaphthene-d10	9.822	164	195731	20.000	ng	-0.01
64) Phenanthrene-d10	11.304	188	353644	20.000	ng	-0.01
76) Chrysene-d12	13.951	240	263315	20.000	ng	-0.01
86) Perylene-d12	15.421	264	191778	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.416	112	762993	135.982	ng	0.00
7) Phenol-d6	6.428	99	946107	133.408	ng	-0.01
23) Nitrobenzene-d5	7.351	82	625105	93.458	ng	-0.01
42) 2,4,6-Tribromophenol	10.610	330	268720	136.669	ng	-0.02
45) 2-Fluorobiphenyl	9.145	172	1209125	95.173	ng	0.00
79) Terphenyl-d14	12.898	244	1516258	97.211	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021425\
Data File : BF141640.D
Acq On : 14 Feb 2025 15:30
Operator : RC/JU
Sample : PB166719BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166719BL


Quant Time: Feb 14 15:52:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

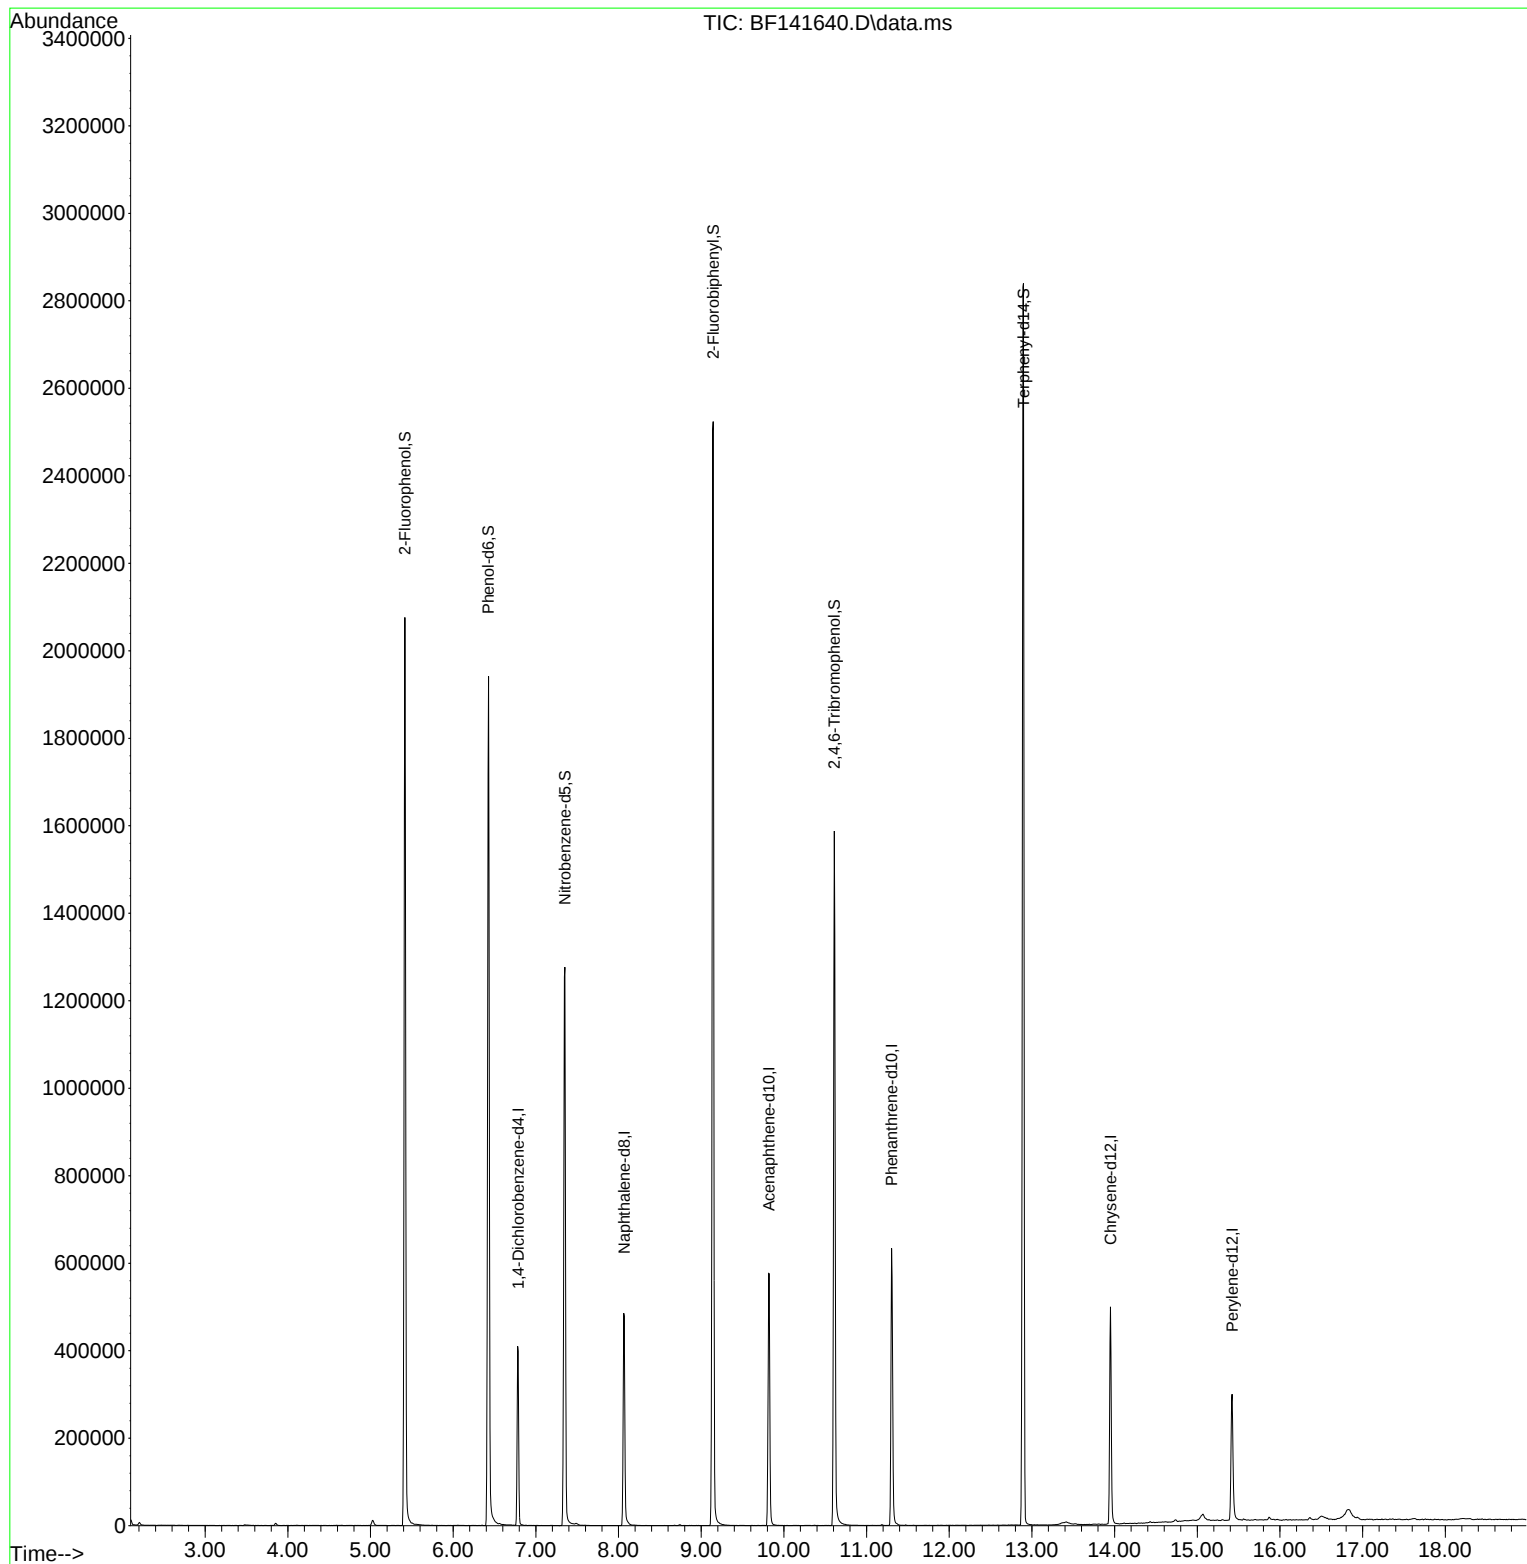






#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.787 min Scan# 798
Delta R.T. -0.005 min
Lab File: BF141640.D
Acq: 14 Feb 2025 15:30

Instrument :
BNA_F
ClientSampleId :
PB166719BL



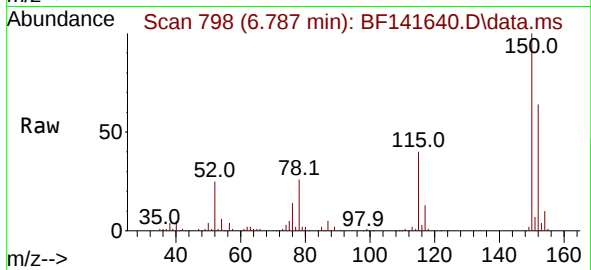



Tgt Ion:152 Resp: 87966
Ion Ratio Lower Upper
152 100
150 155.5 125.0 187.4
115 62.4 53.6 80.4

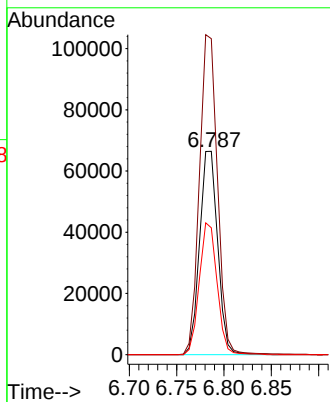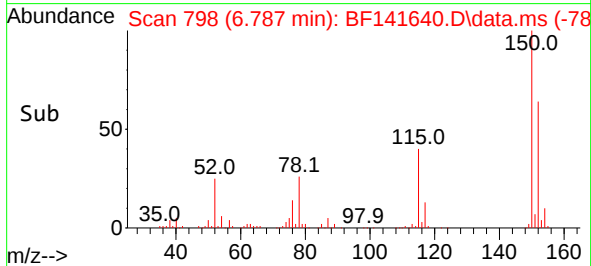

#5
2-Fluorophenol
Concen: 135.982 ng
RT: 5.416 min Scan# 565
Delta R.T. 0.006 min
Lab File: BF141640.D
Acq: 14 Feb 2025 15:30

Tgt Ion:112 Resp: 762993
Ion Ratio Lower Upper
112 100
64 62.6 51.1 76.7
63 34.3 28.4 42.6


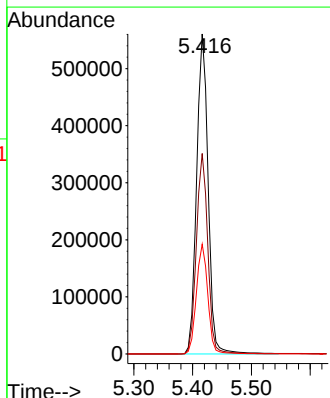

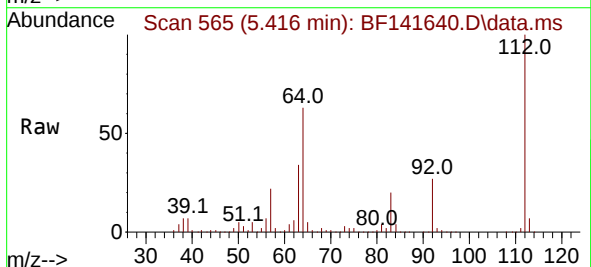


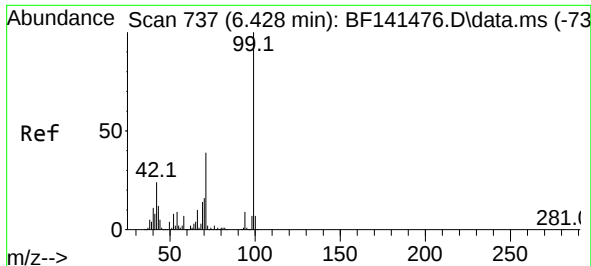

#7
Phenol-d6
Concen: 133.408 ng
RT: 6.428 min Scan# 71
Delta R.T. -0.012 min
Lab File: BF141640.D
Acq: 14 Feb 2025 15:30




Instrument :
BNA_F
ClientSampleId :
PB166719BL


Tgt Ion: 99 Resp: 946107
Ion Ratio Lower Upper
99 100
42 21.4 19.1 28.7
71 37.1 31.1 46.7

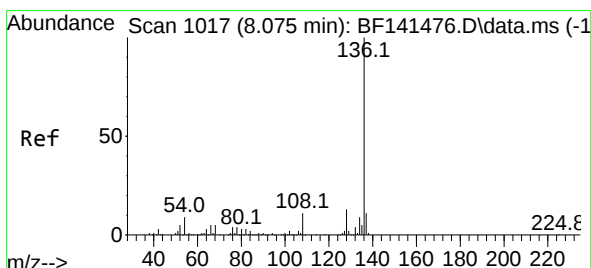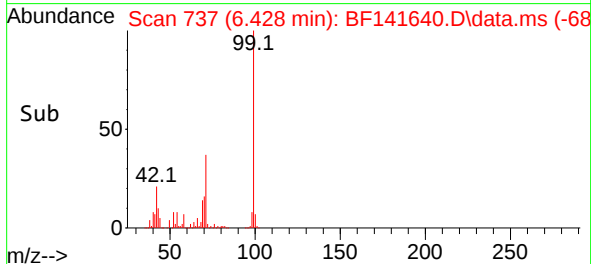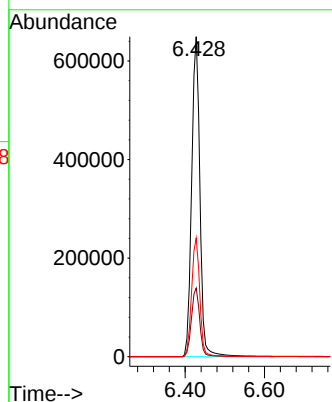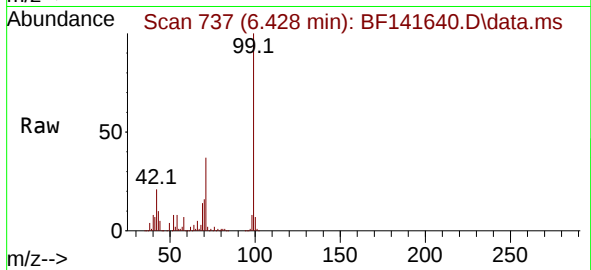

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.069 min Scan# 1016
Delta R.T. -0.006 min
Lab File: BF141640.D
Acq: 14 Feb 2025 15:30

Tgt Ion: 136 Resp: 348866
Ion Ratio Lower Upper
136 100
137 10.7 8.6 13.0
54 8.8 7.2 10.8
68 5.1 3.7 5.5

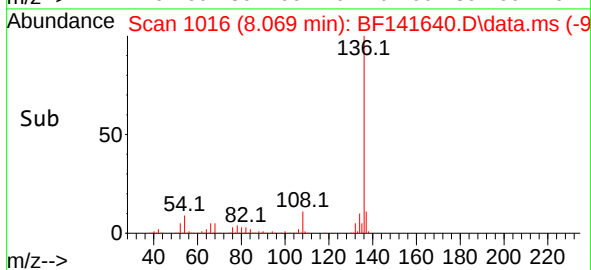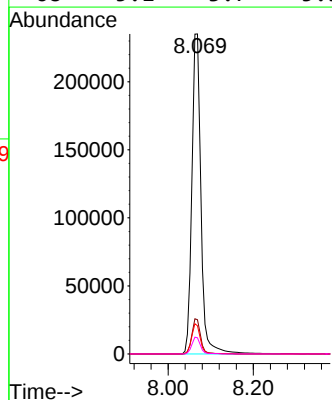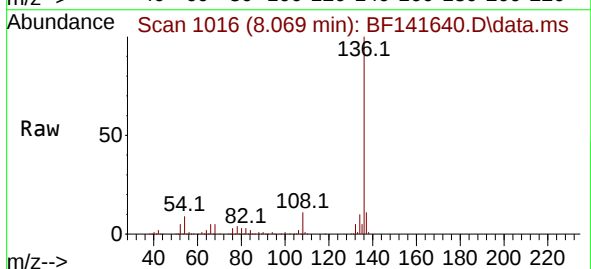

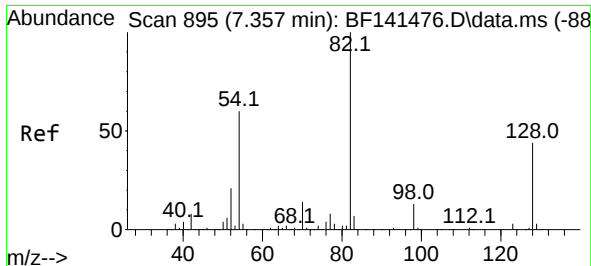

#23

Nitrobenzene-d5

Concen: 93.458 ng

RT: 7.351 min Scan# 894

Delta R.T. -0.012 min

Lab File: BF141640.D

Acq: 14 Feb 2025 15:30

Instrument :

BNA_F

ClientSampleId :

PB166719BL





Tgt Ion: 82 Resp: 625105

Ion Ratio Lower Upper

82 100

128 44.9 34.8 52.2

54 57.4 48.2 72.4

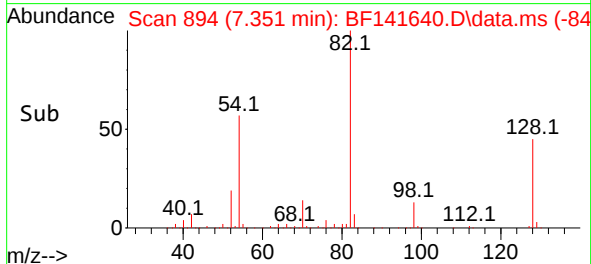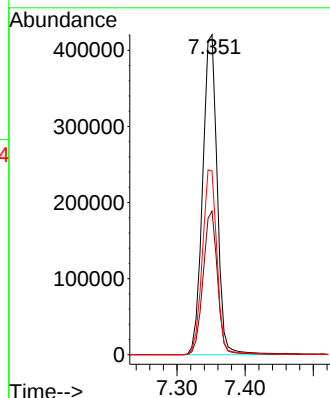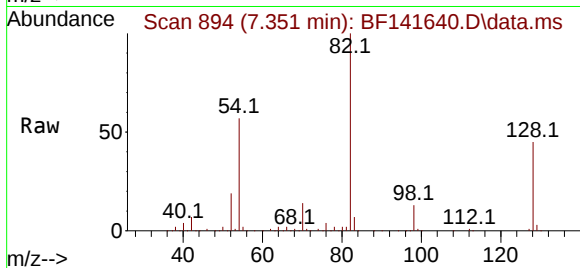

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.822 min Scan# 1314

Delta R.T. -0.012 min

Lab File: BF141640.D

Acq: 14 Feb 2025 15:30




Tgt Ion:164 Resp: 195731


Ion Ratio Lower Upper

164 100

162 99.8 81.3 121.9

160 45.3 35.9 53.9

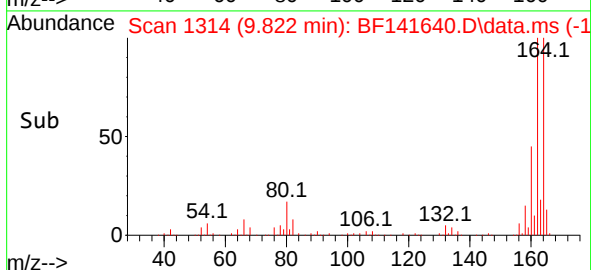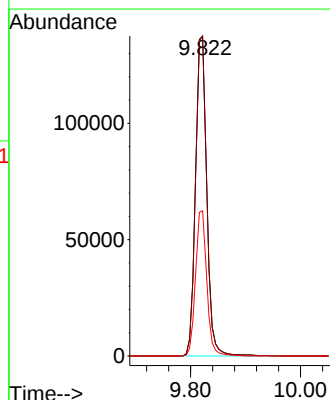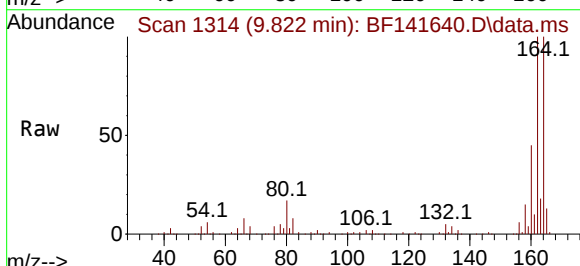

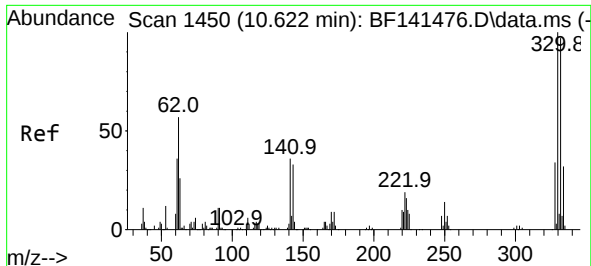

#42

2,4,6-Tribromophenol

Concen: 136.669 ng

RT: 10.610 min Scan# 1448

Delta R.T. -0.017 min

Lab File: BF141640.D

Acq: 14 Feb 2025 15:30

Instrument :

BNA_F

ClientSampleId :

PB166719BL





Tgt Ion:330 Resp: 268720

Ion Ratio Lower Upper

330 100

332 97.5 78.5 117.7

141 35.9 31.0 46.4

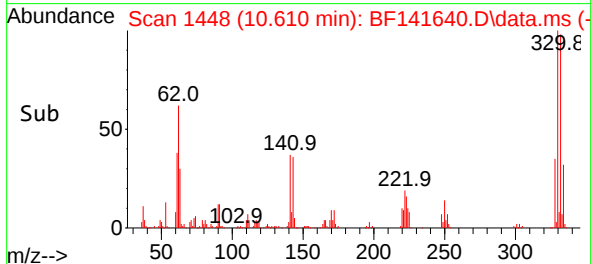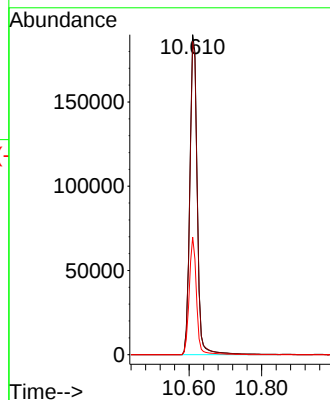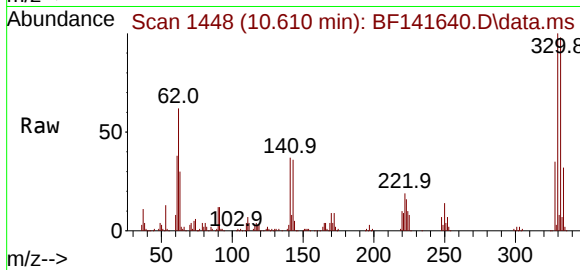

#45

2-Fluorobiphenyl

Concen: 95.173 ng

RT: 9.145 min Scan# 1199

Delta R.T. -0.006 min

Lab File: BF141640.D

Acq: 14 Feb 2025 15:30




Tgt Ion:172 Resp: 1209125


Ion Ratio Lower Upper

172 100

171 35.4 28.7 43.1

170 23.5 18.9 28.3


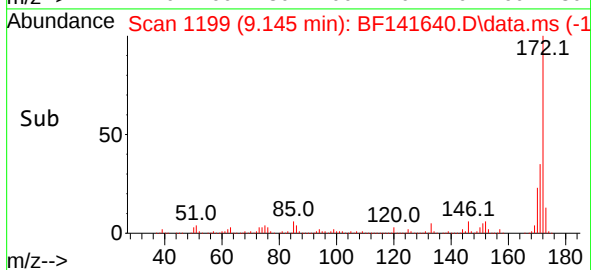
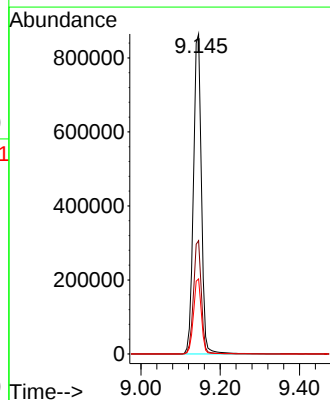
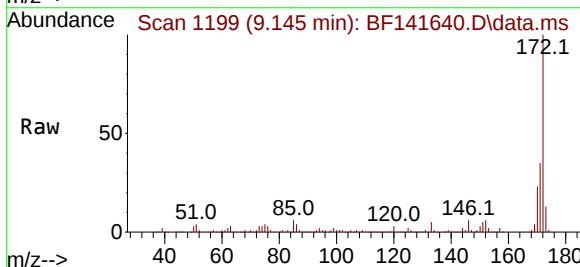




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.304 min Scan# 1
Delta R.T. -0.012 min
Lab File: BF141640.D
Acq: 14 Feb 2025 15:30




Instrument :
BNA_F
ClientSampleId :
PB166719BL


Tgt Ion:188 Resp: 353644
Ion Ratio Lower Upper
188 100
94 8.8 6.6 10.0
80 9.9 7.3 10.9

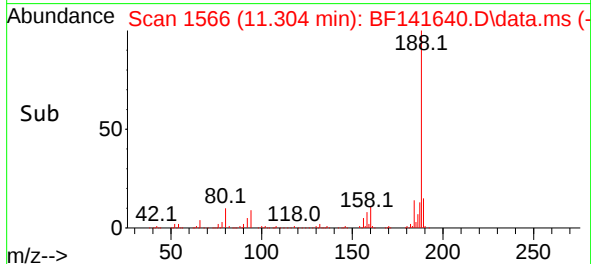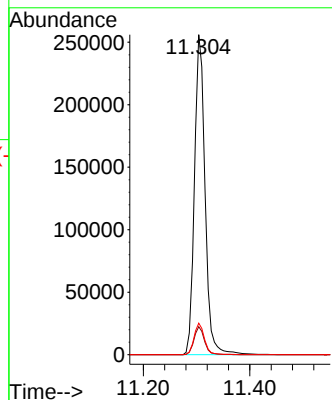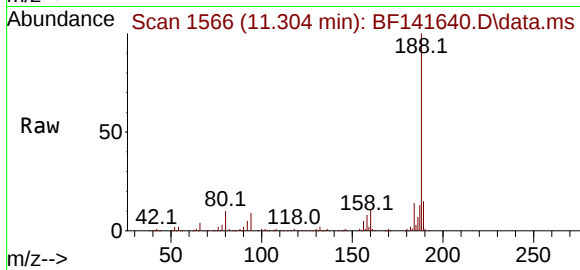

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.951 min Scan# 2016
Delta R.T. -0.012 min
Lab File: BF141640.D
Acq: 14 Feb 2025 15:30


Tgt Ion:240 Resp: 263315
Ion Ratio Lower Upper
240 100
120 9.6 8.0 12.0
236 25.9 19.8 29.8

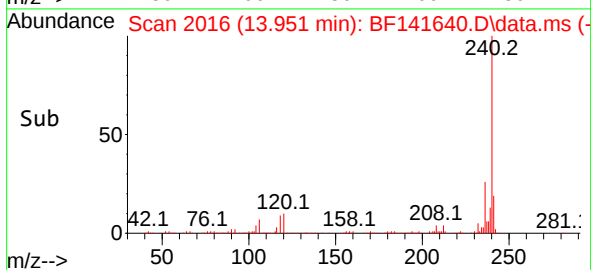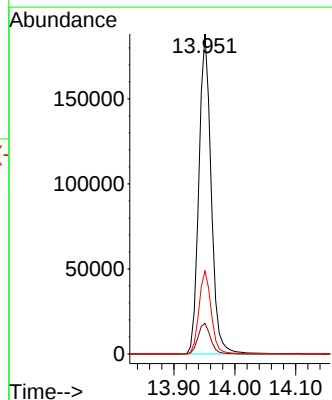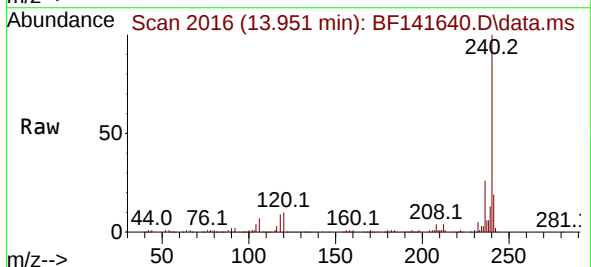



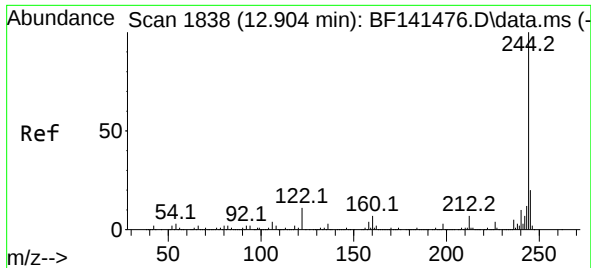


#79
Terphenyl-d14
Concen: 97.211 ng
RT: 12.898 min Scan# 1837
Delta R.T. -0.006 min
Lab File: BF141640.D
Acq: 14 Feb 2025 15:30

Instrument :
BNA_F
ClientSampleId :
PB166719BL

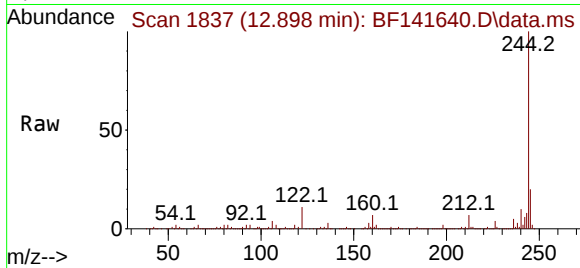

Tgt Ion:244 Resp: 1516258
Ion Ratio Lower Upper
244 100
212 6.8 5.6 8.4
122 10.5 8.4 12.6

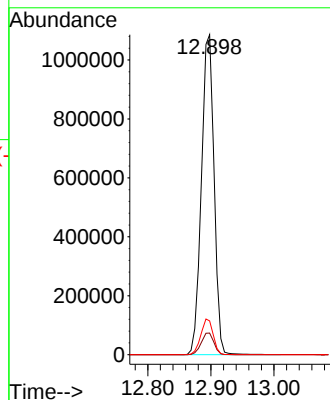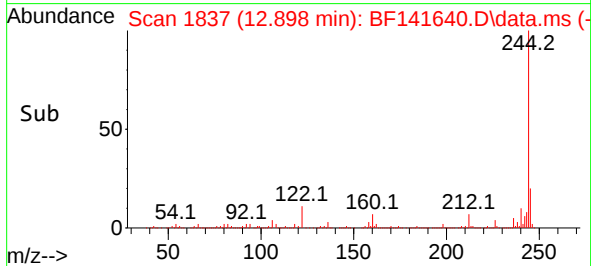

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.421 min Scan# 2266
Delta R.T. 0.006 min
Lab File: BF141640.D
Acq: 14 Feb 2025 15:30

Tgt Ion:264 Resp: 191778
Ion Ratio Lower Upper
264 100
260 23.1 18.6 28.0
265 21.6 17.0 25.4

