

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021425\
 Data File : BF141640.D
 Acq On : 14 Feb 2025 15:30
 Operator : RC/JU
 Sample : PB166719BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB166719BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141640.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.416	559	565	579	rBV	2075707	2798448	70.21%	13.113%
2	6.428	731	737	757	rBV	1940962	2827161	70.93%	13.248%
3	6.781	793	797	810	rVB	409031	533020	13.37%	2.498%
4	7.351	887	894	913	rBV	1276677	1903533	47.76%	8.920%
5	8.063	1010	1015	1036	rBV	485350	705383	17.70%	3.305%
6	9.145	1192	1199	1219	rBV	2523468	3527489	88.50%	16.530%
7	9.816	1308	1313	1325	rBV	576106	812844	20.39%	3.809%
8	10.610	1442	1448	1469	rBV	1587280	2189254	54.93%	10.259%
9	11.304	1561	1566	1585	rBV	633103	867442	21.76%	4.065%
10	12.898	1830	1837	1842	rBV	2838434	3985779	100.00%	18.677%
11	13.951	2010	2016	2035	rVB	496249	687987	17.26%	3.224%
12	15.421	2259	2266	2280	rBV	287819	502026	12.60%	2.352%




Sum of corrected areas: 21340366

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021425\
Data File : BF141640.D
Acq On : 14 Feb 2025 15:30
Operator : RC/JU
Sample : PB166719BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166719BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

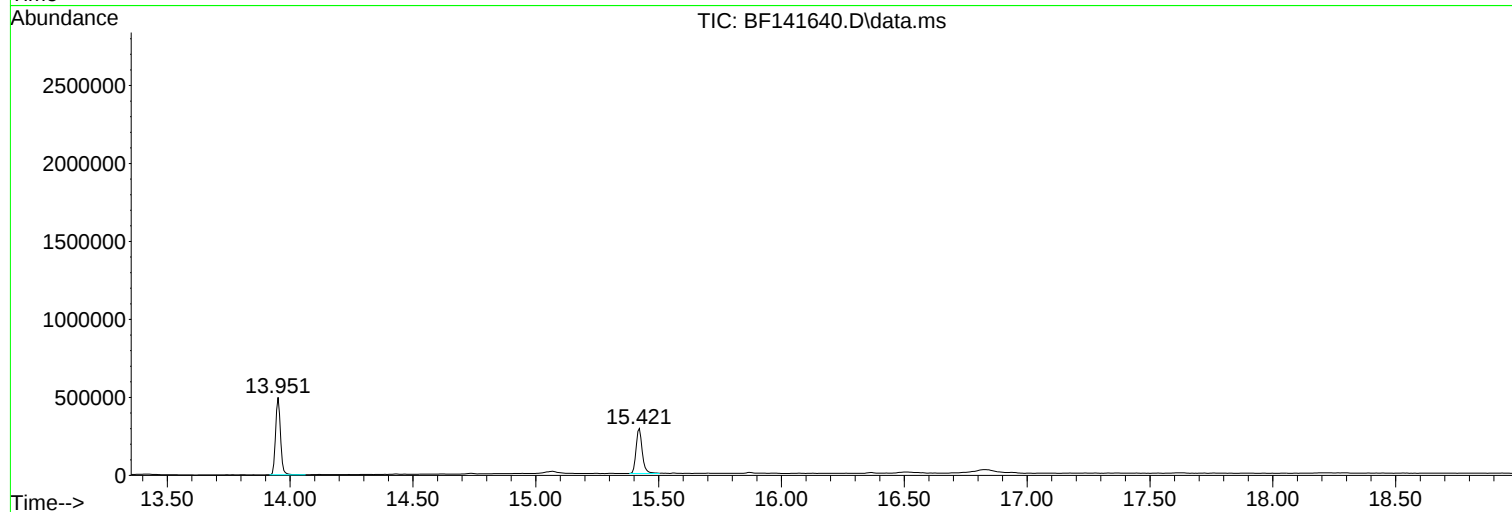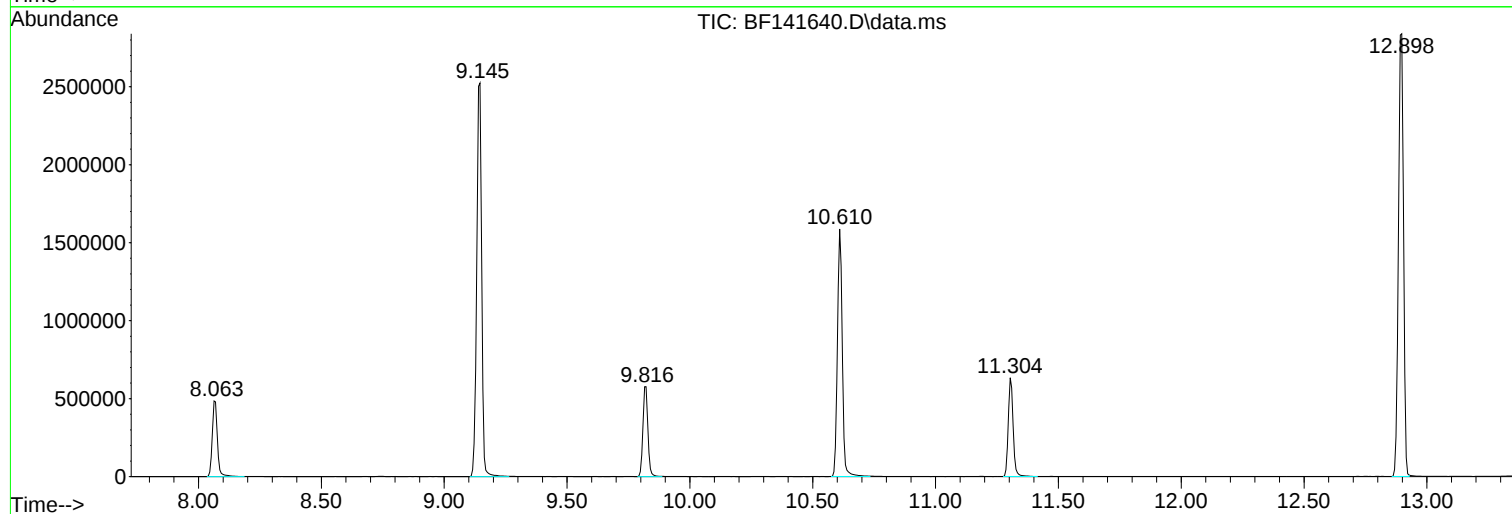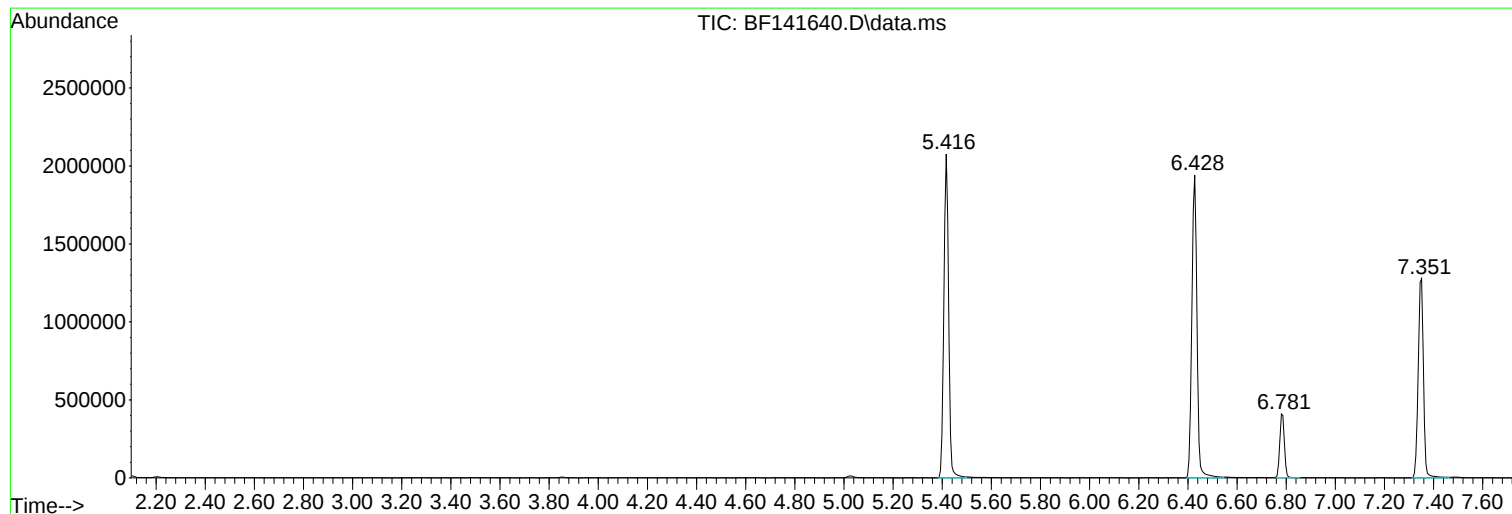

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021425\
Data File : BF141640.D
Acq On : 14 Feb 2025 15:30
Operator : RC/JU
Sample : PB166719BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166719BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021425\
Data File : BF141640.D
Acq On : 14 Feb 2025 15:30
Operator : RC/JU
Sample : PB166719BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166719BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------