
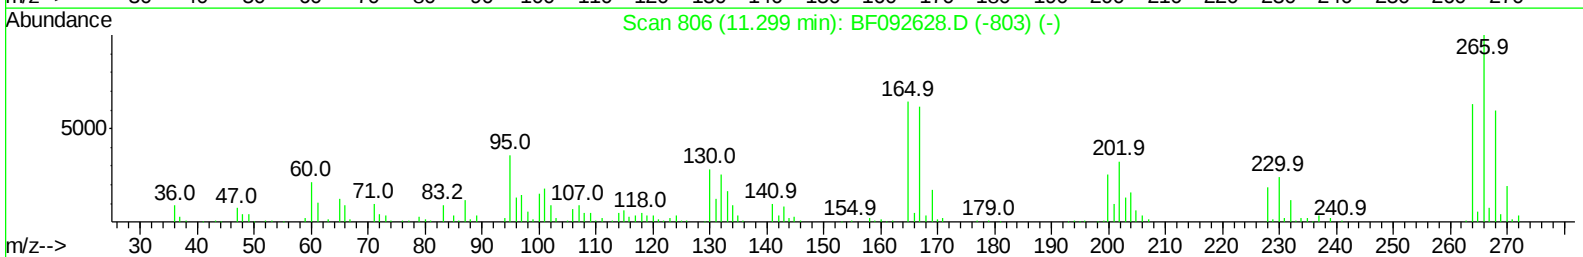
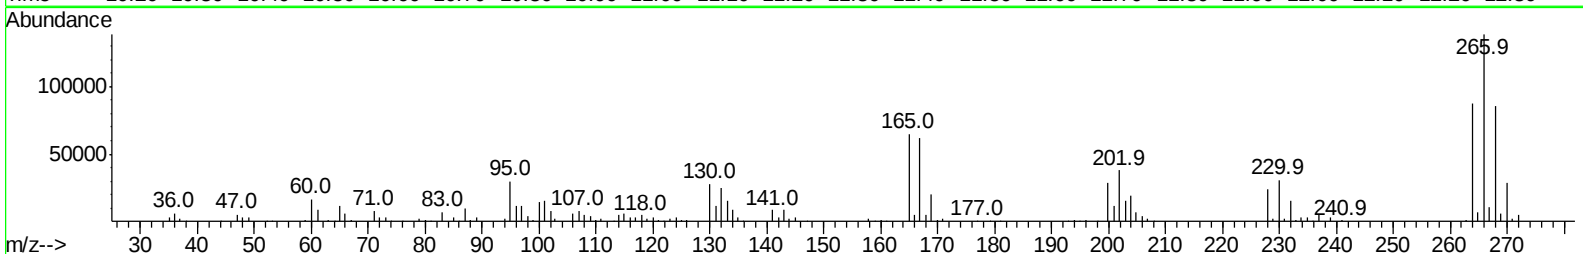


Data Path : Z:\HPCHEM1\BNA F\Data\BF021517\
Data File : BF092975.D
Acq On : 16 Feb 2017 4:10
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 16 11:46:54 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 13 18:04:38 2017
Response via : Initial Calibration

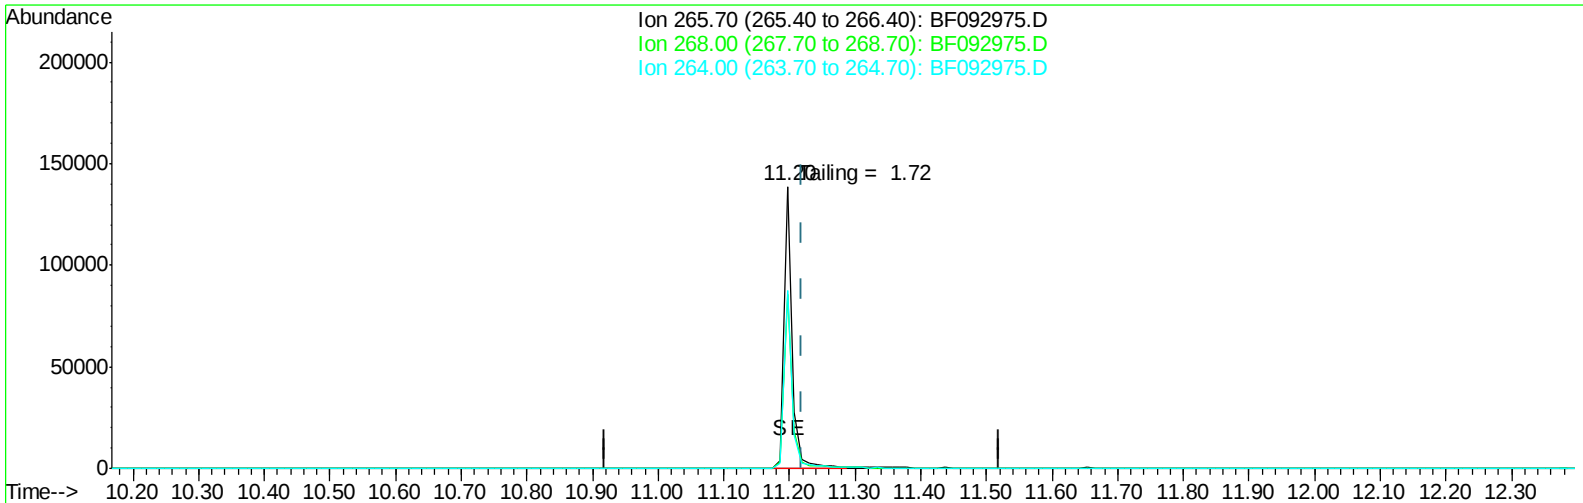

TIC: BF092975.D

(69) Pentachlorophenol (C)




11.196min (-0.023) 0.00ng

response 128578

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	61.61
264.00	62.90	63.27
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF021517\
Data File : BF092975.D
Acq On : 16 Feb 2017 4:10
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 16 11:46:54 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 13 18:04:38 2017
Response via : Initial Calibration

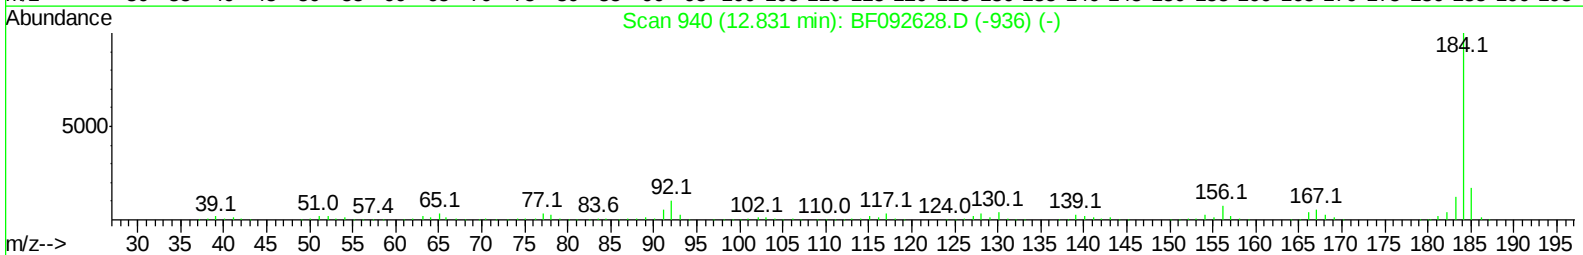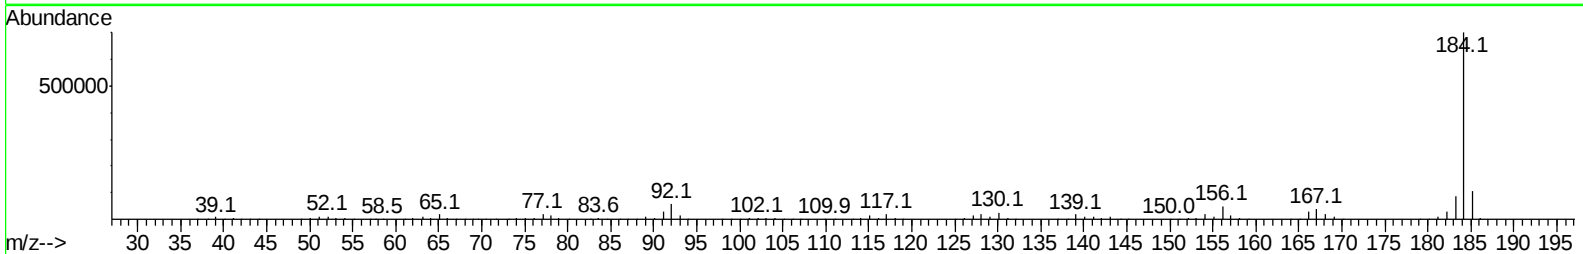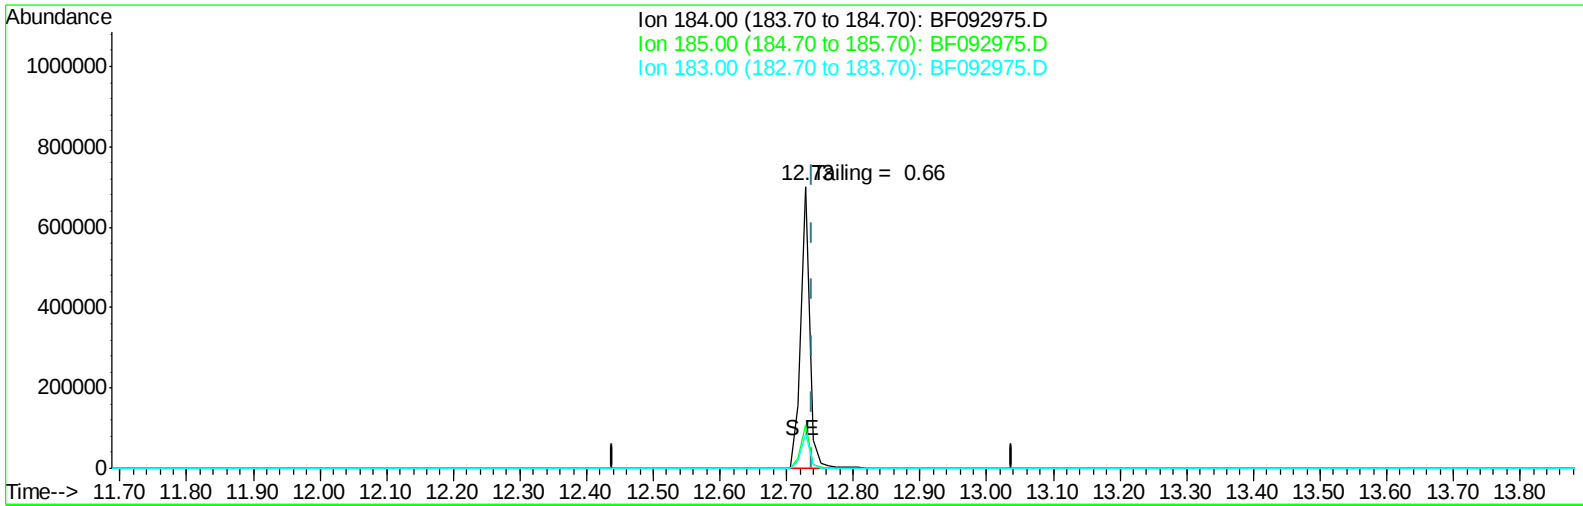

TIC: BF092975.D

(76) Benzidine

12.728min (-0.011) 61138.08ng

response 661736

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	15.27
183.00	11.50	12.19
0.00	0.00	0.00